

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112320\
Data File : FE033169.D
Signal(s) : FID1B.CH
Acq On : 23 Nov 2020 17:17
Operator : DD\AJ
Sample : L4868-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
KENS-B3-112020-0-2

Integration File: autoint1.e
Quant Time: Nov 24 00:11:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.613	4130406	13.079 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112320\
Data File : FE033169.D
Signal(s) : FID1B.CH
Acq On : 23 Nov 2020 17:17
Operator : DD\AJ
Sample : L4868-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
KENS-B3-112020-0-2

Integration File: autoint1.e
Quant Time: Nov 24 00:11:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

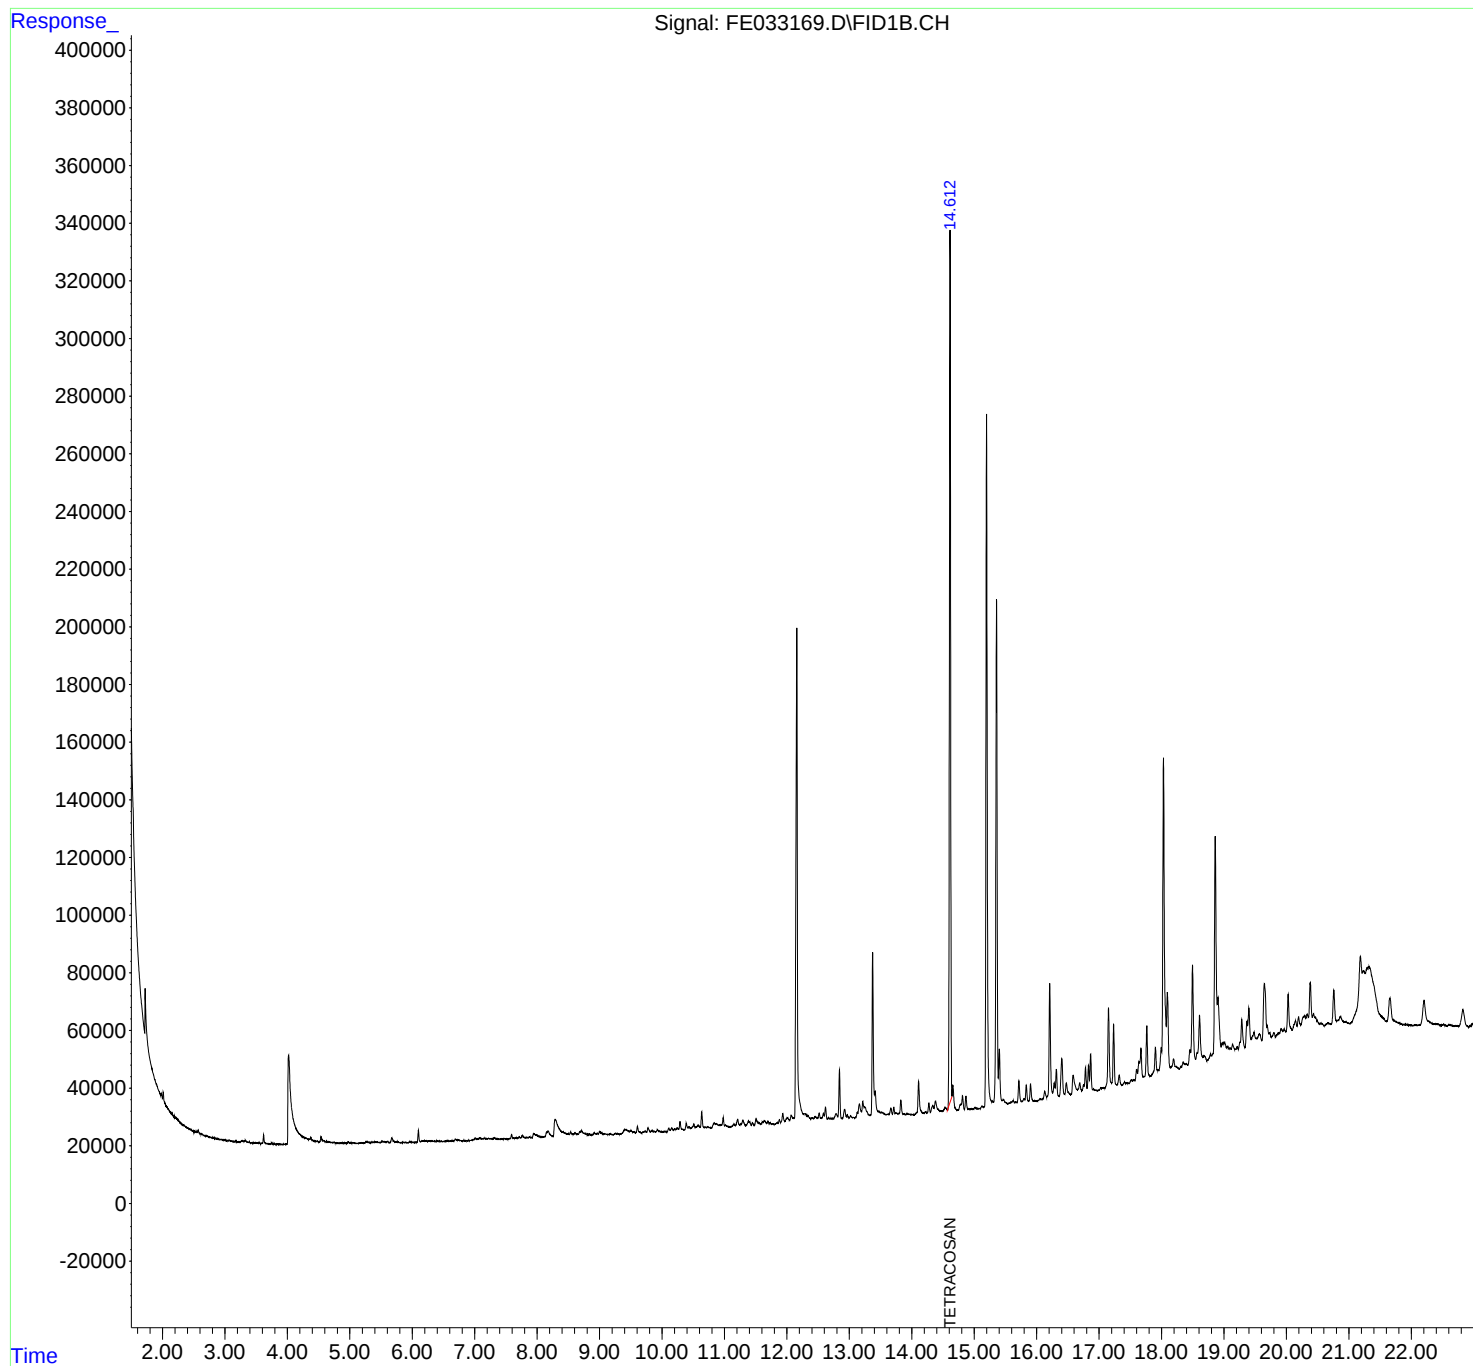

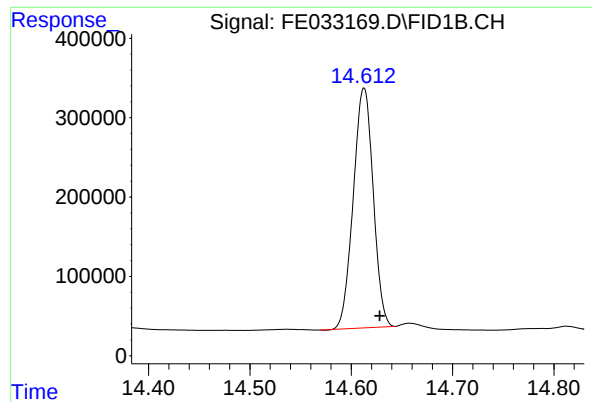

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.613 min
Delta R.T.: -0.015 min
Response: 4130406
Conc: 13.08 ug/ml

Instrument :
FID_E
ClientSampleId :
KENS-B3-112020-0-2