

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112823AL\
 Data File : FE045548.D
 Signal(s) : FID1B.ch
 Acq On : 28 Nov 2023 08:50
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 28 23:05:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 110423.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 05:16:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.467	306443	1.993 ug/ml
13) T n-Docosane (C22)	14.061	277221	1.830 ug/ml
14) T n-Tetracosane (C24)	15.172	222231	1.500 ug/ml
15) T n-Hexacosane (C26)	16.196	157042	1.077 ug/ml
16) T n-Octacosane (C28)	17.149	126797	0.868 ug/ml
17) T n-Tricontane (C30)	18.035	170422	1.122 ug/ml
18) T n-Dotriacontane (C32)	18.876	273974	1.754 ug/ml
19) T n-Tetratriacontane (C34)	19.658	129609	0.830 ug/ml
20) T n-Hexatriacontane (C36)	20.400	293153	1.806 ug/ml
21) T n-Octatriacontane (C38)	21.135	384062	2.312 ug/ml
22) T n-Tetracontane (C40)	22.042	560747	3.283 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112823AL\
Data File : FE045548.D
Signal(s) : FID1B.ch
Acq On : 28 Nov 2023 08:50
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 28 23:05:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 110423.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 05:16:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

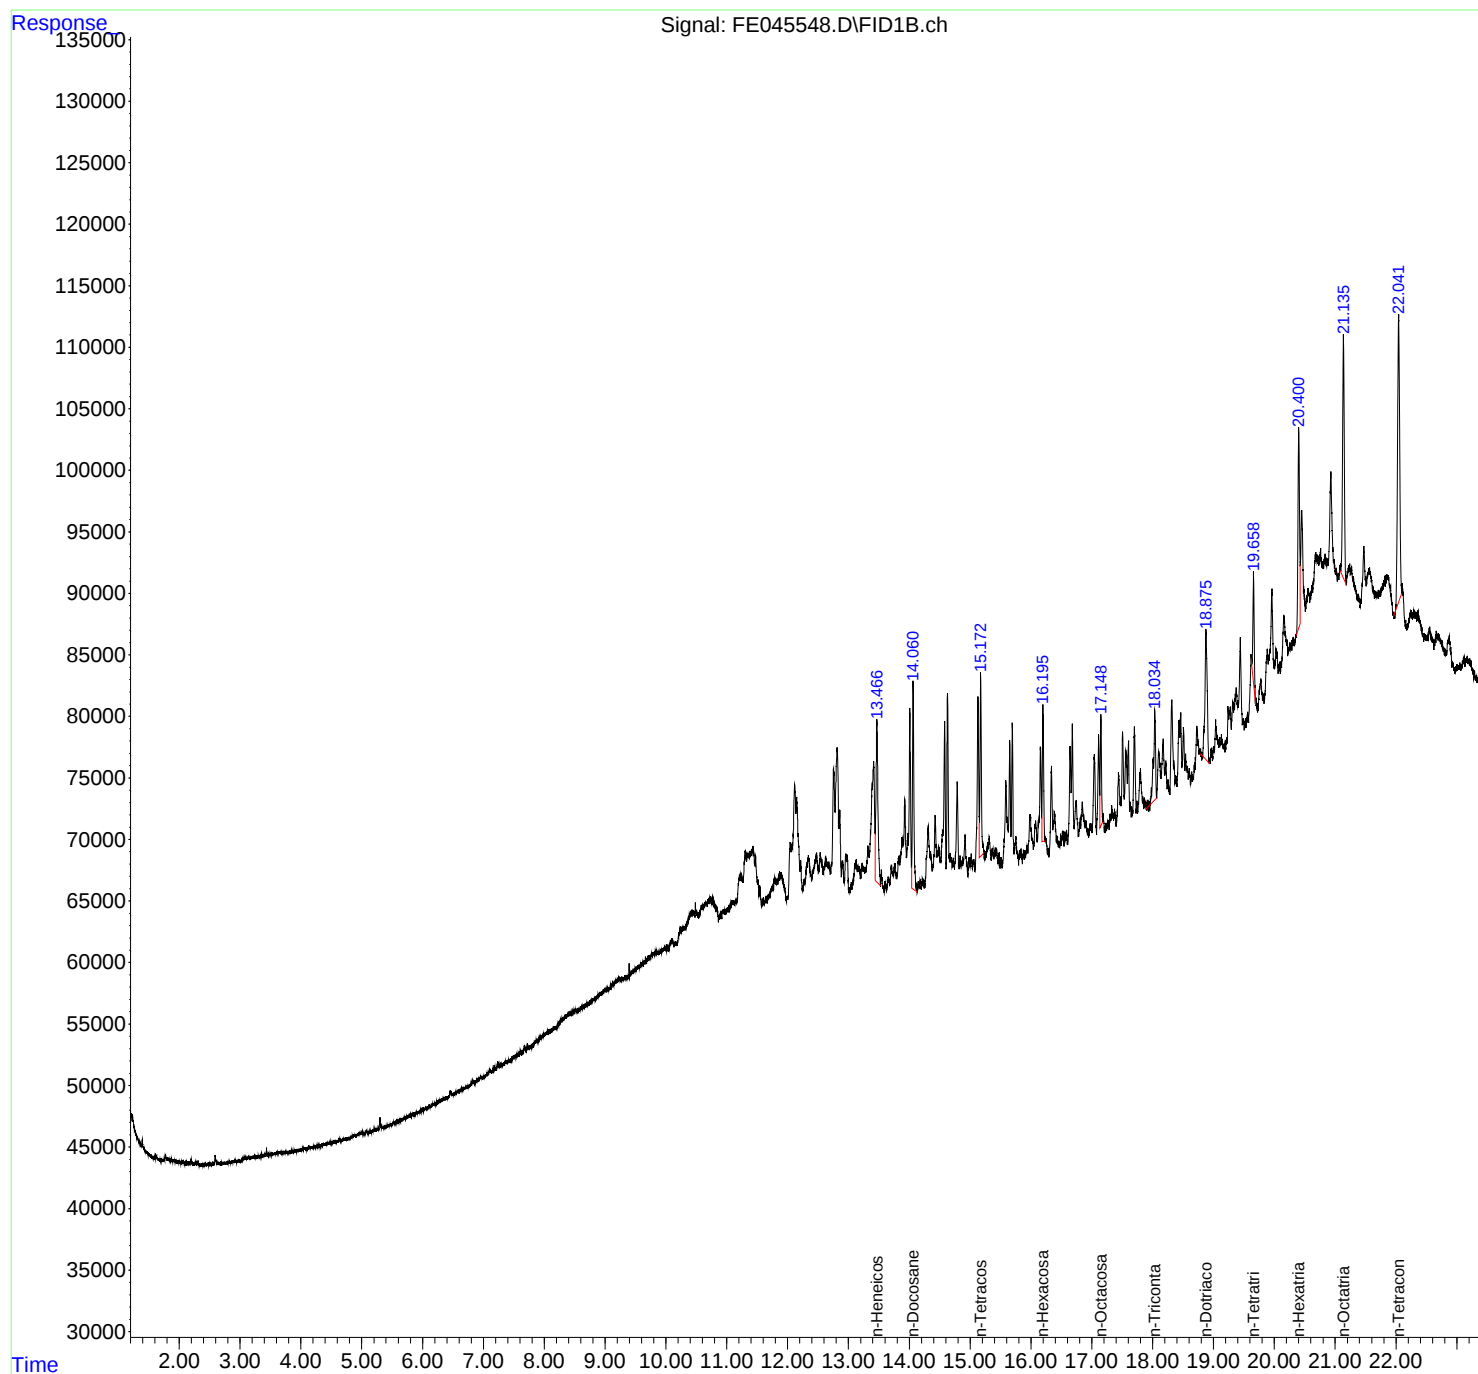


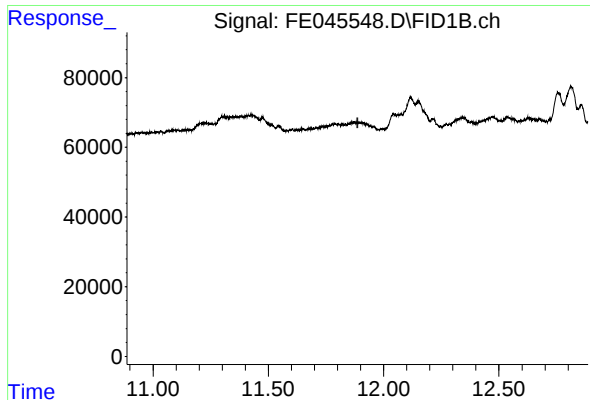

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.887 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

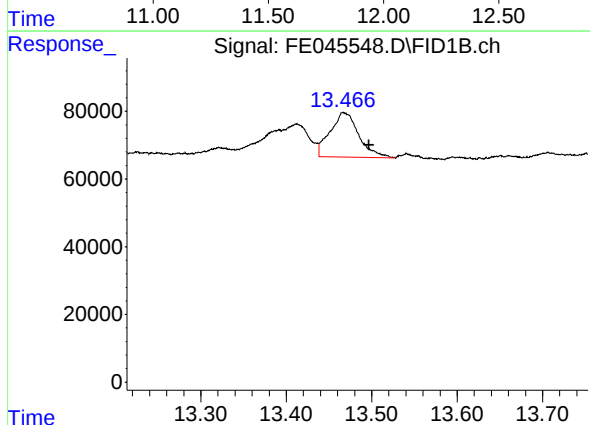


#11 n-Heneicosane (C21)

R.T.: 13.467 min
Delta R.T.: -0.030 min
Response: 306443
Conc: 1.99 ug/ml

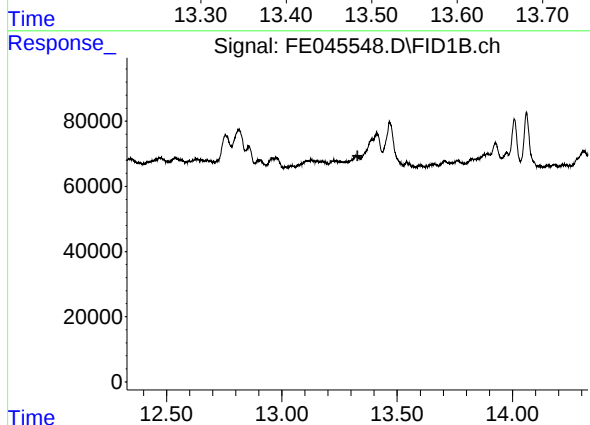


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.328 min
Response: 0
Conc: N.D.

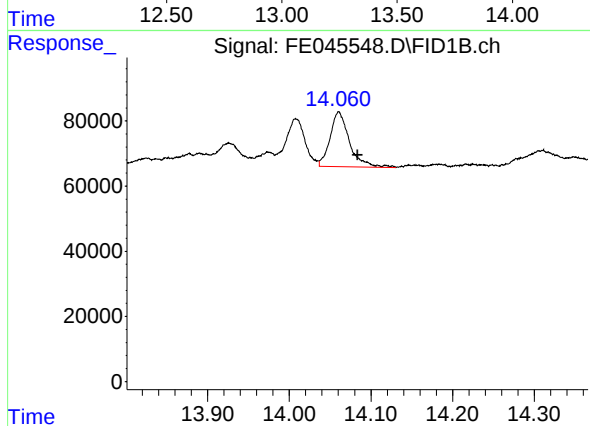

#13 n-Docosane (C22)


R.T.: 14.061 min
Delta R.T.: -0.023 min
Response: 277221
Conc: 1.83 ug/ml

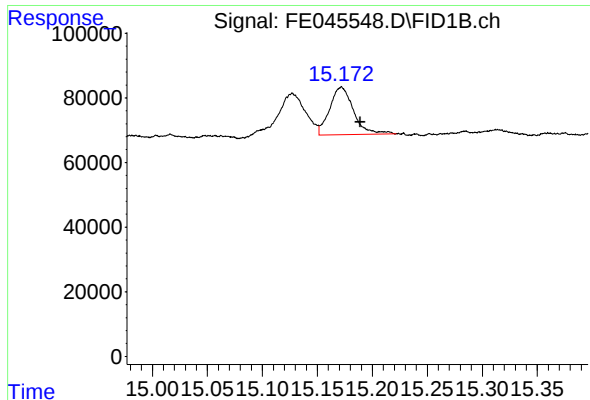

#14 n-Tetracosane (C24)


R.T.: 15.172 min
Delta R.T.: -0.017 min
Response: 222231
Conc: 1.50 ug/ml

Instrument :
FID_E
ClientSampleId :

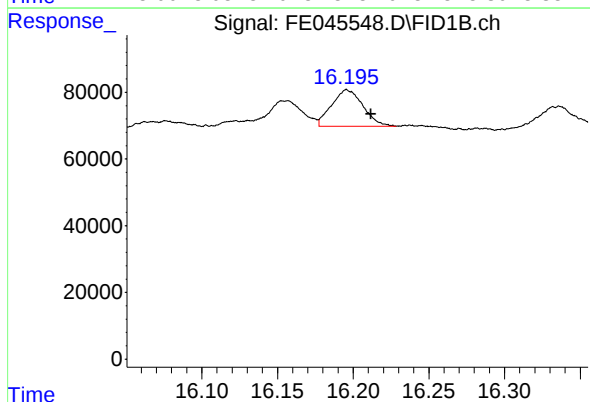


#15 n-Hexacosane (C26)

R.T.: 16.196 min
Delta R.T.: -0.016 min
Response: 157042
Conc: 1.08 ug/ml

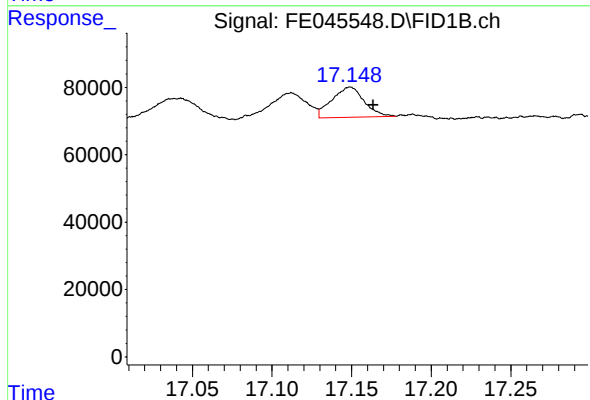


#16 n-Octacosane (C28)

R.T.: 17.149 min
Delta R.T.: -0.015 min
Response: 126797
Conc: 0.87 ug/ml

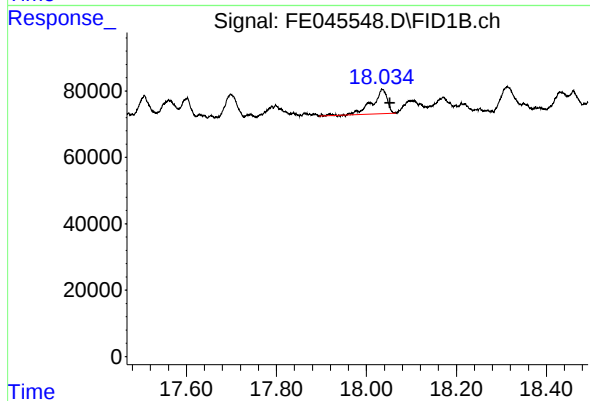

#17 n-Tricontane (C30)


R.T.: 18.035 min
Delta R.T.: -0.017 min
Response: 170422
Conc: 1.12 ug/ml

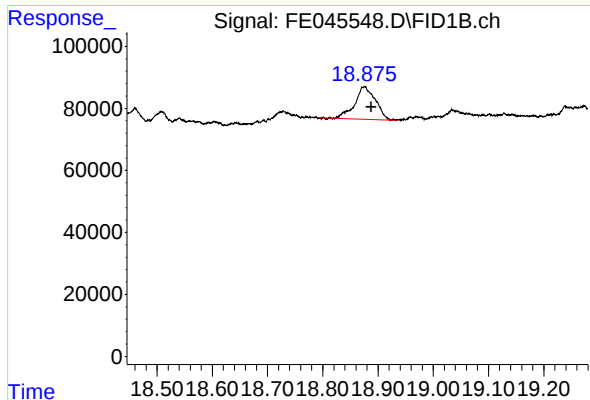

#18 n-Dotriacontane (C32)


R.T.: 18.876 min
Delta R.T.: -0.011 min
Response: 273974
Conc: 1.75 ug/ml

Instrument :
FID_E
ClientSampleId :

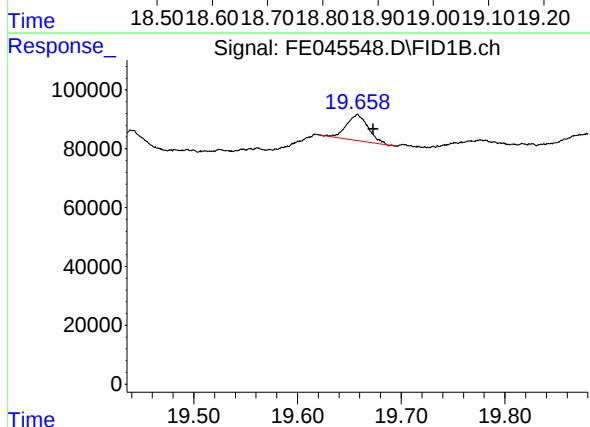


#19 n-Tetratriacontane (C34)

R.T.: 19.658 min
Delta R.T.: -0.015 min
Response: 129609
Conc: 0.83 ug/ml

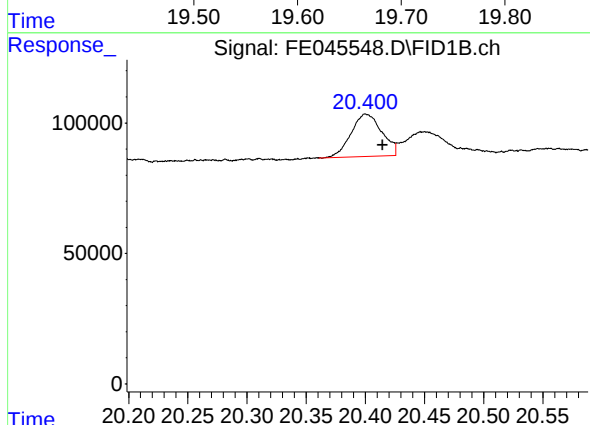


#20 n-Hexatriacontane (C36)

R.T.: 20.400 min
Delta R.T.: -0.014 min
Response: 293153
Conc: 1.81 ug/ml

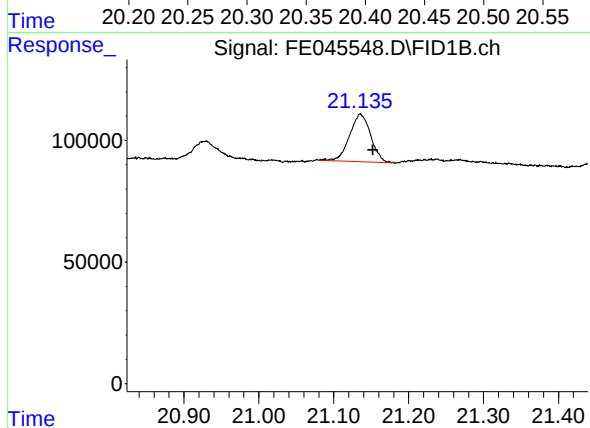

#21 n-Octatriacontane (C38)

R.T.: 21.135 min
Delta R.T.: -0.017 min
Response: 384062
Conc: 2.31 ug/ml

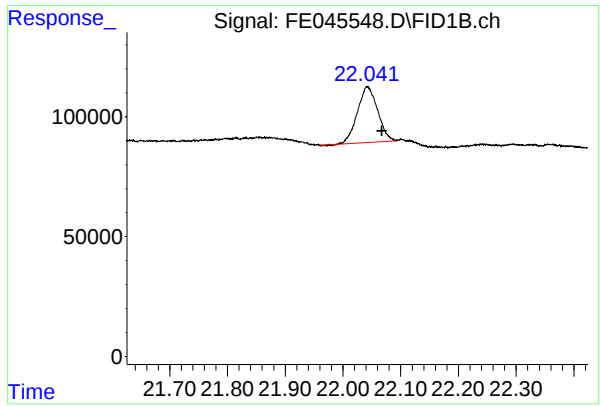

#22 n-Tetracontane (C40)

R.T.: 22.042 min
Delta R.T.: -0.026 min
Response: 560747
Conc: 3.28 ug/ml

Instrument :
FID_E
ClientSampleId :