

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112922AL\
 Data File : FE038995.D
 Signal(s) : FID1B.ch
 Acq On : 29 Nov 2022 09:01
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 30 03:04:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.876f	553969	3.902 ug/ml
11) T	n-Heneicosane (C21)	13.531	125906	0.886 ug/ml
13) T	n-Docosane (C22)	14.130	311171	2.226 ug/ml
14) T	n-Tetracosane (C24)	15.237	210248	1.522 ug/ml
15) T	n-Hexacosane (C26)	16.259	190150	1.416 ug/ml
16) T	n-Octacosane (C28)	17.211	138578	1.044 ug/ml
17) T	n-Tricontane (C30)	18.098	105611	0.800 ug/ml
18) T	n-Dotriacontane (C32)	18.929	187185	1.404 ug/ml
20) T	n-Hexatriacontane (C36)	20.459	42834	0.333 ug/ml
22) T	n-Tetracontane (C40)	22.106	14942	0.110 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112922AL\
Data File : FE038995.D
Signal(s) : FID1B.ch
Acq On : 29 Nov 2022 09:01
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 30 03:04:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

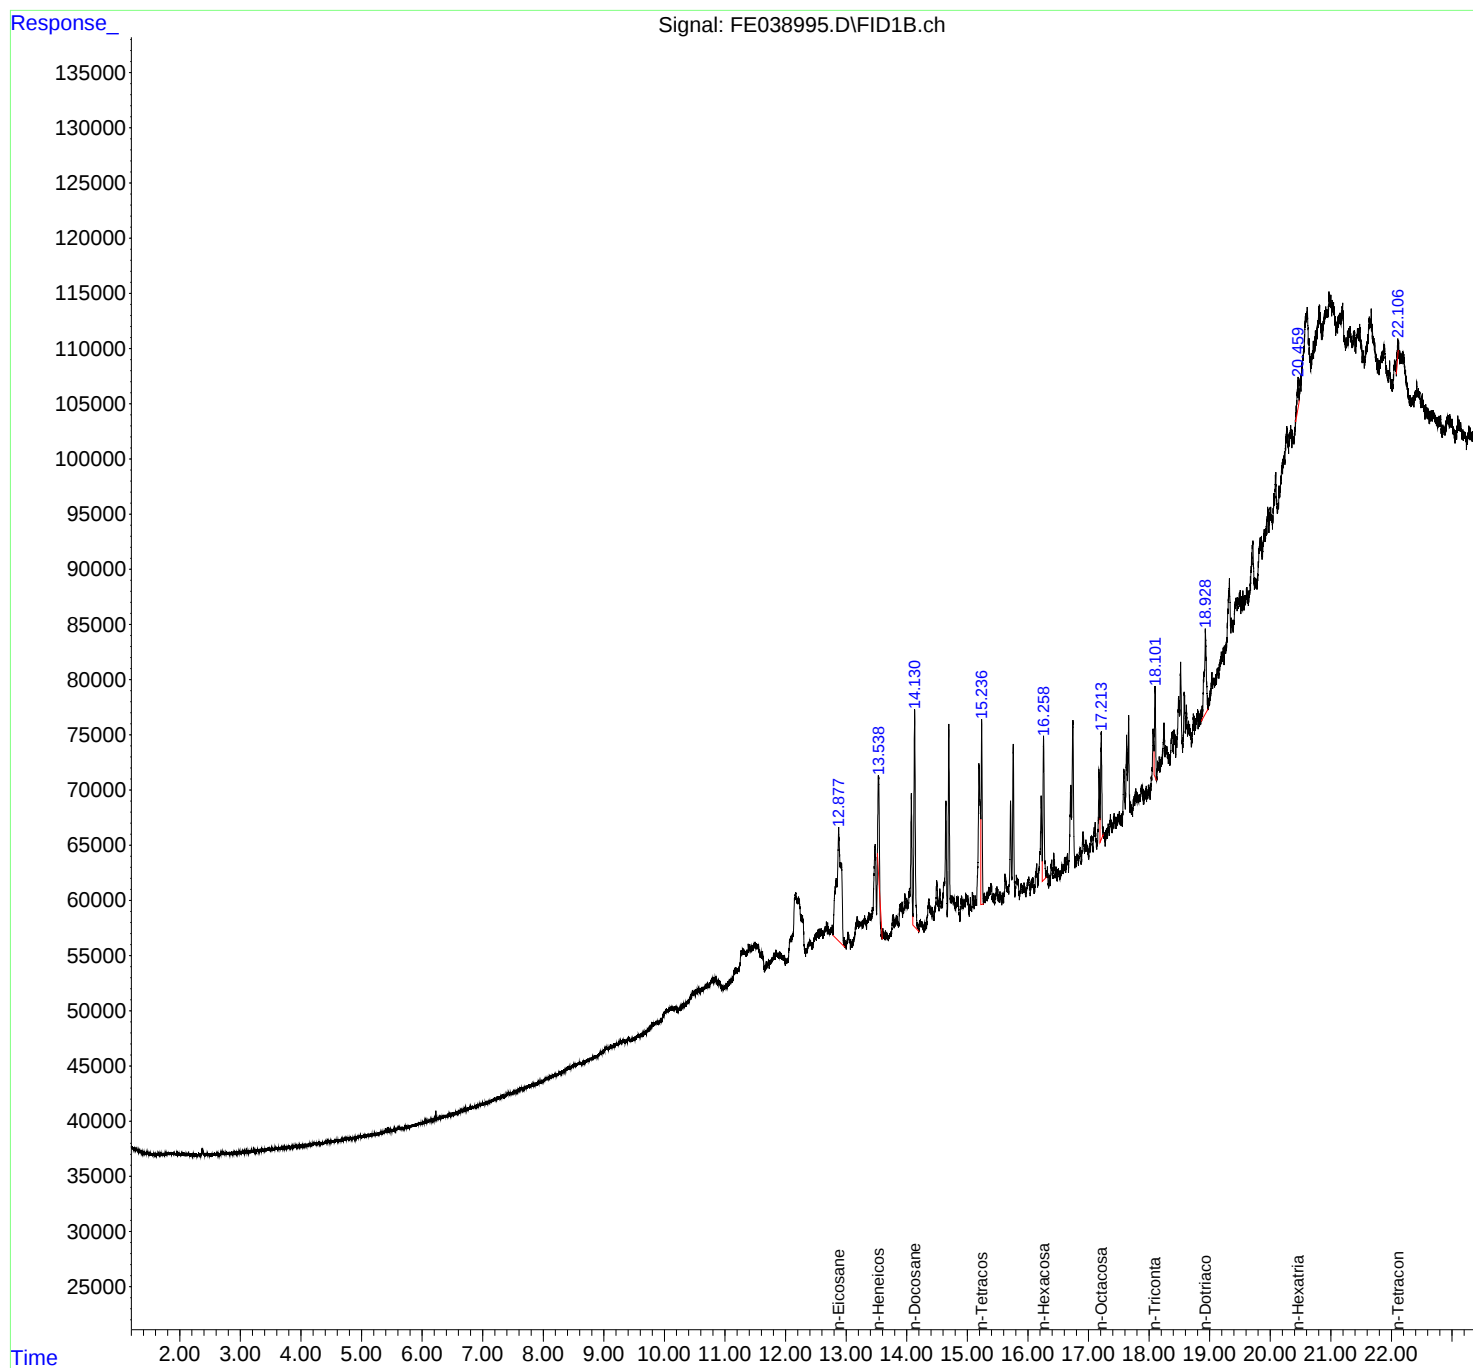


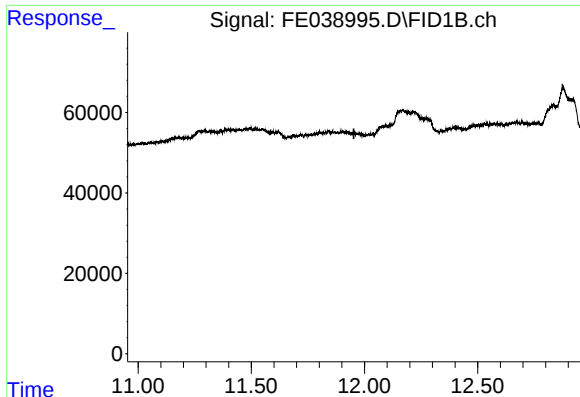

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.953 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

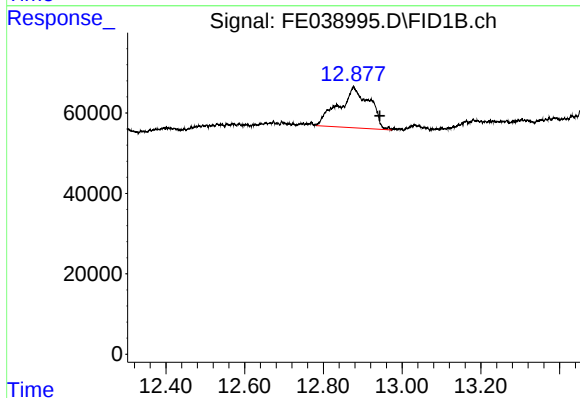


#10 n-Eicosane (C20)

R.T.: 12.876 min
Delta R.T.: -0.066 min
Response: 553969
Conc: 3.90 ug/ml

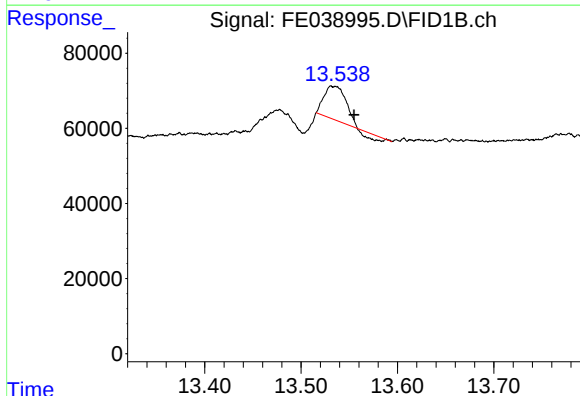


#11 n-Heneicosane (C21)

R.T.: 13.531 min
Delta R.T.: -0.023 min
Response: 125906
Conc: 0.89 ug/ml

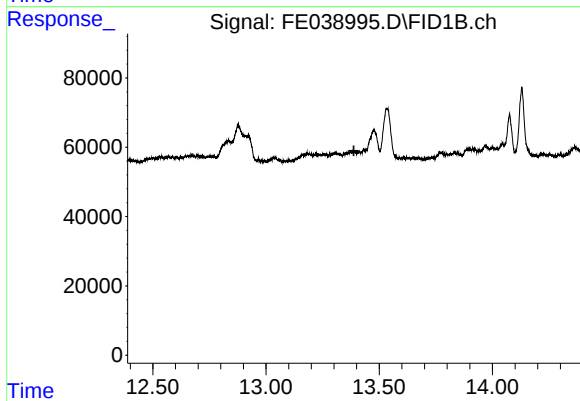

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.388 min
Response: 0
Conc: N.D.

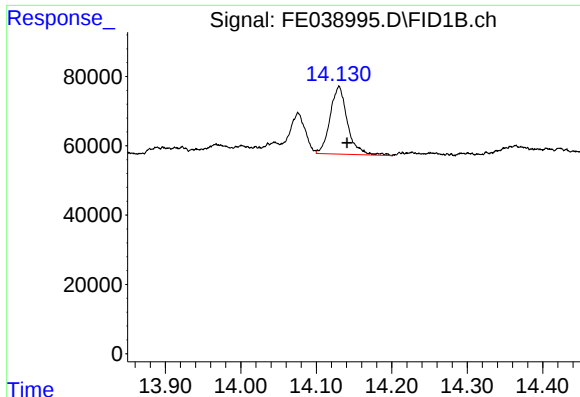

#13 n-Docosane (C22)


R.T.: 14.130 min
Delta R.T.: -0.011 min
Response: 311171
Conc: 2.23 ug/ml

Instrument :
FID_E
ClientSampleId :

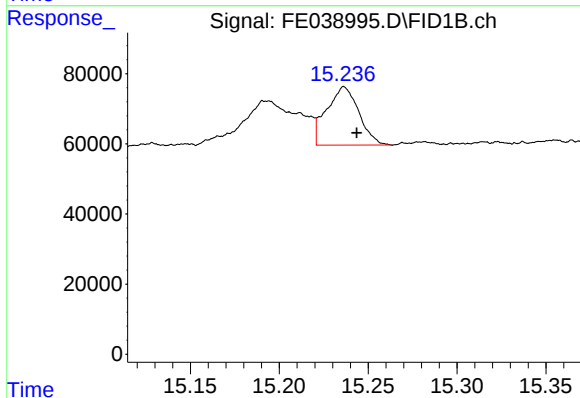


#14 n-Tetracosane (C24)

R.T.: 15.237 min
Delta R.T.: -0.007 min
Response: 210248
Conc: 1.52 ug/ml

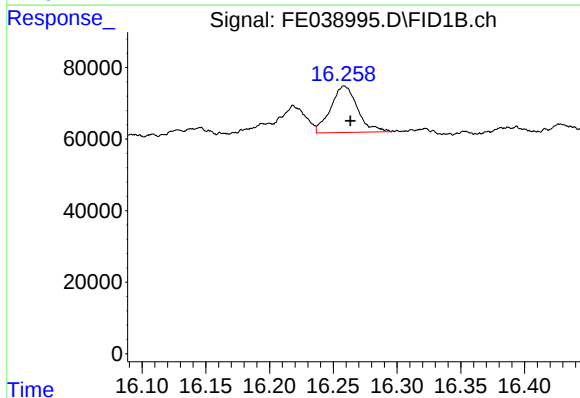


#15 n-Hexacosane (C26)

R.T.: 16.259 min
Delta R.T.: -0.005 min
Response: 190150
Conc: 1.42 ug/ml

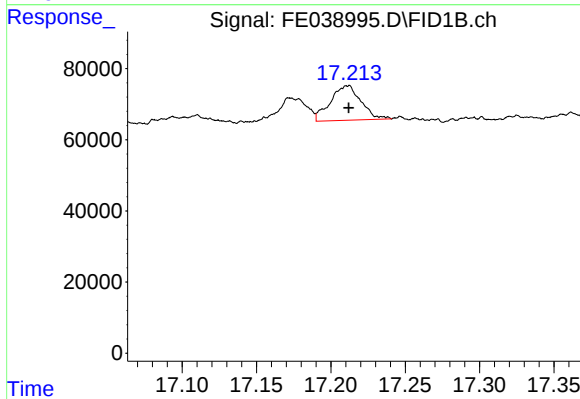

#16 n-Octacosane (C28)


R.T.: 17.211 min
Delta R.T.: 0.000 min
Response: 138578
Conc: 1.04 ug/ml

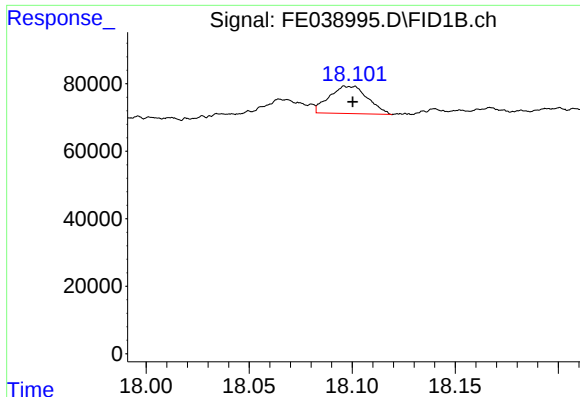

#17 n-Tricontane (C30)


R.T.: 18.098 min
Delta R.T.: -0.003 min
Response: 105611
Conc: 0.80 ug/ml

Instrument :
FID_E
ClientSampleId :

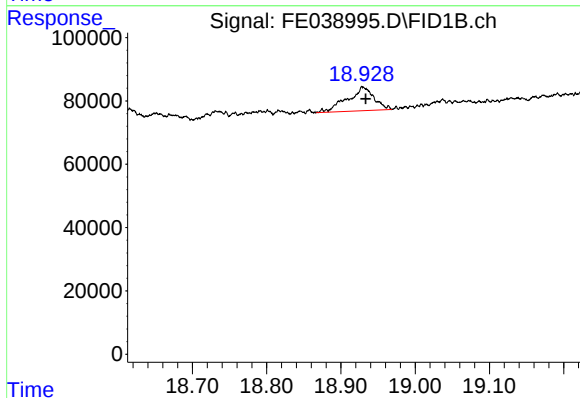


#18 n-Dotriacontane (C32)

R.T.: 18.929 min
Delta R.T.: -0.004 min
Response: 187185
Conc: 1.40 ug/ml

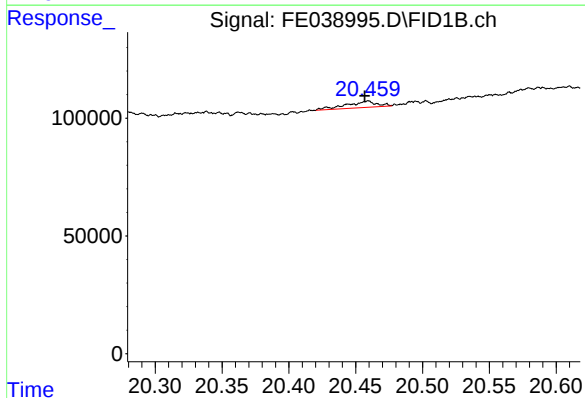

#20 n-Hexatriacontane (C36)

R.T.: 20.459 min
Delta R.T.: 0.002 min
Response: 42834
Conc: 0.33 ug/ml

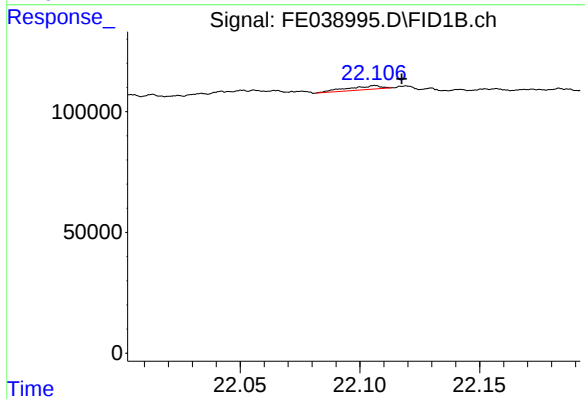

#22 n-Tetracontane (C40)

R.T.: 22.106 min
Delta R.T.: -0.011 min
Response: 14942
Conc: 0.11 ug/ml