

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112922AL\
 Data File : FE038999.D
 Signal(s) : FID1B.ch
 Acq On : 29 Nov 2022 15:08
 Operator : YP\AJ
 Sample : N5787-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 30 03:05:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.952	5572861	35.623 ug/ml
Spiked Amount 50.000		Recovery =	71.25%
12) S 1-chlorooctadecane (S...	13.387	4260280	35.285 ug/ml
Spiked Amount 50.000		Recovery =	70.57%
Target Compounds			
10) T n-Eicosane (C20)	12.886f	56654	0.399 ug/ml
13) T n-Docosane (C22)	14.139	68350	0.489 ug/ml
14) T n-Tetracosane (C24)	15.217	422032	3.056 ug/ml
16) T n-Octacosane (C28)	17.214	125688	0.946 ug/ml
17) T n-Tricontane (C30)	18.097	74379	0.563 ug/ml
18) T n-Dotriacontane (C32)	18.926	36865	0.276 ug/ml
19) T n-Tetratriacontane (C34)	19.777f	55966	0.423 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112922AL\
Data File : FE038999.D
Signal(s) : FID1B.ch
Acq On : 29 Nov 2022 15:08
Operator : YP\AJ
Sample : N5787-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 30 03:05:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

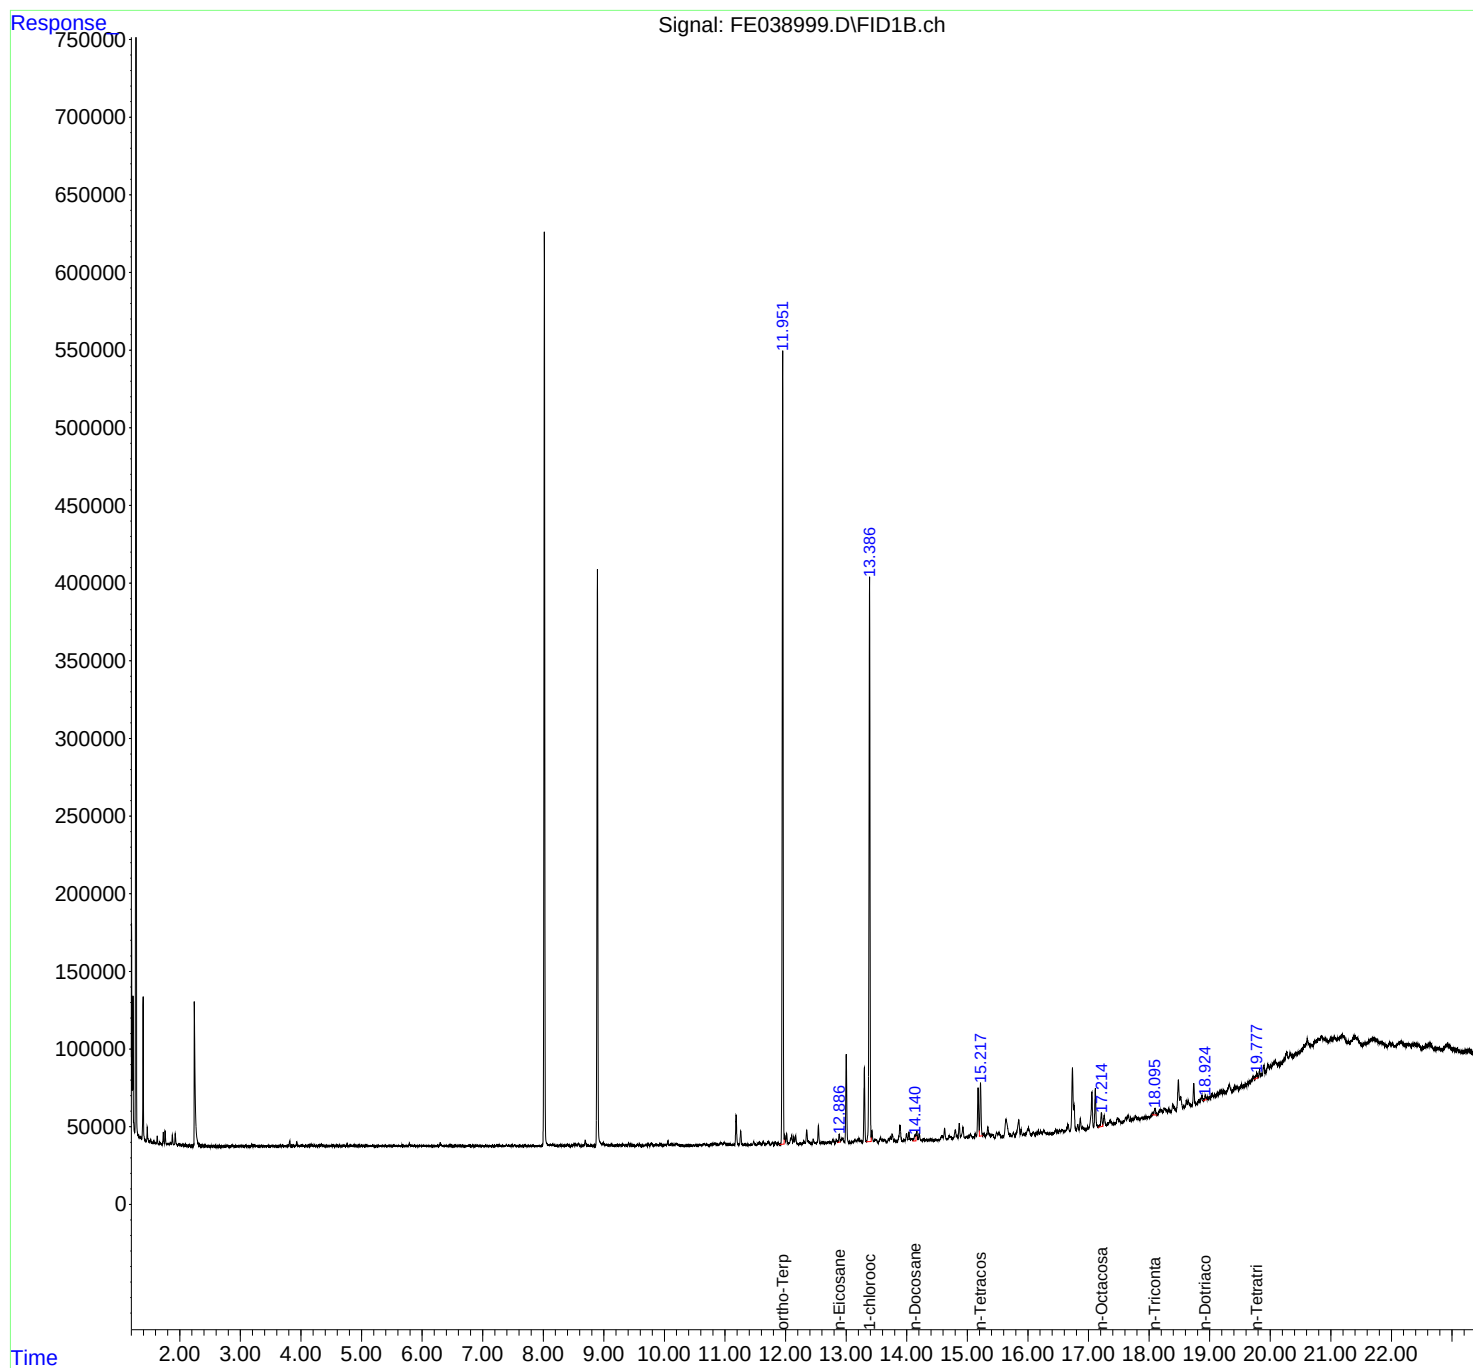


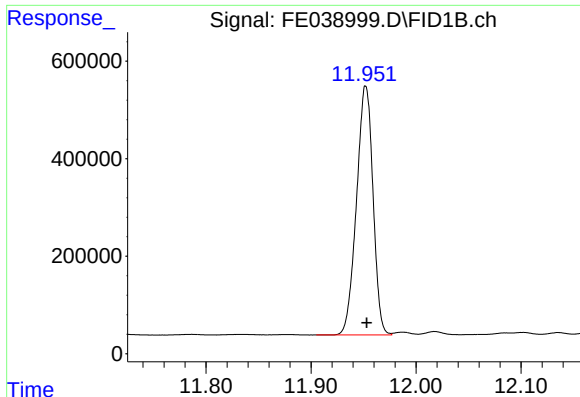

#9 ortho-Terphenyl (SURR)


R.T.: 11.952 min
Delta R.T.: -0.001 min
Response: 5572861
Conc: 35.62 ug/ml

Instrument :
FID_E
ClientSampleId :

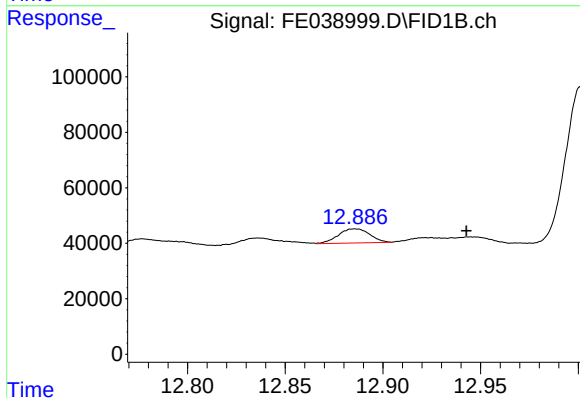


#10 n-Eicosane (C20)

R.T.: 12.886 min
Delta R.T.: -0.057 min
Response: 56654
Conc: 0.40 ug/ml

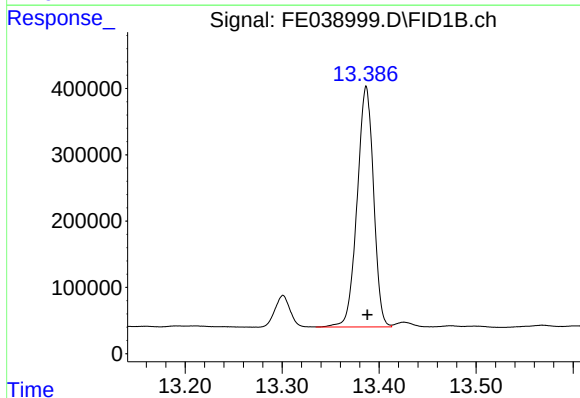


#12 1-chlorooctadecane (SURR)

R.T.: 13.387 min
Delta R.T.: -0.001 min
Response: 4260280
Conc: 35.28 ug/ml

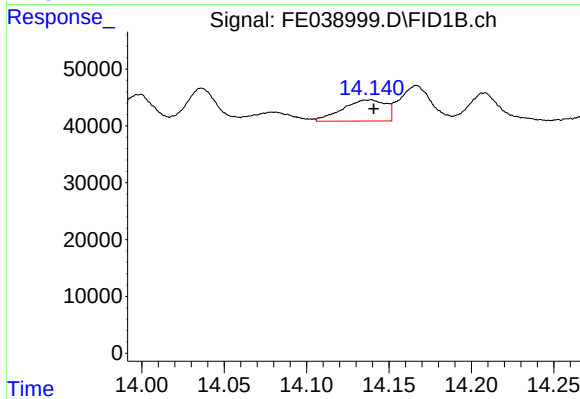

#13 n-Docosane (C22)


R.T.: 14.139 min
Delta R.T.: -0.002 min
Response: 68350
Conc: 0.49 ug/ml

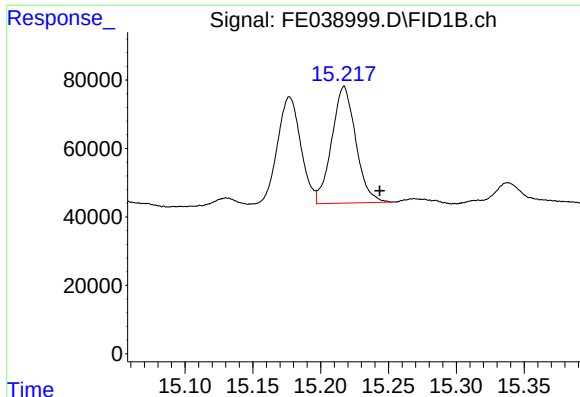

#14 n-Tetracosane (C24)


R.T.: 15.217 min
Delta R.T.: -0.026 min
Response: 422032
Conc: 3.06 ug/ml

Instrument :
FID_E
ClientSampleId :

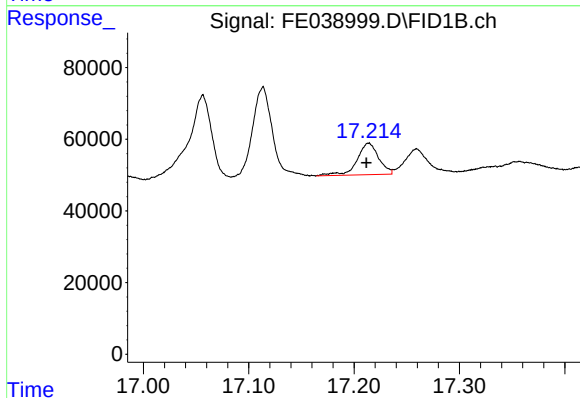


#16 n-Octacosane (C28)

R.T.: 17.214 min
Delta R.T.: 0.002 min
Response: 125688
Conc: 0.95 ug/ml

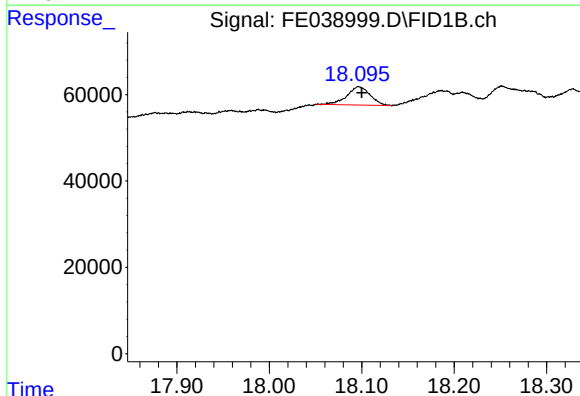


#17 n-Tricontane (C30)

R.T.: 18.097 min
Delta R.T.: -0.004 min
Response: 74379
Conc: 0.56 ug/ml

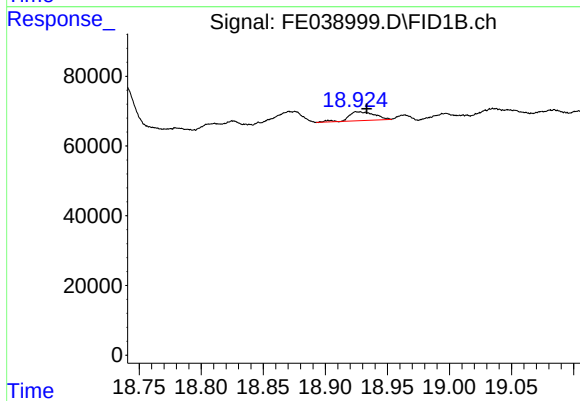

#18 n-Dotriacontane (C32)

R.T.: 18.926 min
Delta R.T.: -0.007 min
Response: 36865
Conc: 0.28 ug/ml

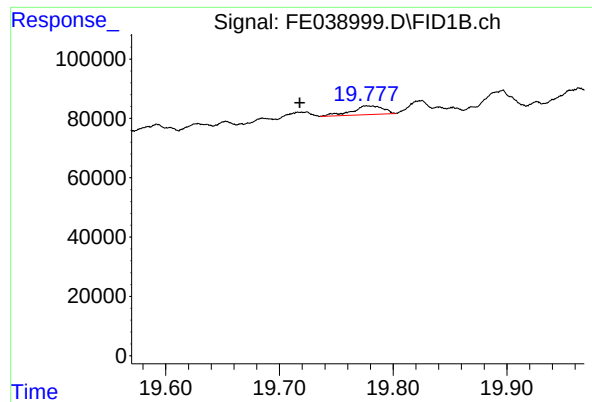

#19 n-Tetratriacontane (C34)

R.T.: 19.777 min
Delta R.T.: 0.059 min
Response: 55966
Conc: 0.42 ug/ml

Instrument :
FID_E
ClientSampleId :