

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112922AL\
 Data File : FE039004.D
 Signal(s) : FID1B.ch
 Acq On : 29 Nov 2022 17:42
 Operator : YP\AJ
 Sample : N5795-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 30 03:06:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.953	6333759	40.487 ug/ml
Spiked Amount 50.000		Recovery =	80.97%
12) S 1-chlorooctadecane (S...	13.387	4798982	39.746 ug/ml
Spiked Amount 50.000		Recovery =	79.49%
Target Compounds			
10) T n-Eicosane (C20)	13.001f	421734	2.971 ug/ml
14) T n-Tetracosane (C24)	15.218	192183	1.392 ug/ml
15) T n-Hexacosane (C26)	16.259	46443	0.346 ug/ml
16) T n-Octacosane (C28)	17.210	104336	0.786 ug/ml
17) T n-Tricontane (C30)	18.096	70194	0.532 ug/ml
18) T n-Dotriacontane (C32)	18.928	51659	0.387 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112922AL\
Data File : FE039004.D
Signal(s) : FID1B.ch
Acq On : 29 Nov 2022 17:42
Operator : YP\AJ
Sample : N5795-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 30 03:06:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

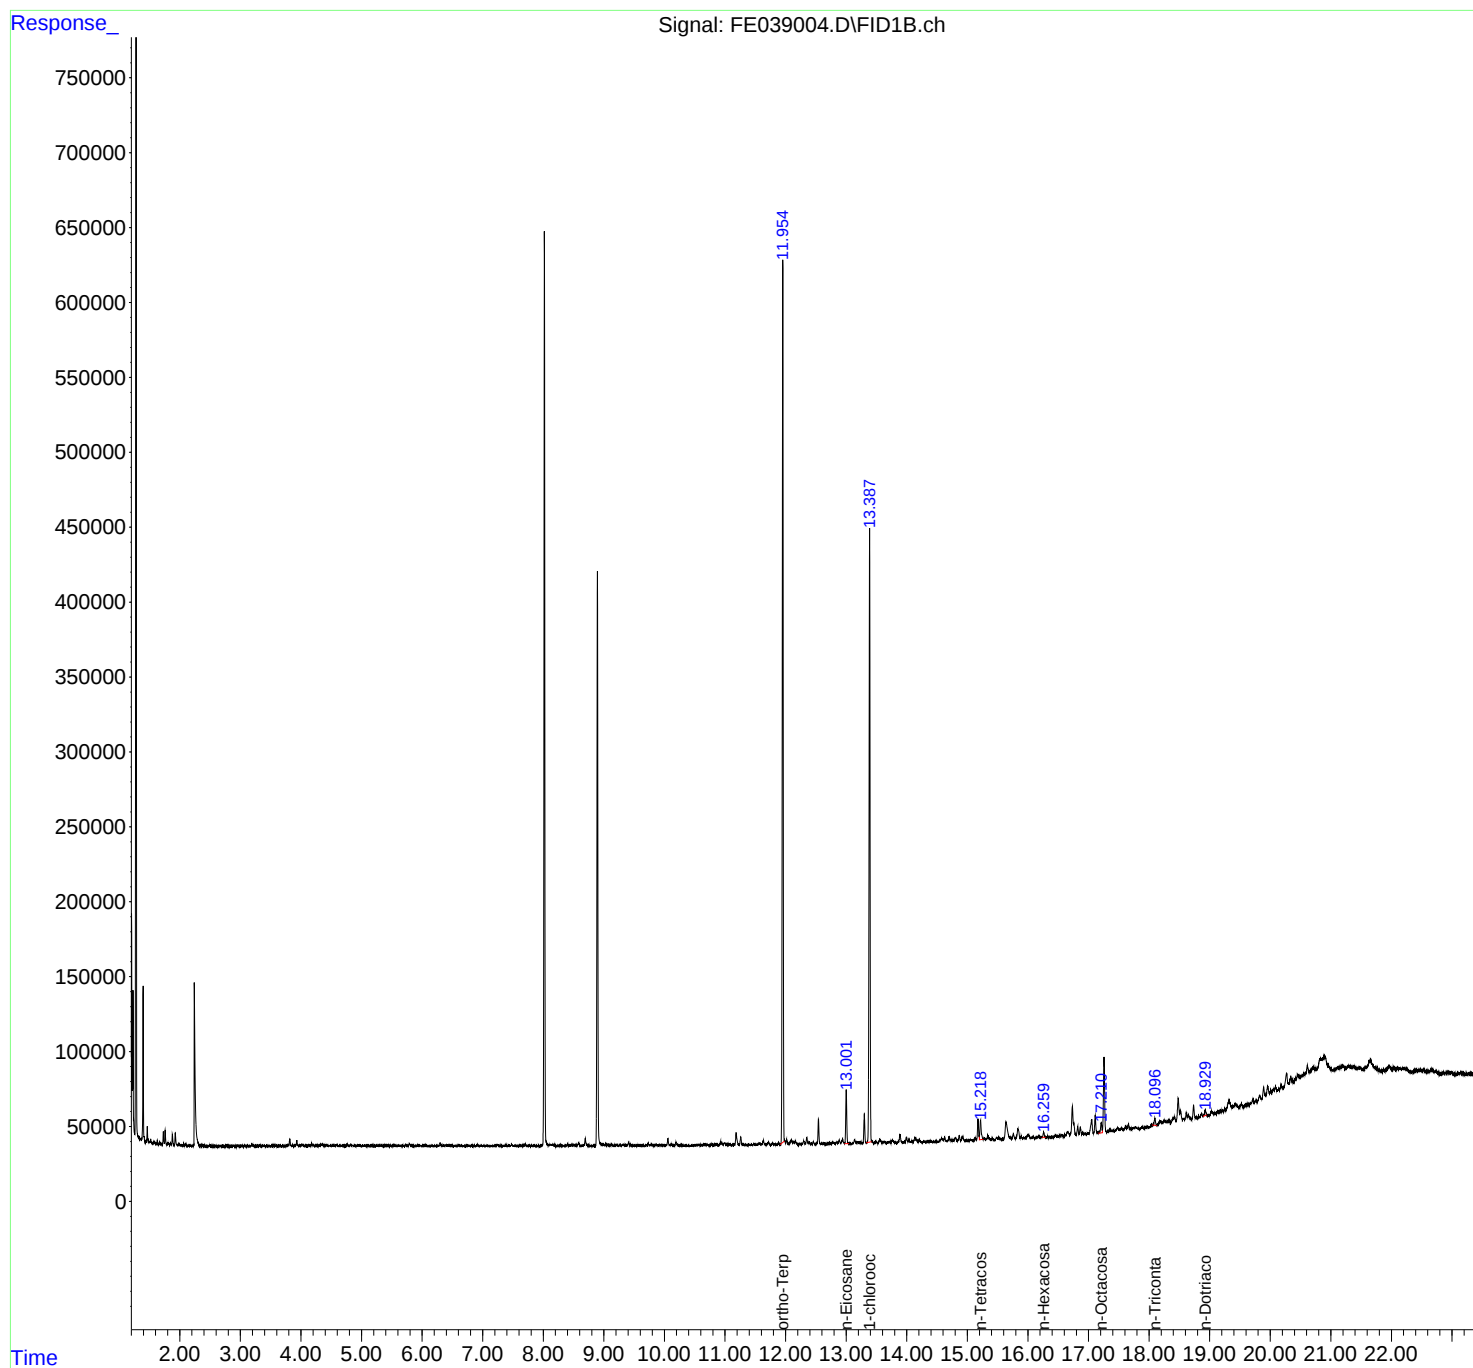


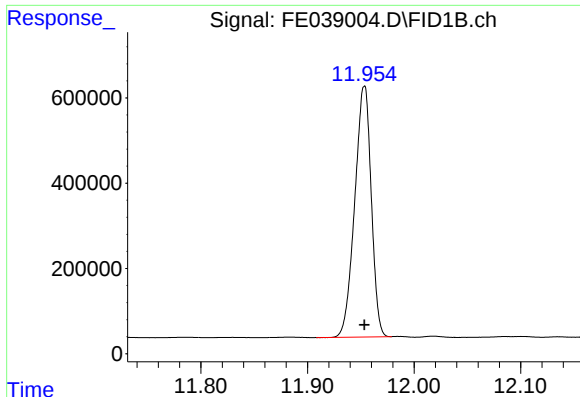

#9 ortho-Terphenyl (SURR)


R.T.: 11.953 min
Delta R.T.: 0.000 min
Response: 6333759
Conc: 40.49 ug/ml

Instrument :
FID_E
ClientSampleId :

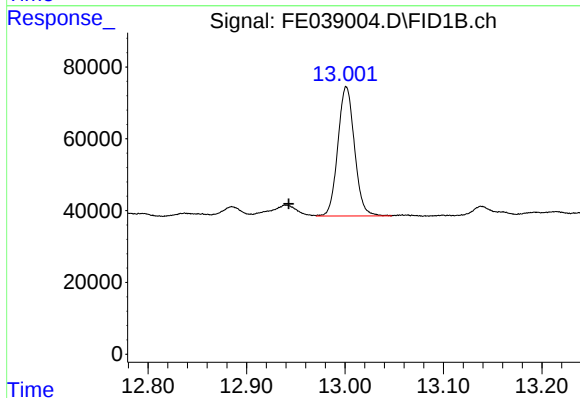


#10 n-Eicosane (C20)

R.T.: 13.001 min
Delta R.T.: 0.059 min
Response: 421734
Conc: 2.97 ug/ml

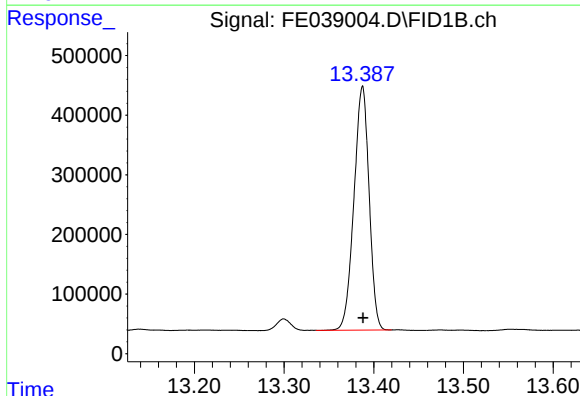


#12 1-chlorooctadecane (SURR)

R.T.: 13.387 min
Delta R.T.: 0.000 min
Response: 4798982
Conc: 39.75 ug/ml

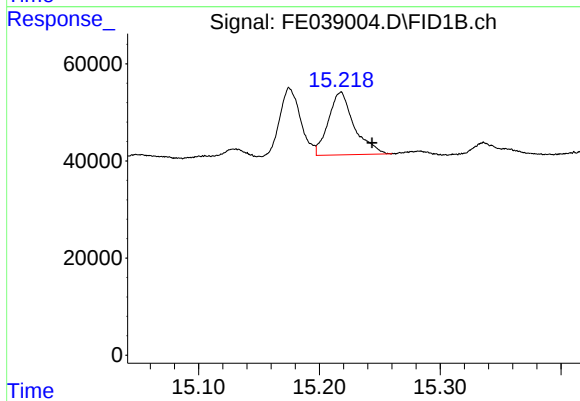

#14 n-Tetracosane (C24)


R.T.: 15.218 min
Delta R.T.: -0.026 min
Response: 192183
Conc: 1.39 ug/ml

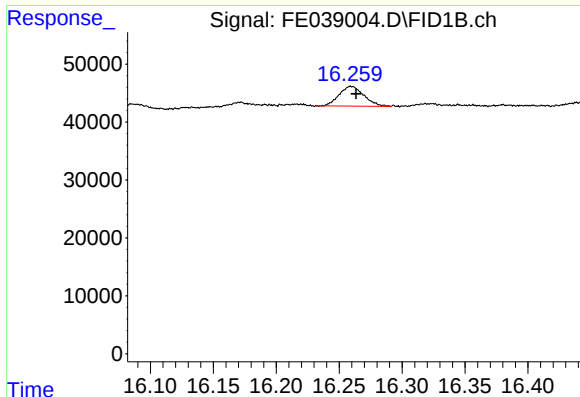

#15 n-Hexacosane (C26)


R.T.: 16.259 min
Delta R.T.: -0.004 min
Response: 46443
Conc: 0.35 ug/ml

Instrument :
FID_E
ClientSampleId :

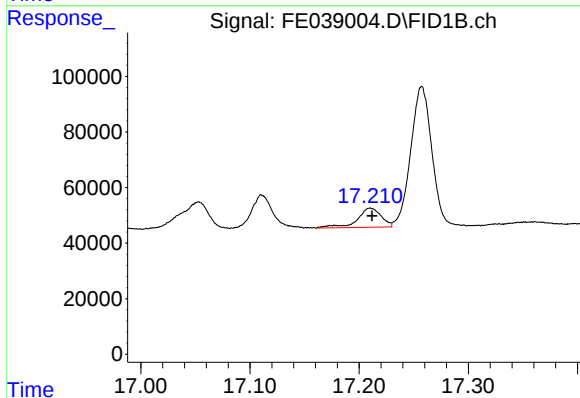


#16 n-Octacosane (C28)

R.T.: 17.210 min
Delta R.T.: -0.002 min
Response: 104336
Conc: 0.79 ug/ml

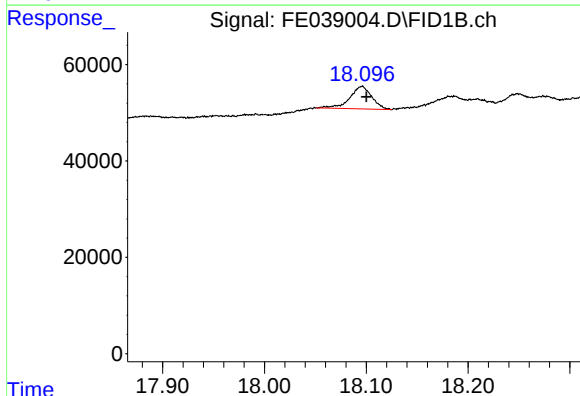

#17 n-Tricontane (C30)

R.T.: 18.096 min
Delta R.T.: -0.004 min
Response: 70194
Conc: 0.53 ug/ml

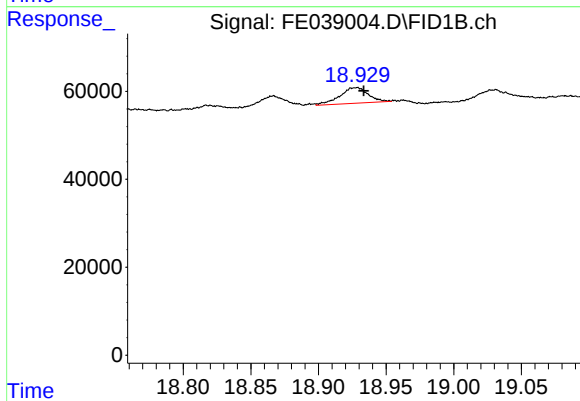

#18 n-Dotriacontane (C32)

R.T.: 18.928 min
Delta R.T.: -0.005 min
Response: 51659
Conc: 0.39 ug/ml