

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112922AL\
 Data File : FE039008.D
 Signal(s) : FID1B.ch
 Acq On : 29 Nov 2022 19:46
 Operator : YP\AJ
 Sample : N5796-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 30 03:07:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.953	5520332	35.287 ug/ml
Spiked Amount 50.000		Recovery =	70.57%
12) S 1-chlorooctadecane (S...	13.387	4194587	34.741 ug/ml
Spiked Amount 50.000		Recovery =	69.48%
Target Compounds			
10) T n-Eicosane (C20)	12.885f	38730	0.273 ug/ml
14) T n-Tetracosane (C24)	15.216	65582	0.475 ug/ml
15) T n-Hexacosane (C26)	16.261	22265	0.166 ug/ml
16) T n-Octacosane (C28)	17.212	97908	0.737 ug/ml
17) T n-Tricontane (C30)	18.098	121164	0.917 ug/ml
18) T n-Dotriacontane (C32)	18.928	180752	1.355 ug/ml
20) T n-Hexatriacontane (C36)	20.526f	9133	0.071 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112922AL\
Data File : FE039008.D
Signal(s) : FID1B.ch
Acq On : 29 Nov 2022 19:46
Operator : YP\AJ
Sample : N5796-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 30 03:07:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

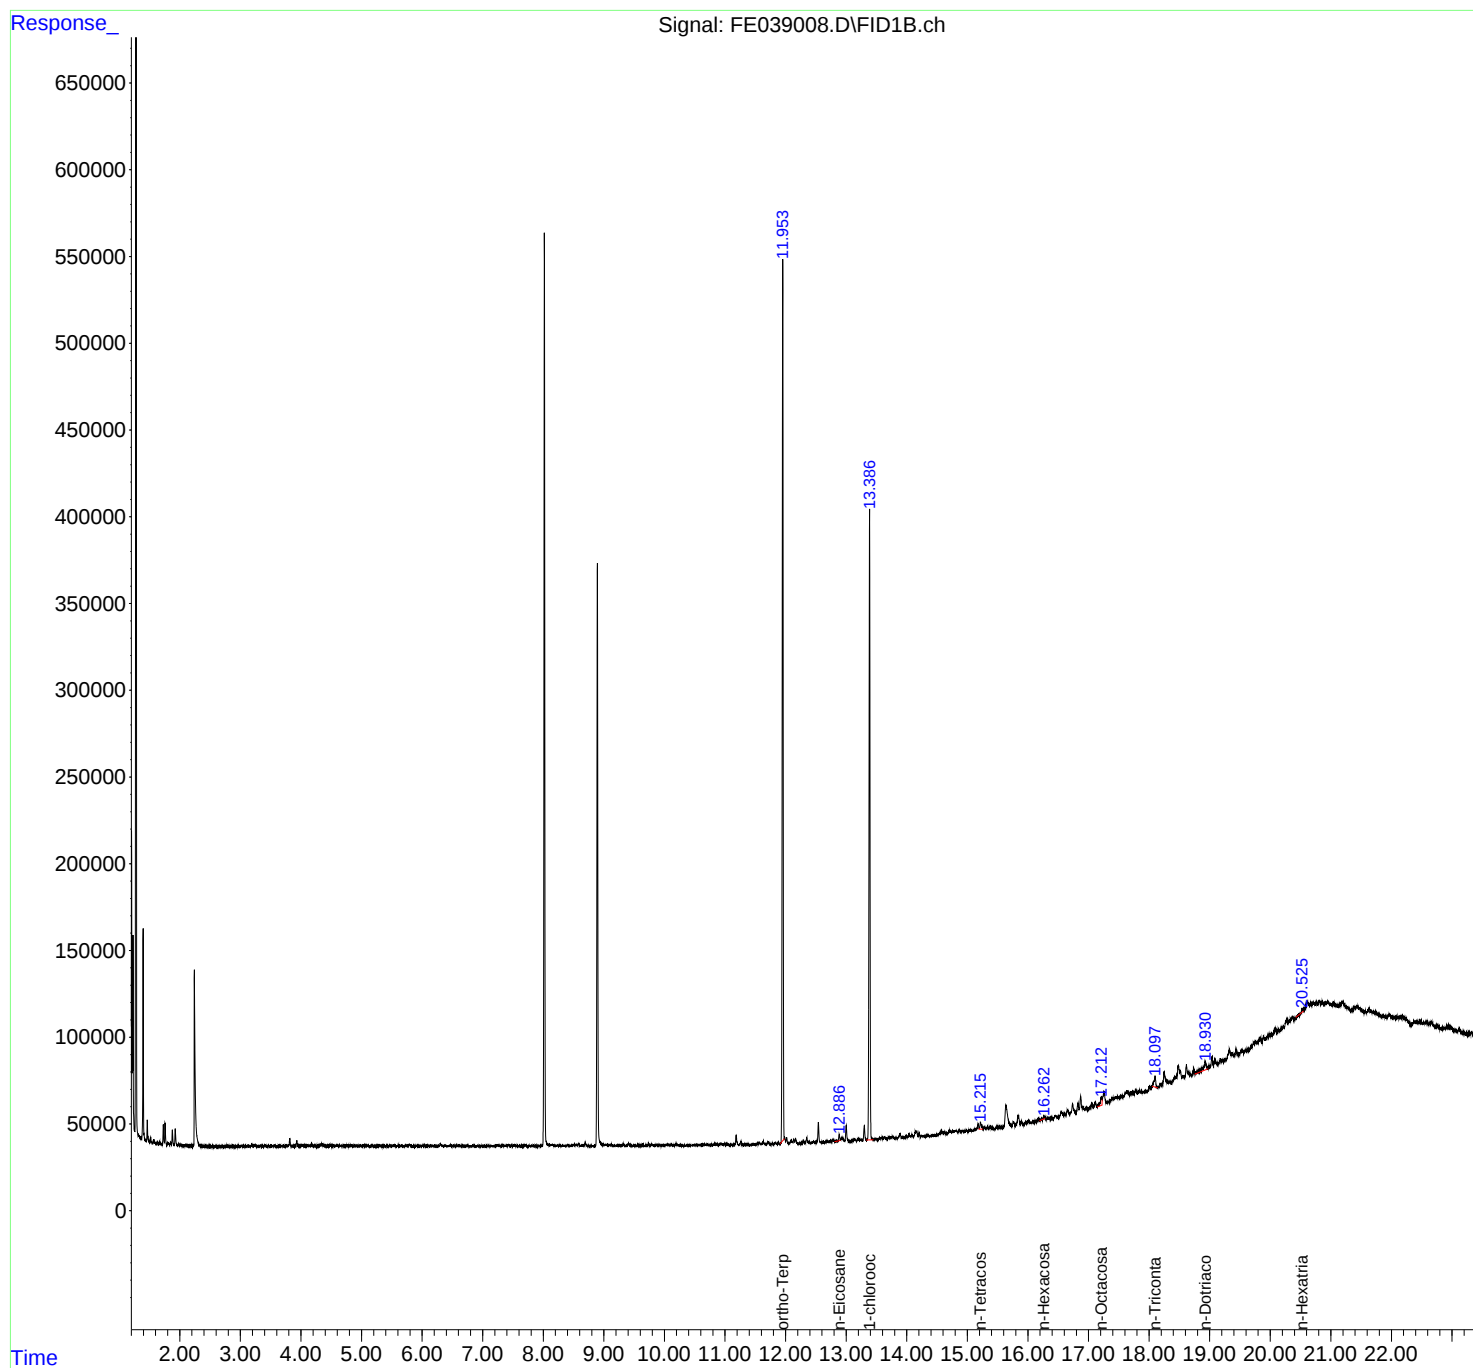


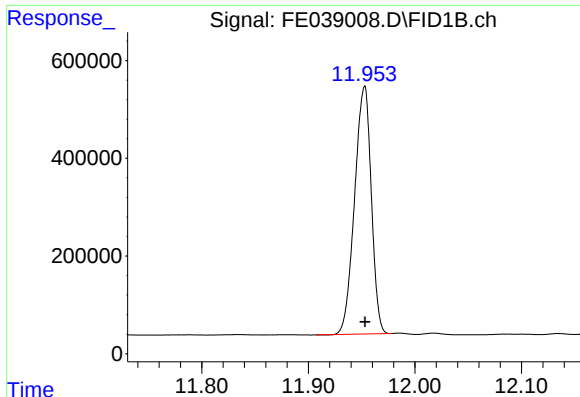

#9 ortho-Terphenyl (SURR)


R.T.: 11.953 min
Delta R.T.: 0.000 min
Response: 5520332
Conc: 35.29 ug/ml

Instrument :
FID_E
ClientSampleId :

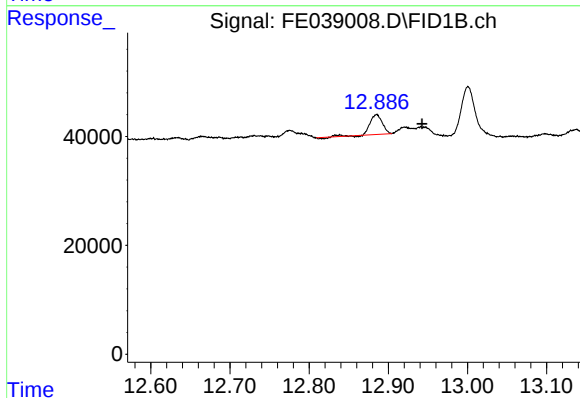


#10 n-Eicosane (C20)

R.T.: 12.885 min
Delta R.T.: -0.057 min
Response: 38730
Conc: 0.27 ug/ml

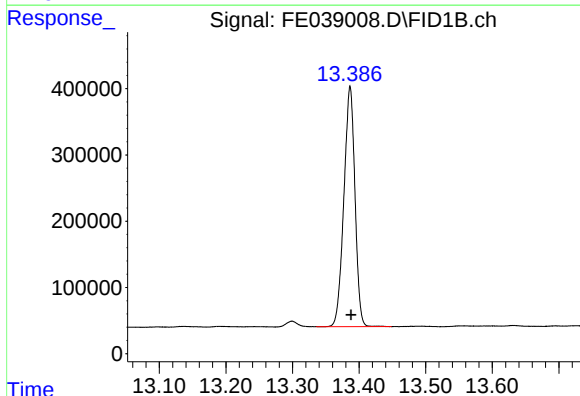


#12 1-chlorooctadecane (SURR)

R.T.: 13.387 min
Delta R.T.: -0.002 min
Response: 4194587
Conc: 34.74 ug/ml

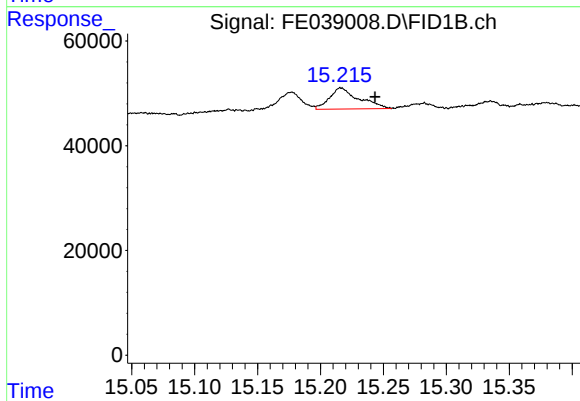

#14 n-Tetracosane (C24)


R.T.: 15.216 min
Delta R.T.: -0.027 min
Response: 65582
Conc: 0.47 ug/ml

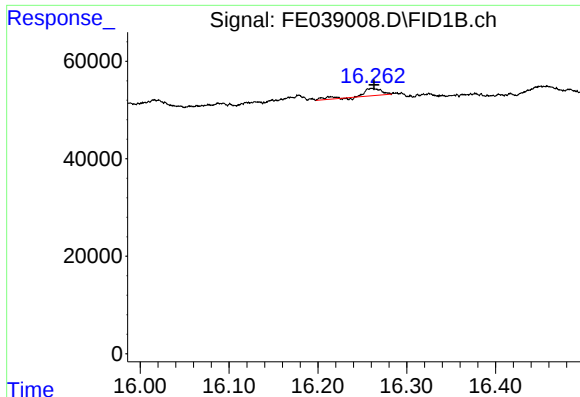

#15 n-Hexacosane (C26)


R.T.: 16.261 min
Delta R.T.: -0.002 min
Response: 22265
Conc: 0.17 ug/ml

Instrument :
FID_E
ClientSampleId :

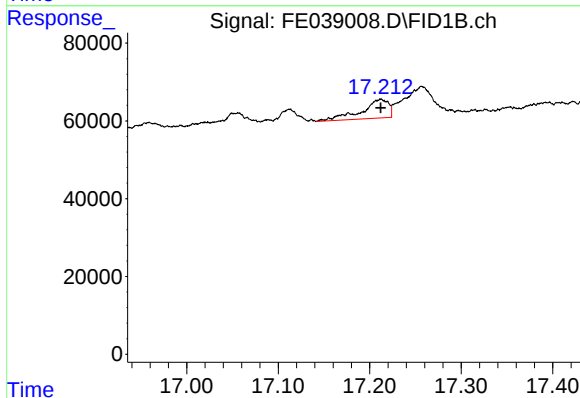


#16 n-Octacosane (C28)

R.T.: 17.212 min
Delta R.T.: 0.000 min
Response: 97908
Conc: 0.74 ug/ml

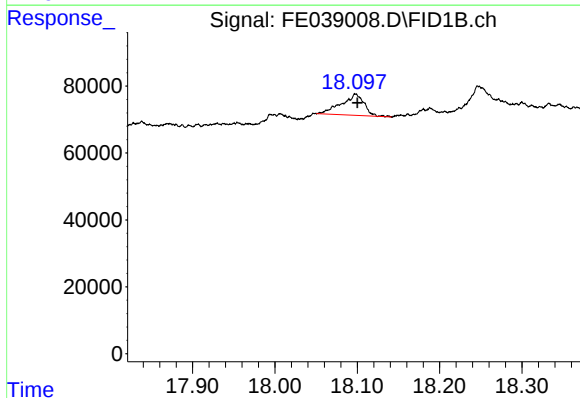


#17 n-Tricontane (C30)

R.T.: 18.098 min
Delta R.T.: -0.002 min
Response: 121164
Conc: 0.92 ug/ml

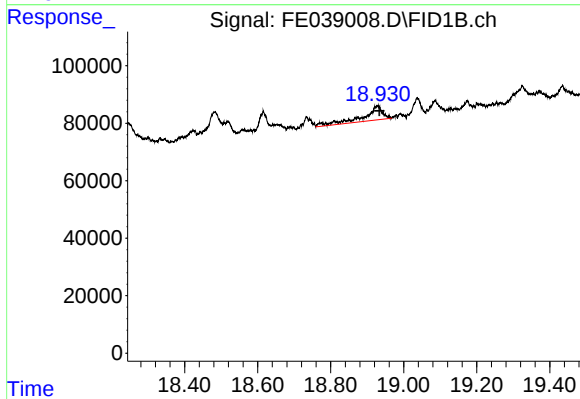

#18 n-Dotriacontane (C32)

R.T.: 18.928 min
Delta R.T.: -0.005 min
Response: 180752
Conc: 1.36 ug/ml

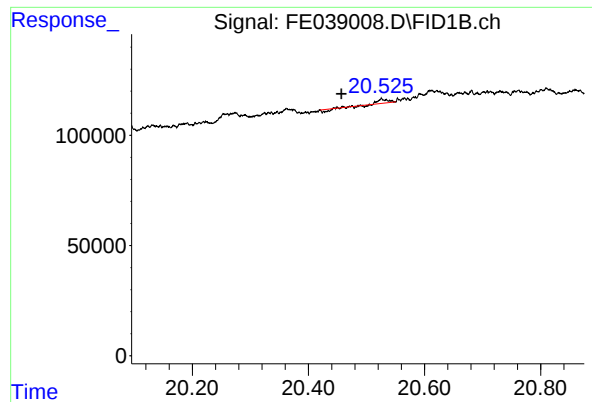

#20 n-Hexatriacontane (C36)

R.T.: 20.526 min
Delta R.T.: 0.069 min
Response: 9133
Conc: 0.07 ug/ml

Instrument :
FID_E
ClientSampleId :