

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE113022AL\
 Data File : FE039047.D
 Signal(s) : FID1B.ch
 Acq On : 01 Dec 2022 06:38
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 01 09:37:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

16) T	n-Octacosane (C28)	17.215	44922	0.338 ug/ml
18) T	n-Dotriacontane (C32)	18.933	96516	0.724 ug/ml
19) T	n-Tetratriacontane (C34)	19.724	37440	0.283 ug/ml
20) T	n-Hexatriacontane (C36)	20.477	90007	0.701 ug/ml
21) T	n-Octatriacontane (C38)	21.179	265884	2.029 ug/ml
22) T	n-Tetracontane (C40)	22.117	59526	0.437 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE113022AL\
Data File : FE039047.D
Signal(s) : FID1B.ch
Acq On : 01 Dec 2022 06:38
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 01 09:37:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

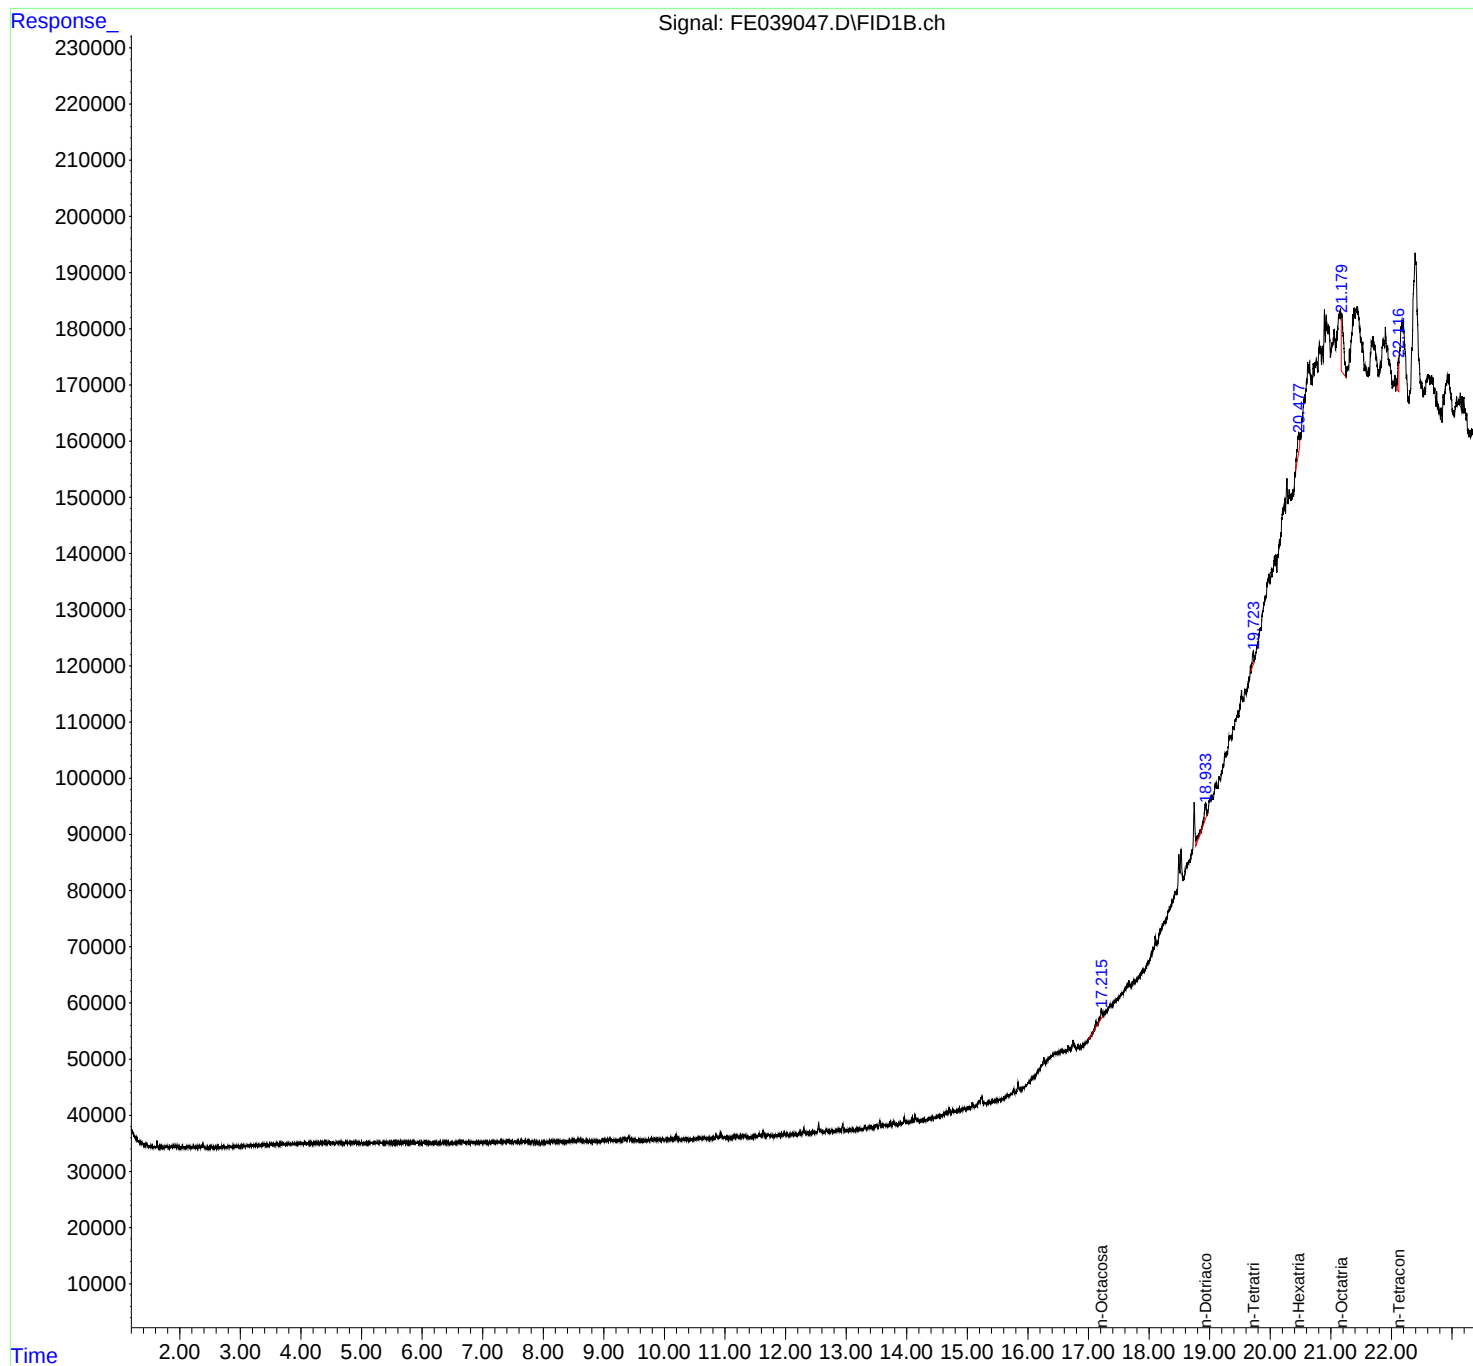


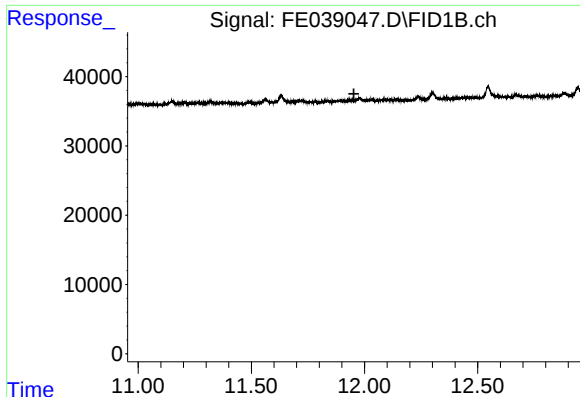

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.953 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

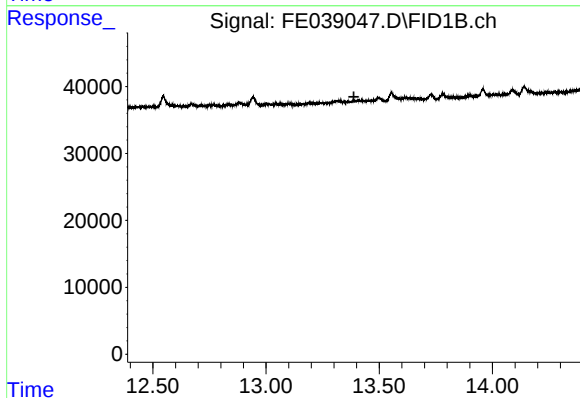


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.388 min
Response: 0
Conc: N.D.

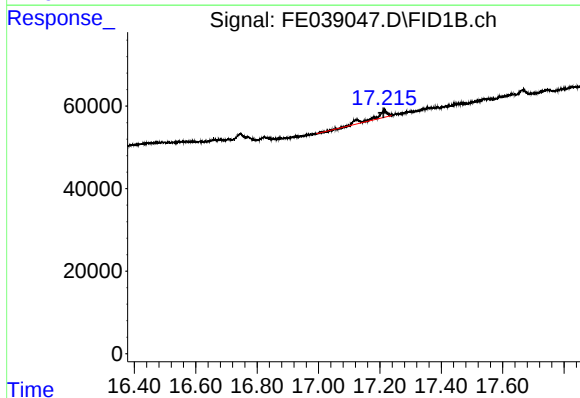


#16 n-Octacosane (C28)

R.T.: 17.215 min
Delta R.T.: 0.003 min
Response: 44922
Conc: 0.34 ug/ml

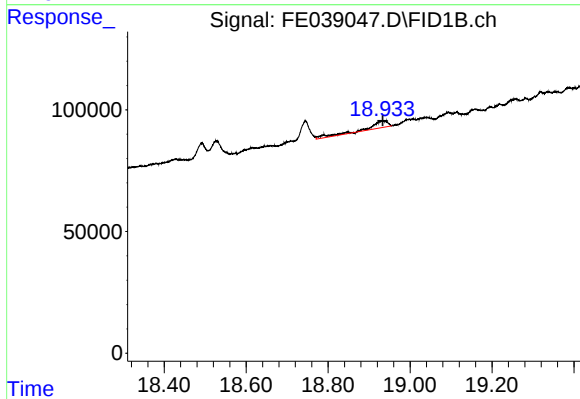

#18 n-Dotriacontane (C32)


R.T.: 18.933 min
Delta R.T.: 0.000 min
Response: 96516
Conc: 0.72 ug/ml

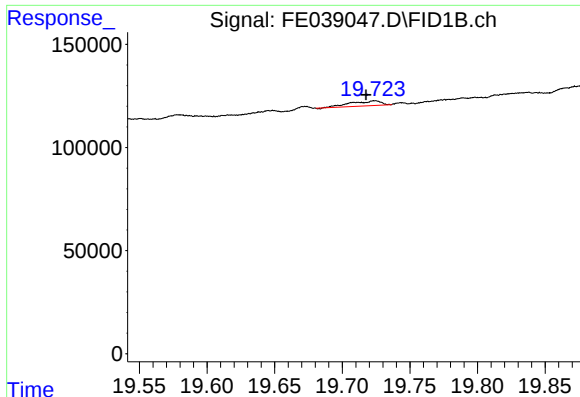

#19 n-Tetratriacontane (C34)


R.T.: 19.724 min
Delta R.T.: 0.006 min
Response: 37440
Conc: 0.28 ug/ml

Instrument :
FID_E
ClientSampleId :

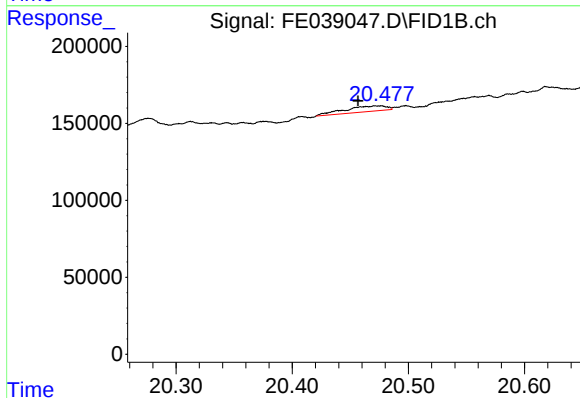


#20 n-Hexatriacontane (C36)

R.T.: 20.477 min
Delta R.T.: 0.020 min
Response: 90007
Conc: 0.70 ug/ml

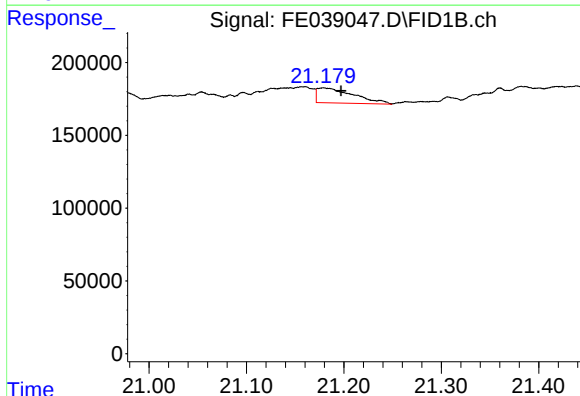

#21 n-Octatriacontane (C38)

R.T.: 21.179 min
Delta R.T.: -0.018 min
Response: 265884
Conc: 2.03 ug/ml

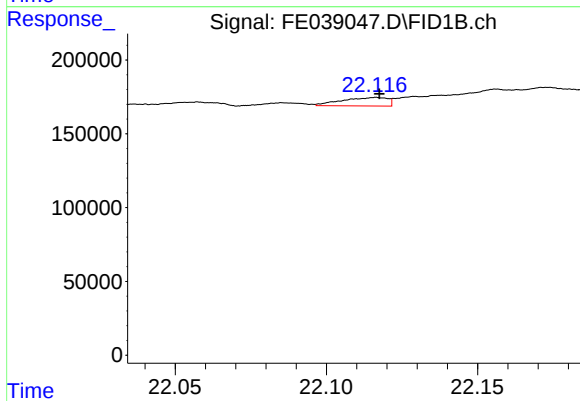

#22 n-Tetracontane (C40)

R.T.: 22.117 min
Delta R.T.: 0.000 min
Response: 59526
Conc: 0.44 ug/ml