

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE113023AL\
 Data File : FE045591.D
 Signal(s) : FID1B.ch
 Acq On : 30 Nov 2023 12:50
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 30 14:28:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 113023.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 30 12:25:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.882	152935	0.838 ug/ml
20) T n-Hexatriacontane (C36)	20.437f	155804	0.982 ug/ml
22) T n-Tetracontane (C40)	22.089f	304619	2.143 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE113023AL\
Data File : FE045591.D
Signal(s) : FID1B.ch
Acq On : 30 Nov 2023 12:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 30 14:28:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 113023.M
Quant Title : GC Extractables
QLast Update : Thu Nov 30 12:25:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

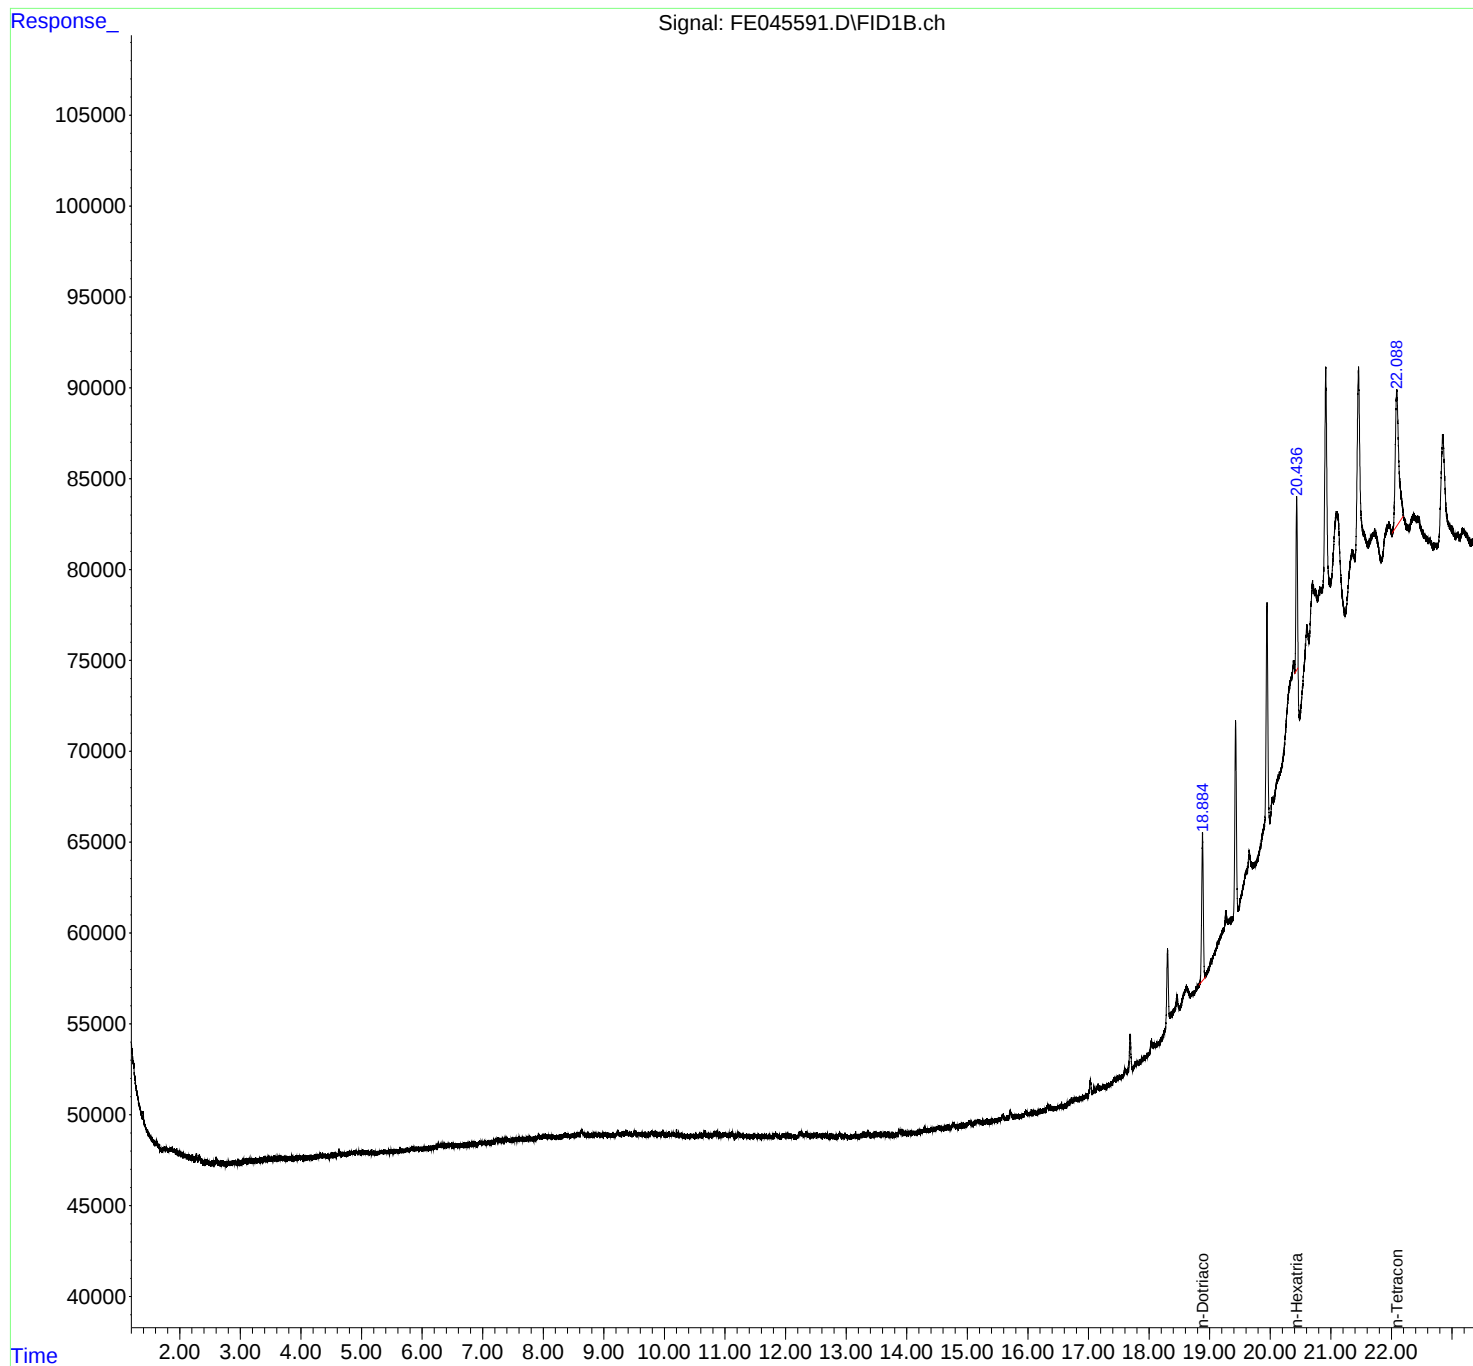


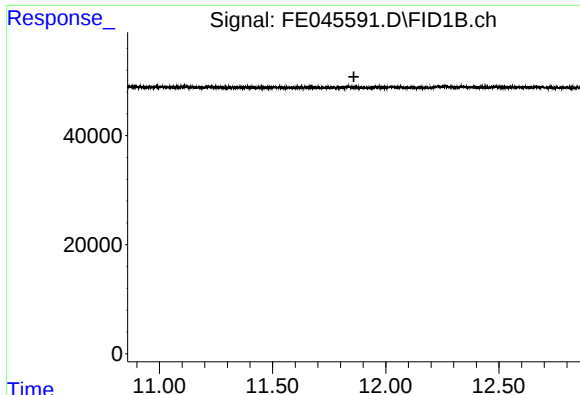

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.859 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

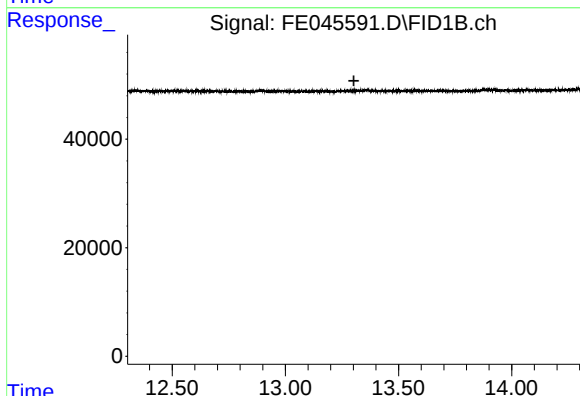


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.303 min
Response: 0
Conc: N.D.

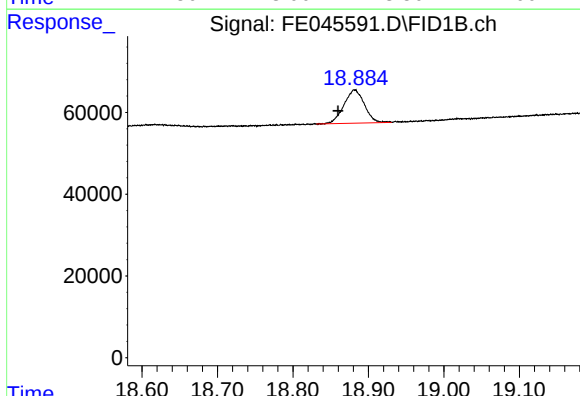


#18 n-Dotriacontane (C32)

R.T.: 18.882 min
Delta R.T.: 0.022 min
Response: 152935
Conc: 0.84 ug/ml

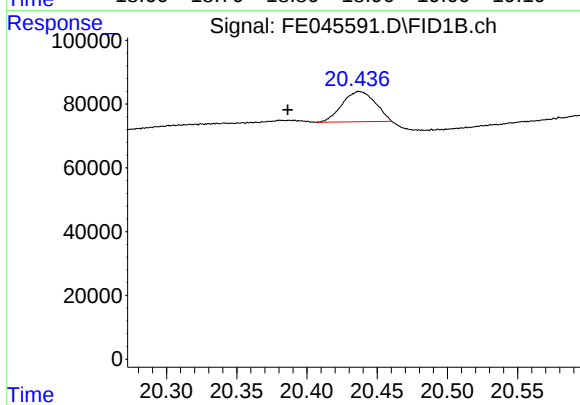

#20 n-Hexatriacontane (C36)

R.T.: 20.437 min
Delta R.T.: 0.051 min
Response: 155804
Conc: 0.98 ug/ml

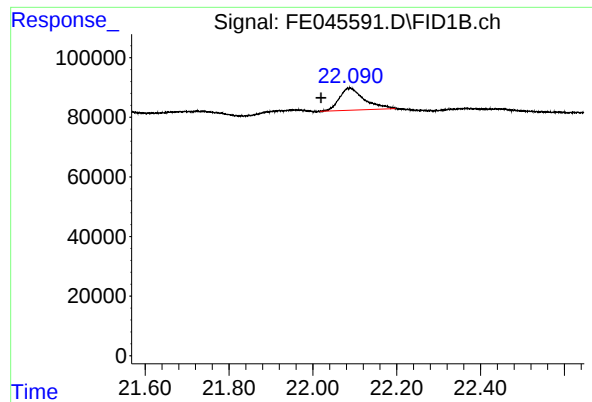

#22 n-Tetracontane (C40)

R.T.: 22.089 min
Delta R.T.: 0.069 min
Response: 304619
Conc: 2.14 ug/ml

Instrument :

FID_E

ClientSampleId :