

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120122AL\
 Data File : FE039054.D
 Signal(s) : FID1B.ch
 Acq On : 01 Dec 2022 10:49
 Operator : YP\AJ
 Sample : N5801-03DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 01 12:57:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.948	831156	5.313 ug/ml
Spiked Amount 50.000		Recovery =	10.63%
12) S 1-chlorooctadecane (S...	13.384	785652	6.507 ug/ml
Spiked Amount 50.000		Recovery =	13.01%
Target Compounds			
10) T n-Eicosane (C20)	12.946	42823	0.302 ug/ml
11) T n-Heneicosane (C21)	13.568	62397	0.439 ug/ml
13) T n-Docosane (C22)	14.166	260085	1.861 ug/ml
14) T n-Tetracosane (C24)	15.218	856346	6.201 ug/ml
16) T n-Octacosane (C28)	17.216	278022	2.094 ug/ml
17) T n-Tricontane (C30)	18.099	86978	0.659 ug/ml
18) T n-Dotriacontane (C32)	18.930	48443	0.363 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120122AL\
Data File : FE039054.D
Signal(s) : FID1B.ch
Acq On : 01 Dec 2022 10:49
Operator : YP\AJ
Sample : N5801-03DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 01 12:57:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

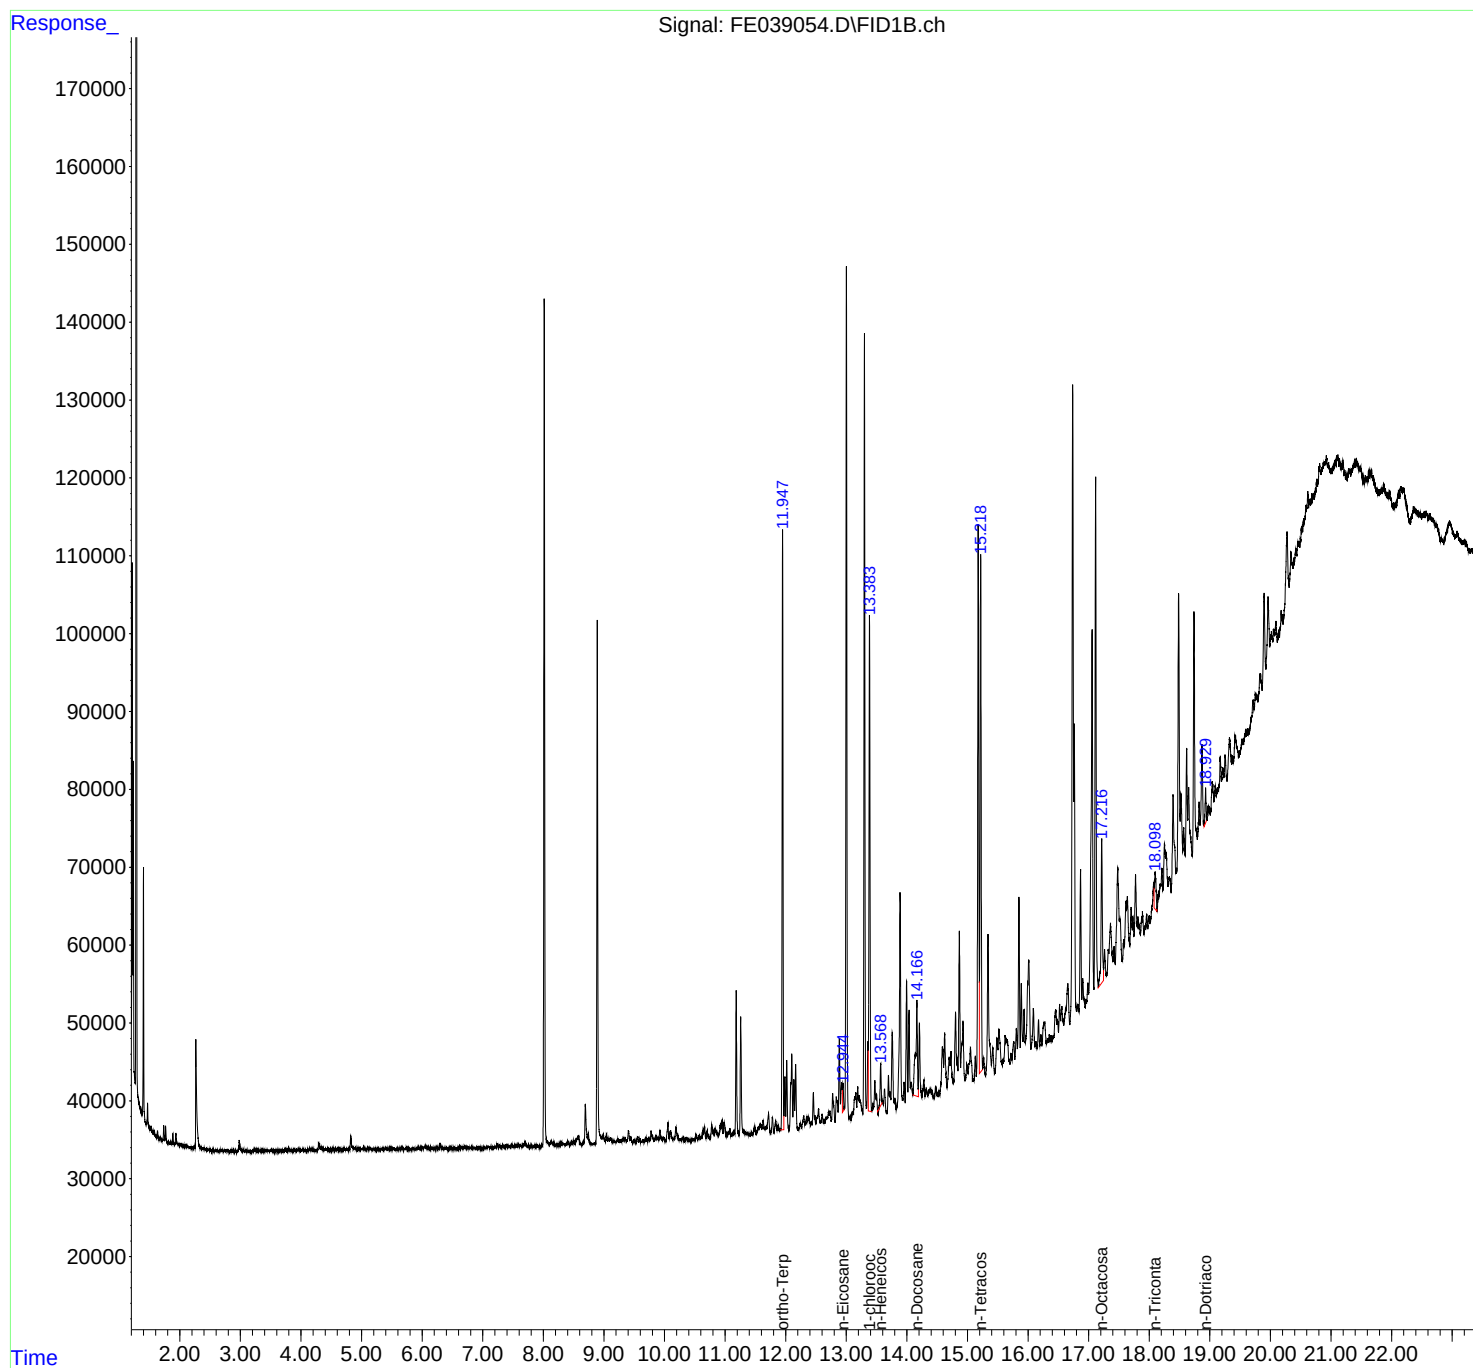


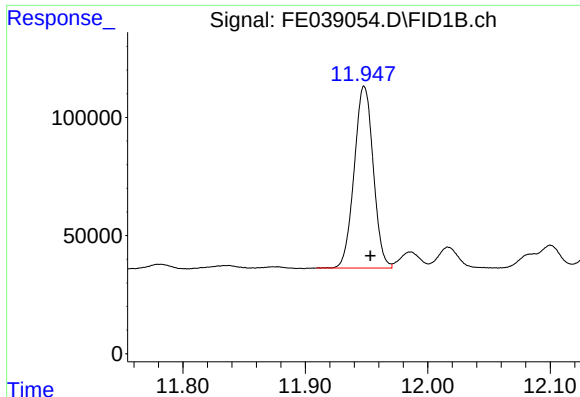

#9 ortho-Terphenyl (SURR)


R.T.: 11.948 min
Delta R.T.: -0.005 min
Response: 831156
Conc: 5.31 ug/ml

Instrument :
FID_E
ClientSampleId :

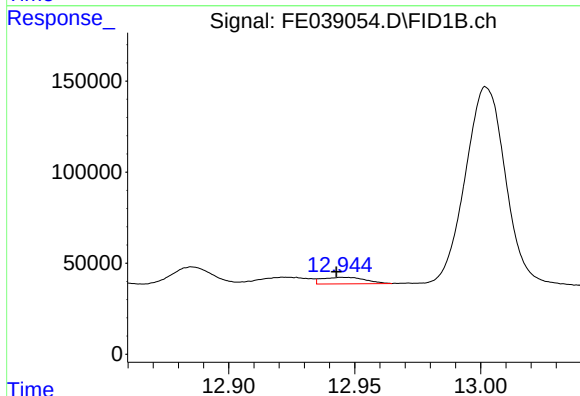


#10 n-Eicosane (C20)

R.T.: 12.946 min
Delta R.T.: 0.003 min
Response: 42823
Conc: 0.30 ug/ml

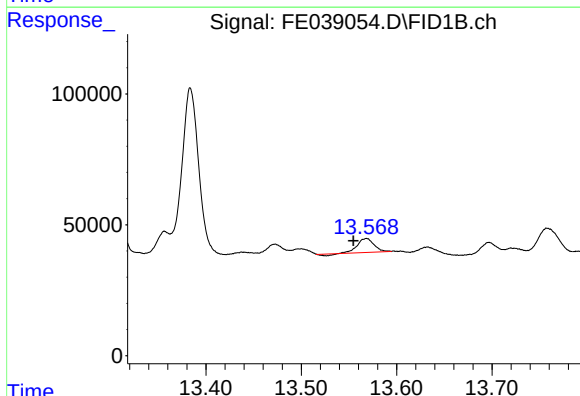


#11 n-Heneicosane (C21)

R.T.: 13.568 min
Delta R.T.: 0.014 min
Response: 62397
Conc: 0.44 ug/ml

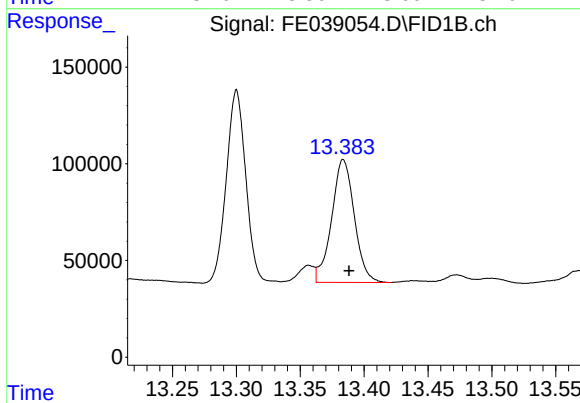

#12 1-chlorooctadecane (SURR)


R.T.: 13.384 min
Delta R.T.: -0.004 min
Response: 785652
Conc: 6.51 ug/ml

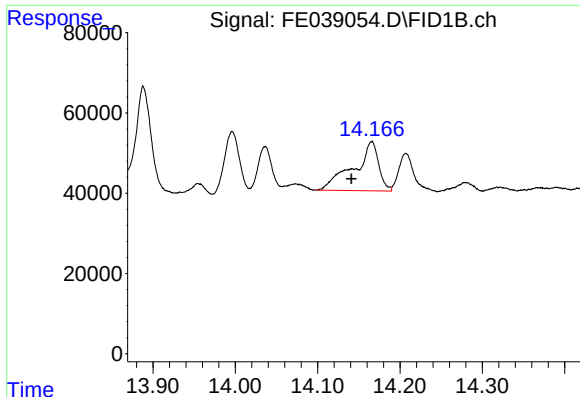

#13 n-Docosane (C22)


R.T.: 14.166 min
Delta R.T.: 0.025 min
Response: 260085
Conc: 1.86 ug/ml

Instrument :
FID_E
ClientSampleId :

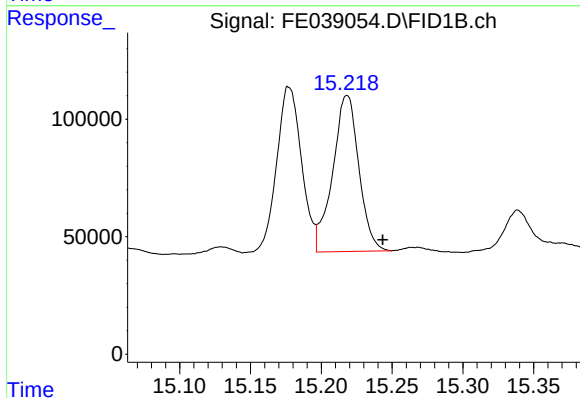


#14 n-Tetracosane (C24)

R.T.: 15.218 min
Delta R.T.: -0.025 min
Response: 856346
Conc: 6.20 ug/ml

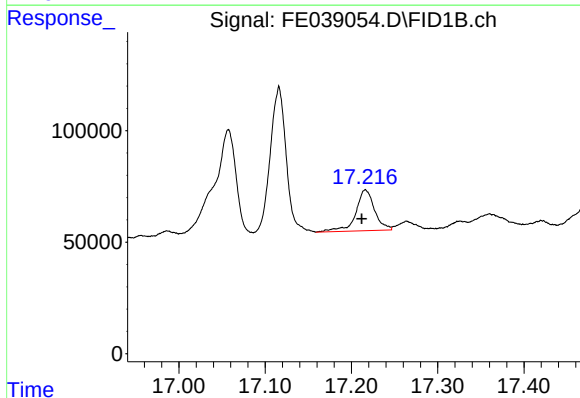


#16 n-Octacosane (C28)

R.T.: 17.216 min
Delta R.T.: 0.004 min
Response: 278022
Conc: 2.09 ug/ml

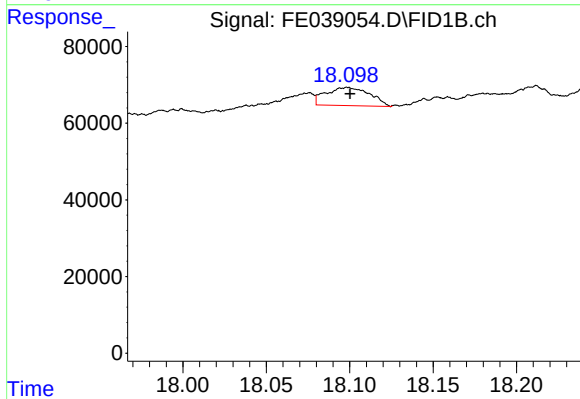

#17 n-Tricontane (C30)

R.T.: 18.099 min
Delta R.T.: -0.002 min
Response: 86978
Conc: 0.66 ug/ml

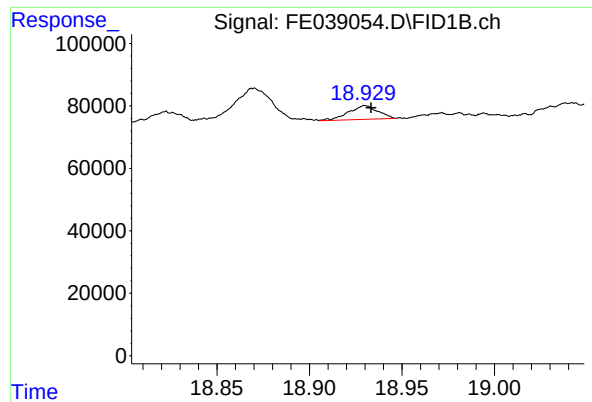

#18 n-Dotriacontane (C32)

R.T.: 18.930 min
Delta R.T.: -0.003 min
Response: 48443
Conc: 0.36 ug/ml

Instrument :

FID_E

ClientSampleId :