

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120222AL\
 Data File : FE039087.D
 Signal(s) : FID1B.ch
 Acq On : 02 Dec 2022 15:11
 Operator : YP\AJ
 Sample : PB149395BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 02 15:56:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.947	7443222	47.579 ug/ml
Spiked Amount 50.000		Recovery =	95.16%
12) S 1-chlorooctadecane (S...	13.381	5518030	45.702 ug/ml
Spiked Amount 50.000		Recovery =	91.40%
Target Compounds			
10) T n-Eicosane (C20)	12.929	99853	0.703 ug/ml
11) T n-Heneicosane (C21)	13.544	90577	0.637 ug/ml
13) T n-Docosane (C22)	14.130	90683	0.649 ug/ml
14) T n-Tetracosane (C24)	15.233	88507	0.641 ug/ml
15) T n-Hexacosane (C26)	16.253	52498	0.391 ug/ml
16) T n-Octacosane (C28)	17.206	47902	0.361 ug/ml
18) T n-Dotriacontane (C32)	18.924	76052	0.570 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120222AL\
Data File : FE039087.D
Signal(s) : FID1B.ch
Acq On : 02 Dec 2022 15:11
Operator : YP\AJ
Sample : PB149395BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 02 15:56:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

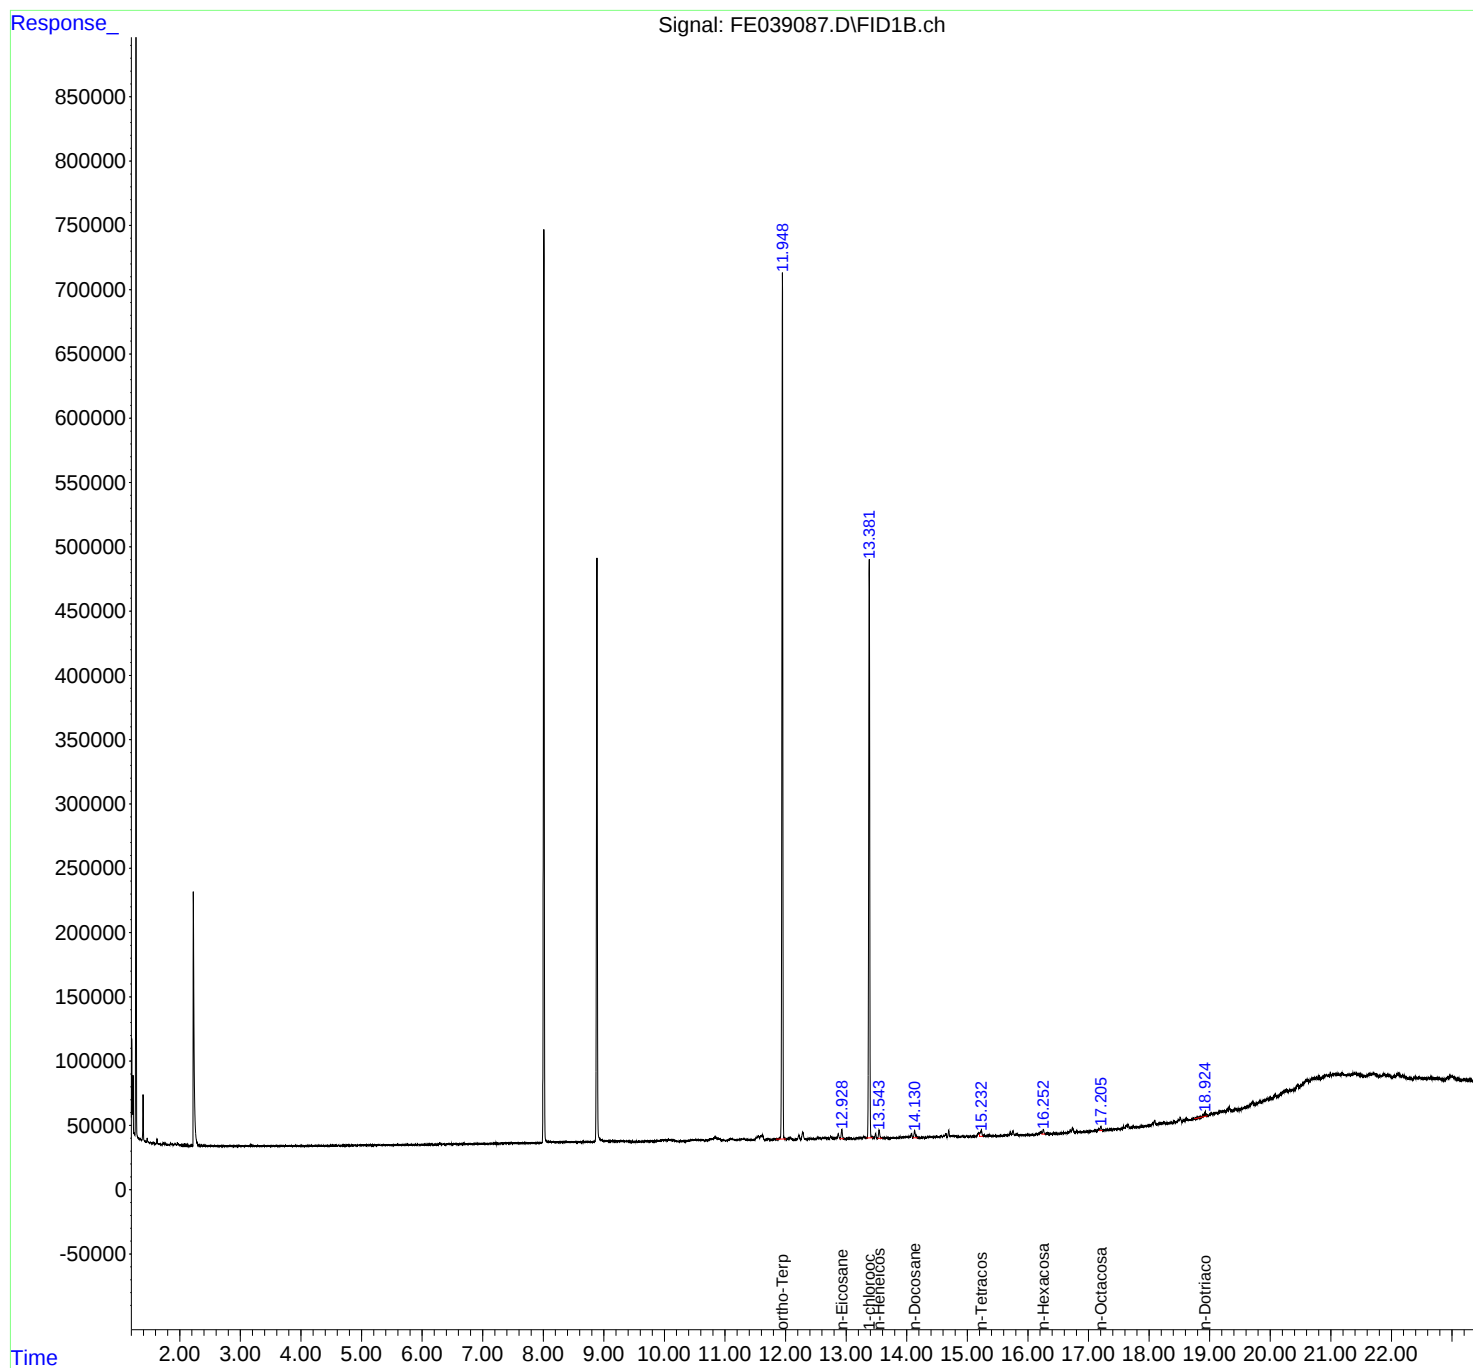


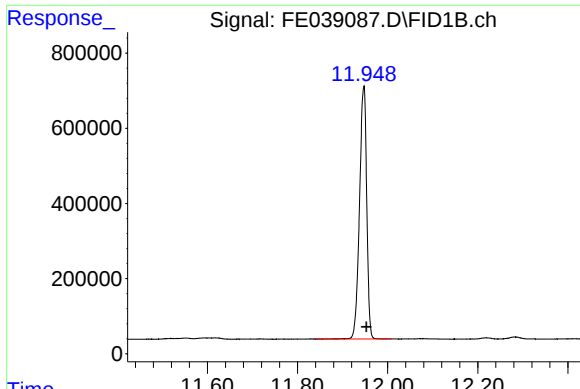

#9 ortho-Terphenyl (SURR)


R.T.: 11.947 min
Delta R.T.: -0.006 min
Response: 7443222
Conc: 47.58 ug/ml

Instrument :
FID_E
ClientSampleId :

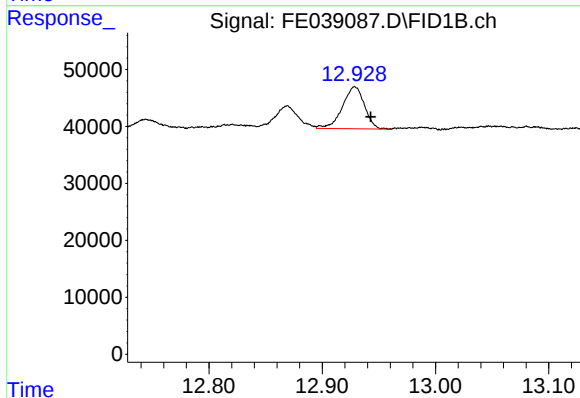


#10 n-Eicosane (C20)

R.T.: 12.929 min
Delta R.T.: -0.014 min
Response: 99853
Conc: 0.70 ug/ml

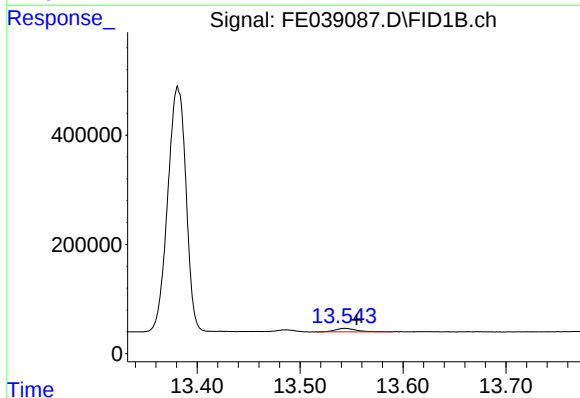


#11 n-Heneicosane (C21)

R.T.: 13.544 min
Delta R.T.: -0.011 min
Response: 90577
Conc: 0.64 ug/ml

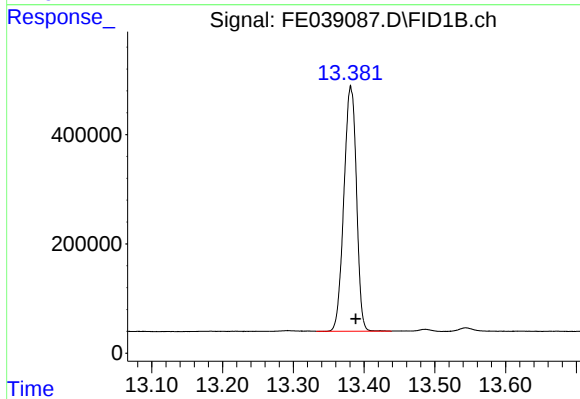

#12 1-chlorooctadecane (SURR)


R.T.: 13.381 min
Delta R.T.: -0.007 min
Response: 5518030
Conc: 45.70 ug/ml

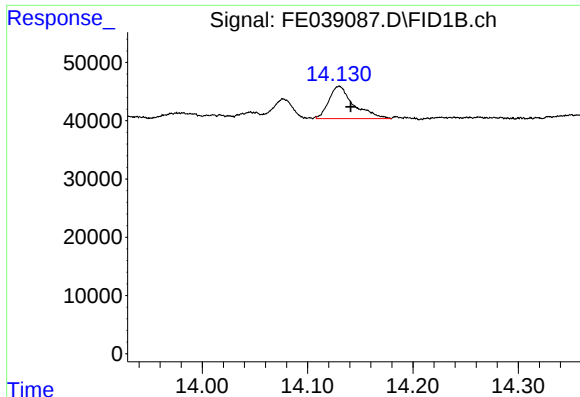

#13 n-Docosane (C22)


R.T.: 14.130 min
Delta R.T.: -0.011 min
Response: 90683
Conc: 0.65 ug/ml

Instrument :
FID_E
ClientSampleId :

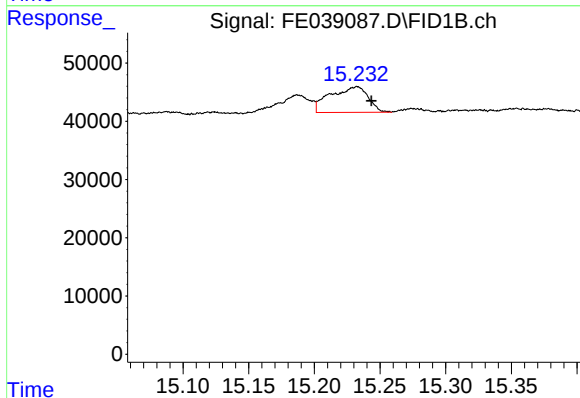


#14 n-Tetracosane (C24)

R.T.: 15.233 min
Delta R.T.: -0.011 min
Response: 88507
Conc: 0.64 ug/ml

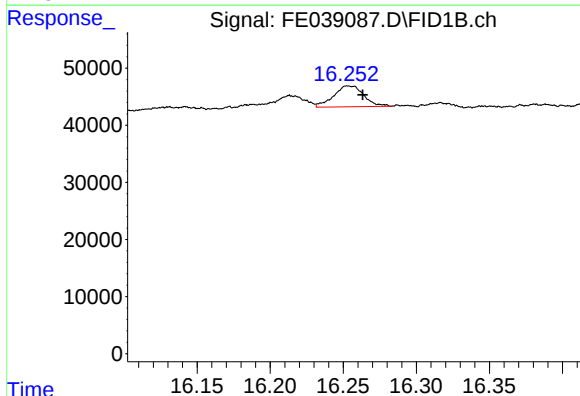


#15 n-Hexacosane (C26)

R.T.: 16.253 min
Delta R.T.: -0.010 min
Response: 52498
Conc: 0.39 ug/ml

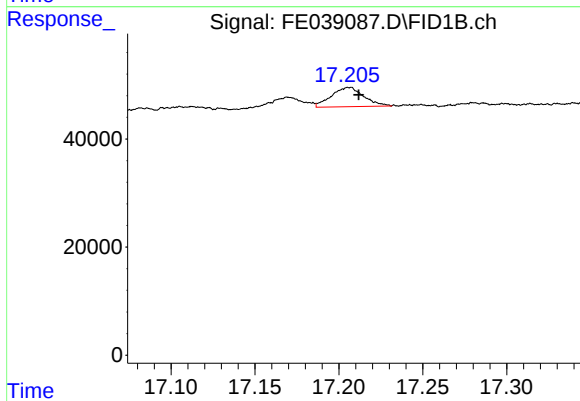

#16 n-Octacosane (C28)

R.T.: 17.206 min
Delta R.T.: -0.006 min
Response: 47902
Conc: 0.36 ug/ml

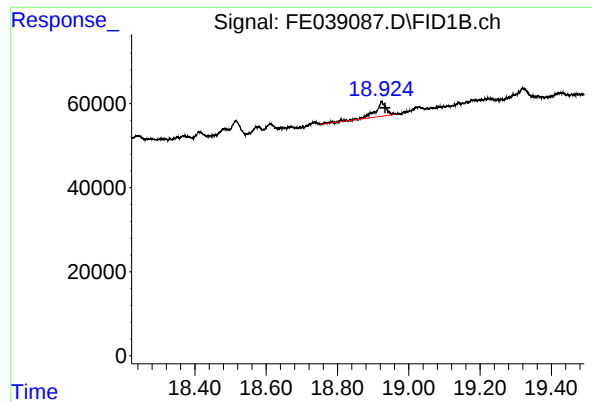

#18 n-Dotriacontane (C32)

R.T.: 18.924 min
Delta R.T.: -0.010 min
Response: 76052
Conc: 0.57 ug/ml

Instrument :

FID_E

ClientSampleId :