

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120522AL\
 Data File : FE039140.D
 Signal(s) : FID1B.ch
 Acq On : 06 Dec 2022 02:31
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:12:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

18) T	n-Dotriacontane (C32)	18.924	126030	0.945 ug/ml
19) T	n-Tetratriacontane (C34)	19.712	29068	0.220 ug/ml
20) T	n-Hexatriacontane (C36)	20.465	92504	0.720 ug/ml
21) T	n-Octatriacontane (C38)	21.200	246532	1.881 ug/ml
22) T	n-Tetracontane (C40)	22.123	93538	0.687 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120522AL\
Data File : FE039140.D
Signal(s) : FID1B.ch
Acq On : 06 Dec 2022 02:31
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:12:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

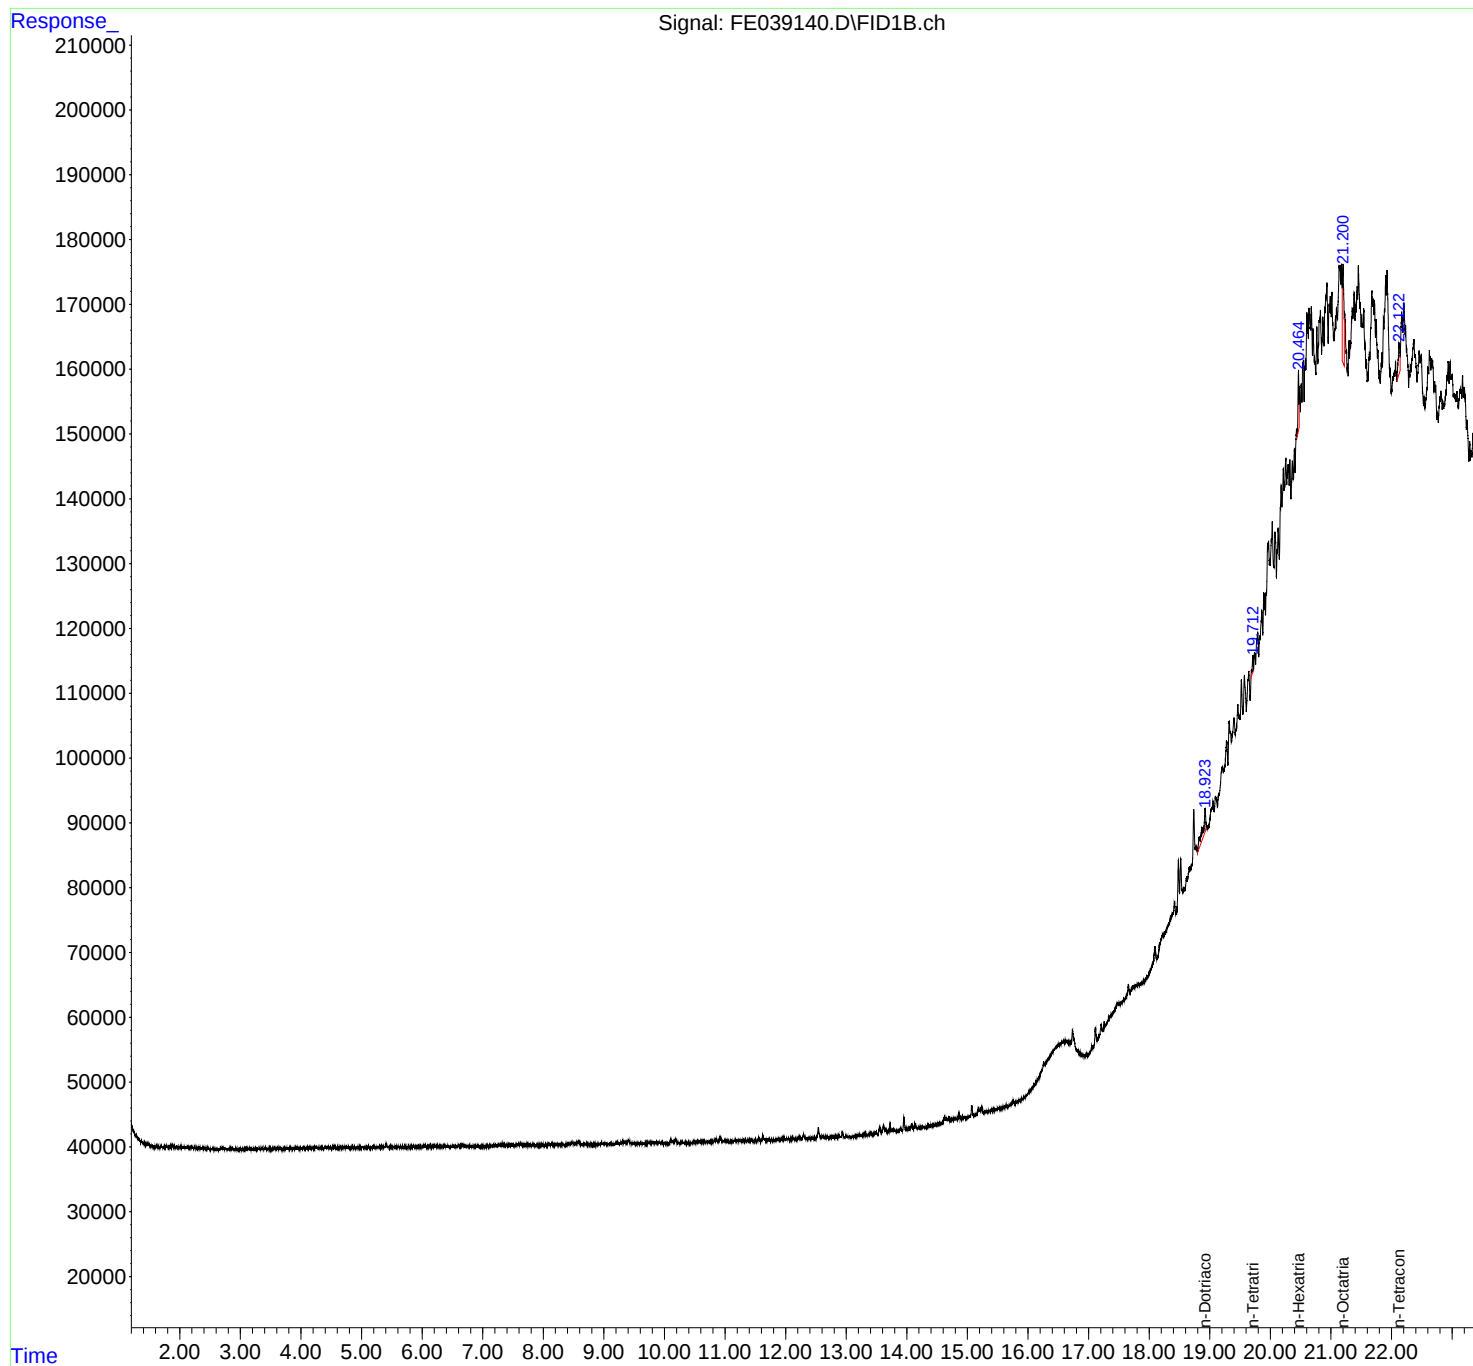


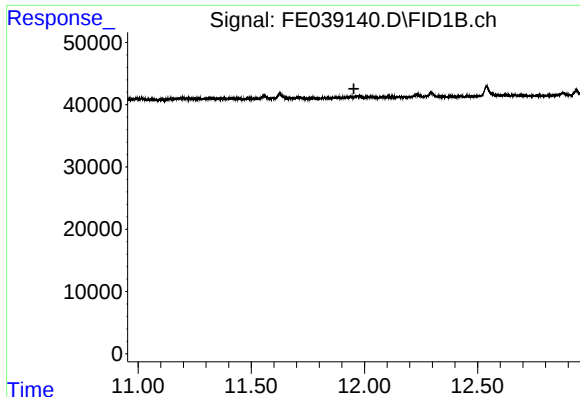

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.953 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

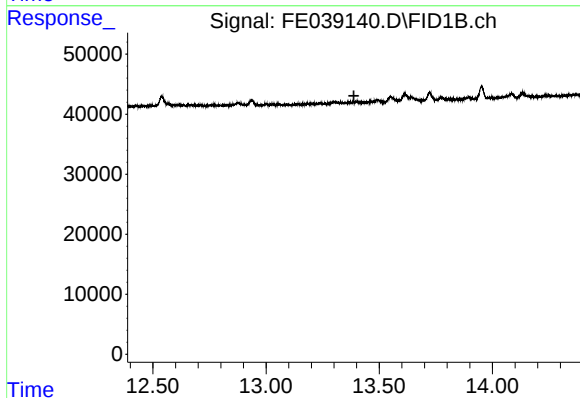


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.388 min
Response: 0
Conc: N.D.

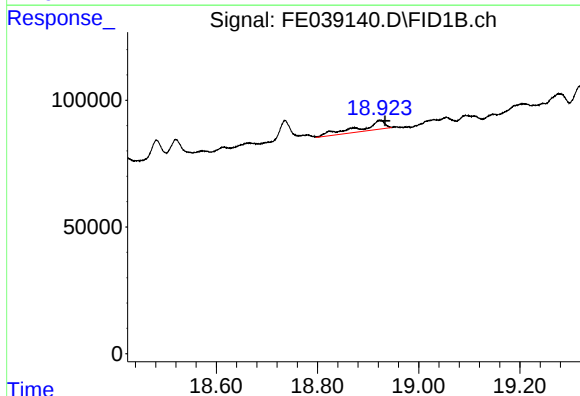


#18 n-Dotriacontane (C32)

R.T.: 18.924 min
Delta R.T.: -0.009 min
Response: 126030
Conc: 0.94 ug/ml

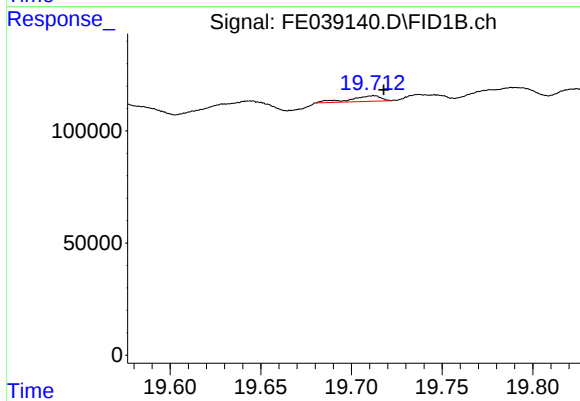

#19 n-Tetratriacontane (C34)


R.T.: 19.712 min
Delta R.T.: -0.006 min
Response: 29068
Conc: 0.22 ug/ml

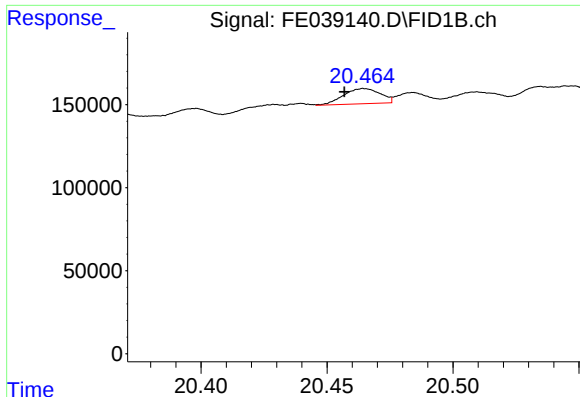

#20 n-Hexatriacontane (C36)


R.T.: 20.465 min
Delta R.T.: 0.008 min
Response: 92504
Conc: 0.72 ug/ml

Instrument :
FID_E
ClientSampleId :

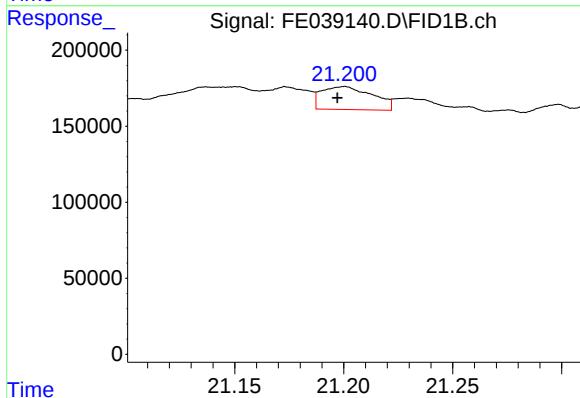

#21 n-Octatriacontane (C38)

R.T.: 21.200 min
Delta R.T.: 0.003 min
Response: 246532
Conc: 1.88 ug/ml

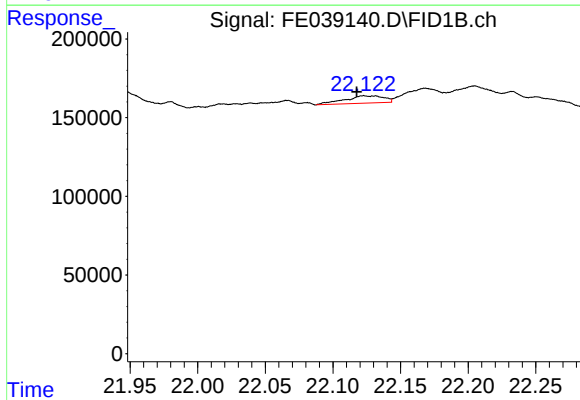

#22 n-Tetracontane (C40)

R.T.: 22.123 min
Delta R.T.: 0.005 min
Response: 93538
Conc: 0.69 ug/ml