

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE120524AL\  
 Data File : FE051542.D  
 Signal(s) : FID1B.ch  
 Acq On : 05 Dec 2024 08:11  
 Operator : YP\AJ  
 Sample : P5072-01DL 5X  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 MH-737DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 12/09/2024  
 Supervised By :Ankita Jodhani 12/09/2024

Integration File: autoint1.e  
 Quant Time: Dec 06 02:03:48 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 120224.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Dec 02 14:18:35 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.826 | 1198165    | 7.929 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 15.86%       |
| 12) S 1-chlorooctadecane (S... | 13.260 | 932455     | 8.344 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 16.69%       |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE120524AL\  
Data File : FE051542.D  
Signal(s) : FID1B.ch  
Acq On : 05 Dec 2024 08:11  
Operator : YP\AJ  
Sample : P5072-01DL 5X  
Misc :  
ALS Vial : 11 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
MH-737DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 12/09/2024  
Supervised By :Ankita Jodhani 12/09/2024

Integration File: autoint1.e  
Quant Time: Dec 06 02:03:48 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 120224.  
Quant Title : GC Extractables  
QLast Update : Mon Dec 02 14:18:35 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

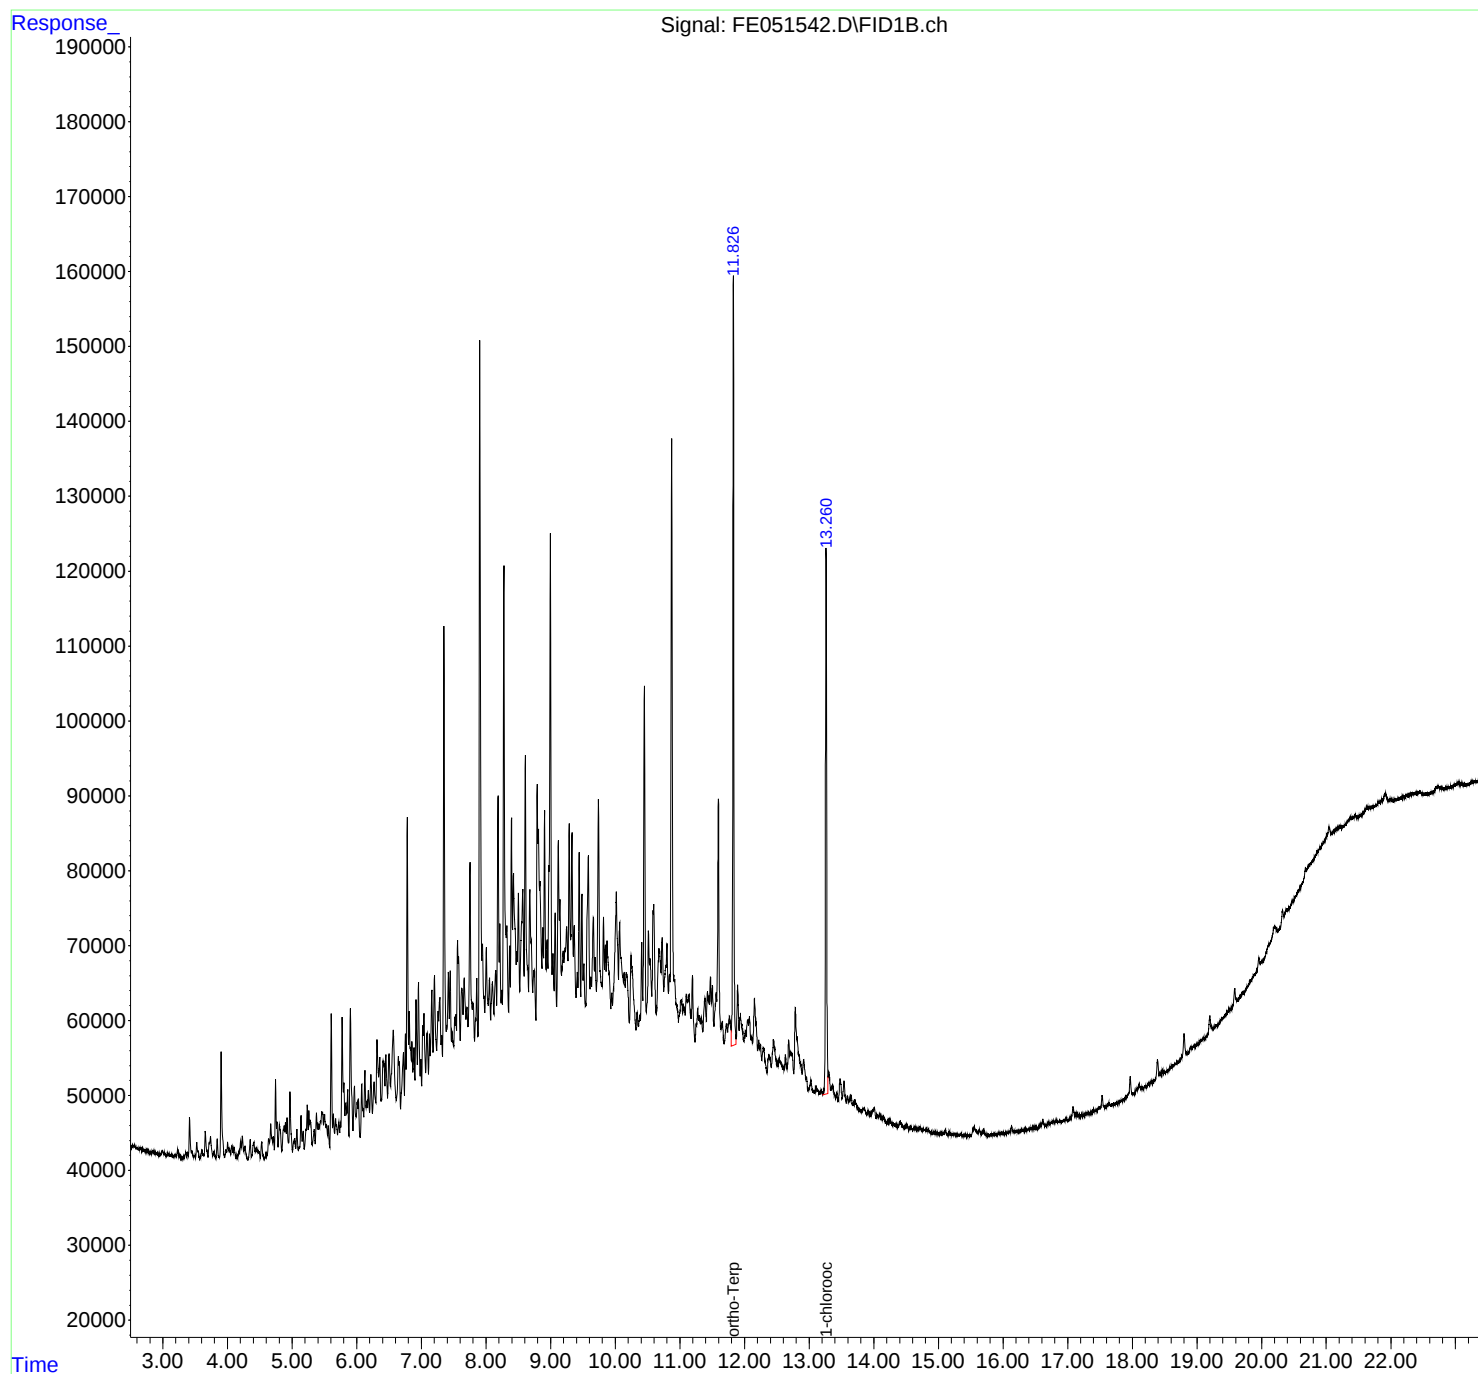

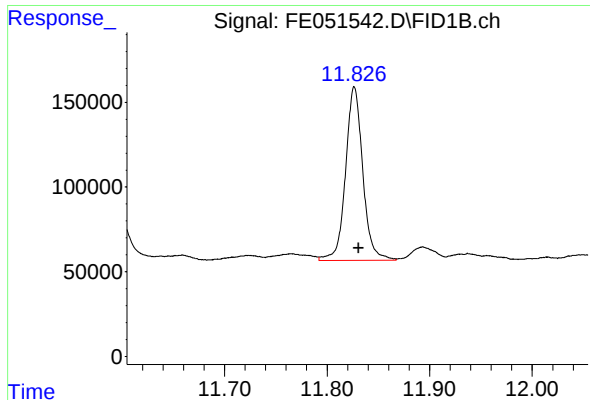


#9 ortho-Terphenyl (SURR)

R.T.: 11.826 min  
Delta R.T.: -0.005 min  
Response: 1198165  
Conc: 7.93 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
MH-737DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 12/09/2024  
Supervised By :Ankita Jodhani 12/09/2024

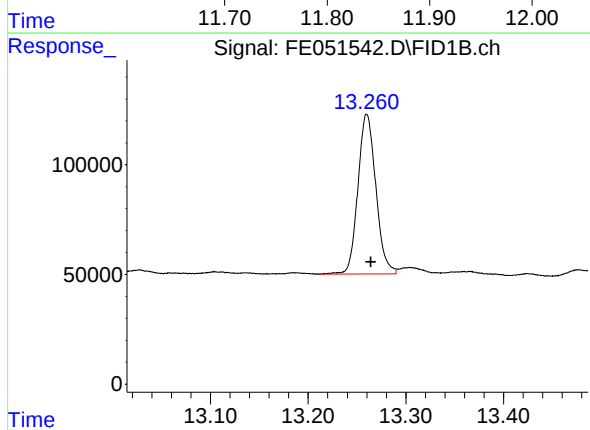

#12 1-chlorooctadecane (SURR)

R.T.: 13.260 min  
Delta R.T.: -0.005 min  
Response: 932455  
Conc: 8.34 ug/ml m