

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120525\
Data File : FB032396.D
Signal(s) : FID2B.CH
Acq On : 5 Dec 2025 18:34
Operator : YP/AJ
Sample : VBF1205S1
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibrat.e
Quant Time: Dec 05 22:59:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	432913	19.216 ng/ml
Target Compounds			
6) t Toluene	10.629	7627	0.167 ng/ml
8) t m-Xylene	13.191	8309	0.193 ng/ml
9) t O-Xylene	13.919	10412	0.252 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	21929	0.623 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120525\
Data File : FB032396.D
Signal(s) : FID2B.CH
Acq On : 5 Dec 2025 18:34
Operator : YP/AJ
Sample : VBF1205S1
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibrat.e
Quant Time: Dec 05 22:59:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

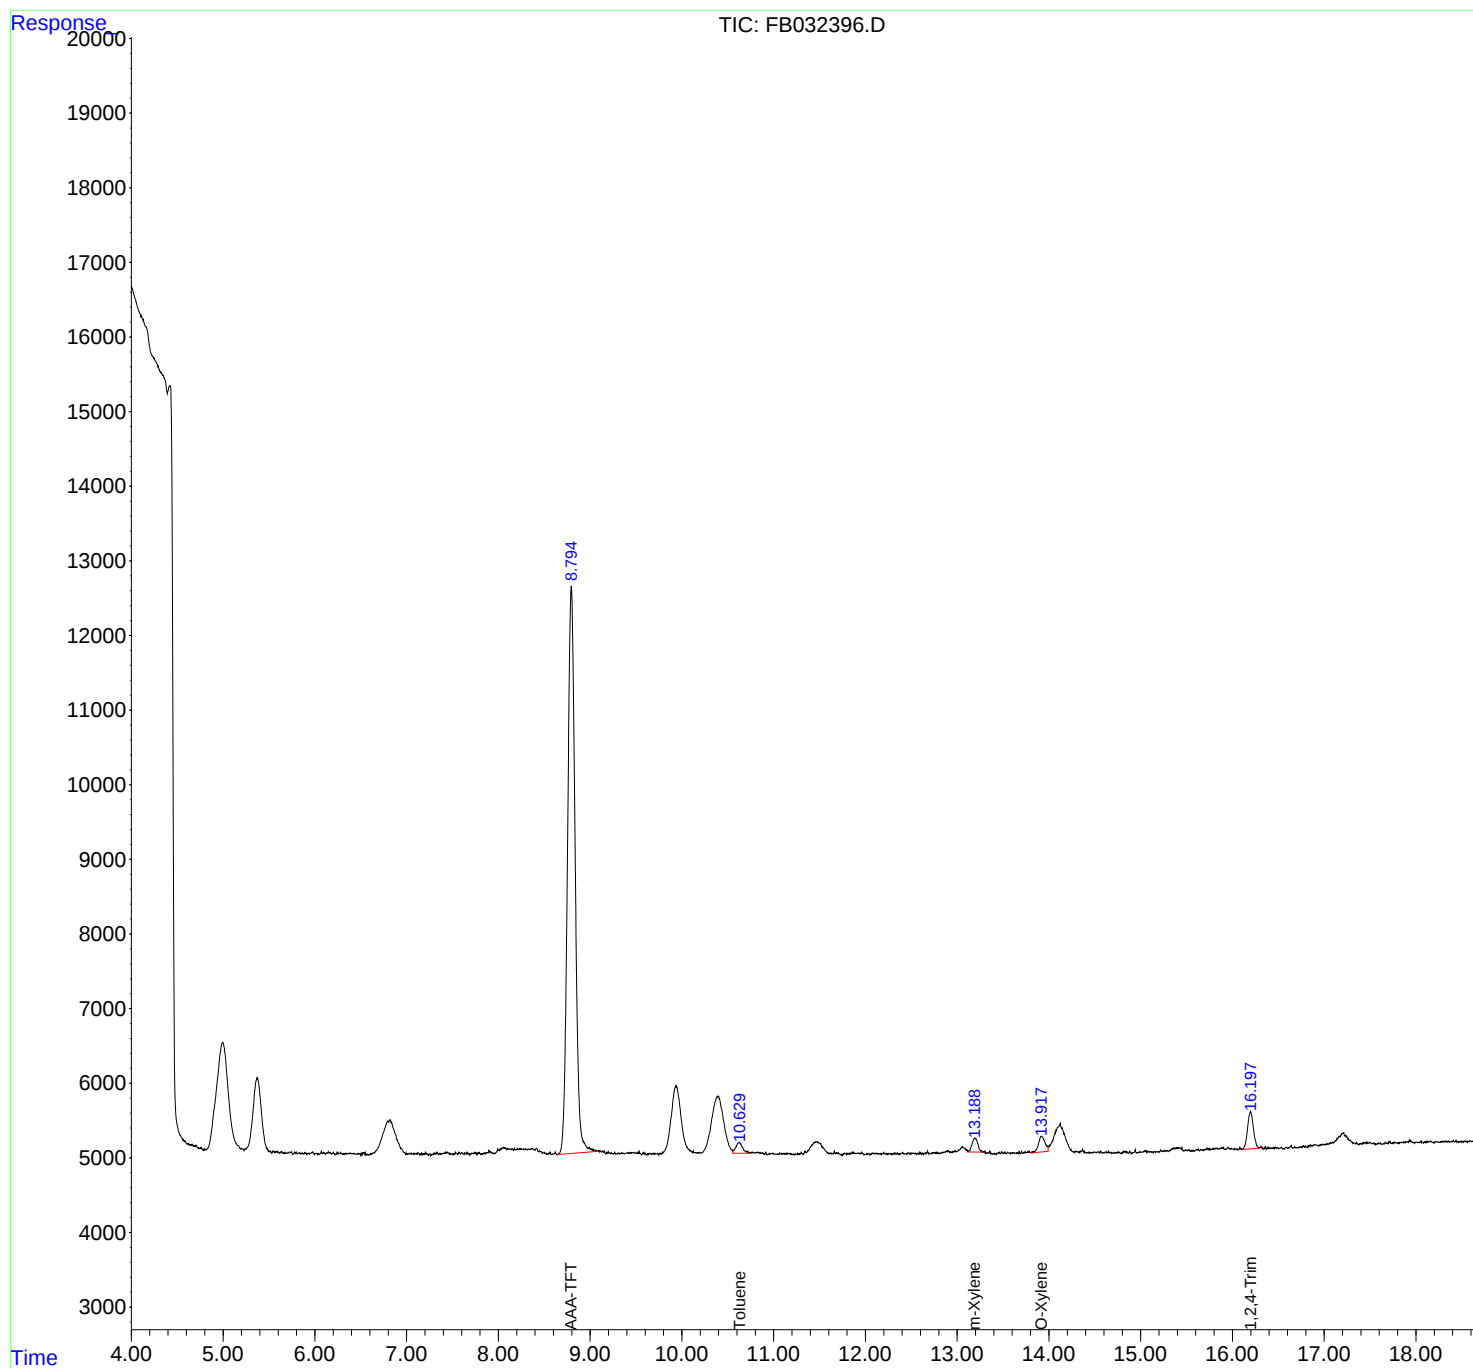


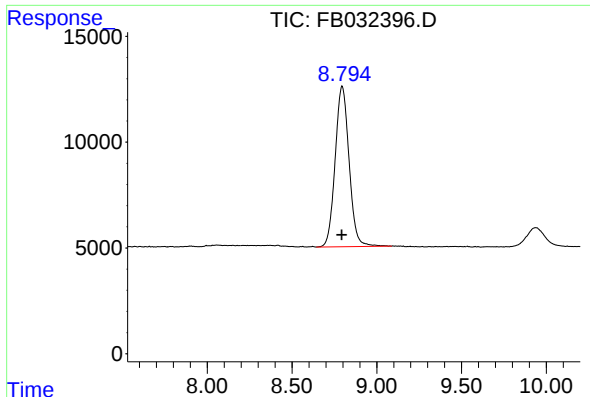

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.001 min
Response: 432913
Conc: 19.22 ng/ml

Instrument :
FID_E
ClientSampleId :

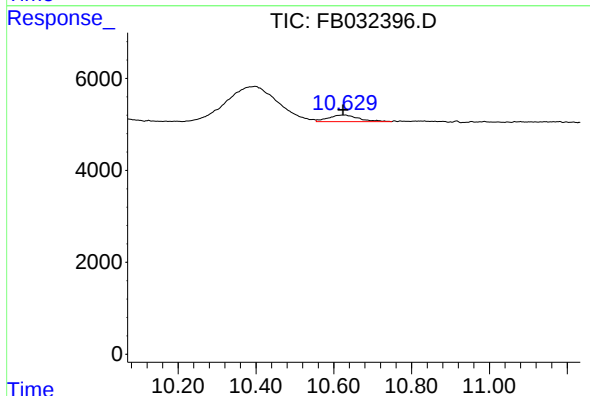


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.005 min
Response: 7627
Conc: 0.17 ng/ml

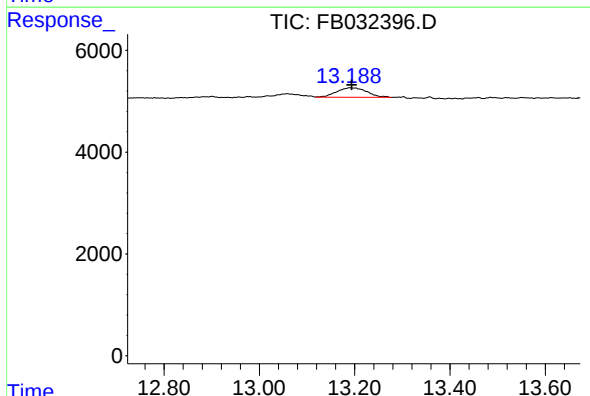


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: -0.002 min
Response: 8309
Conc: 0.19 ng/ml

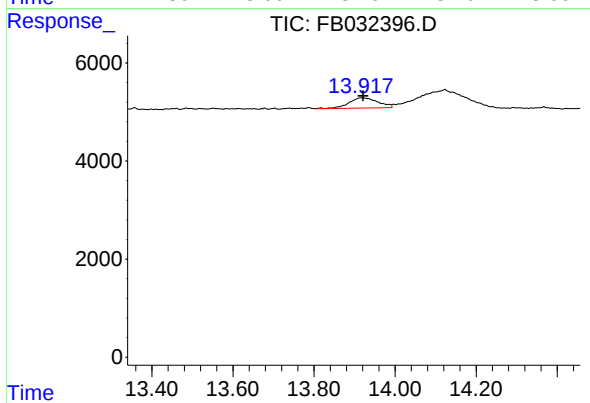

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.002 min
Response: 10412
Conc: 0.25 ng/ml

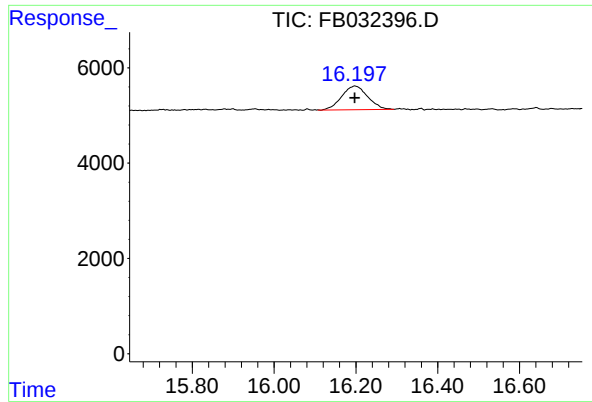

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.001 min
Response: 21929
Conc: 0.62 ng/ml

Instrument :

FID_E

ClientSampleId :