

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120619\
 Data File : FE030974.D
 Signal(s) : FID1B.CH
 Acq On : 06 Dec 2019 14:23
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 21:49:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE112619.M
 Quant Title :
 QLast Update : Tue Nov 26 14:51:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.400	8664376	23.601 ug/ml
12)	N-OCTACOSANE	16.844	8359654	24.613 ug/ml
13)	N-TRIACONTANE	17.727	974545	2.906 ug/ml
14)	N-DOTRIACONTANE	18.562	1050733	3.249 ug/ml
15)	N-TETRATRIACONTANE	19.346	877917	2.795 ug/ml
16)	N-HEXATRIACONTANE	20.089	1596431	5.368 ug/ml
17)	N-OCTATRIACONTANE	20.827	412780	1.490 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120619\
Data File : FE030974.D
Signal(s) : FID1B.CH
Acq On : 06 Dec 2019 14:23
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 21:49:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE112619.M
Quant Title :
QLast Update : Tue Nov 26 14:51:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

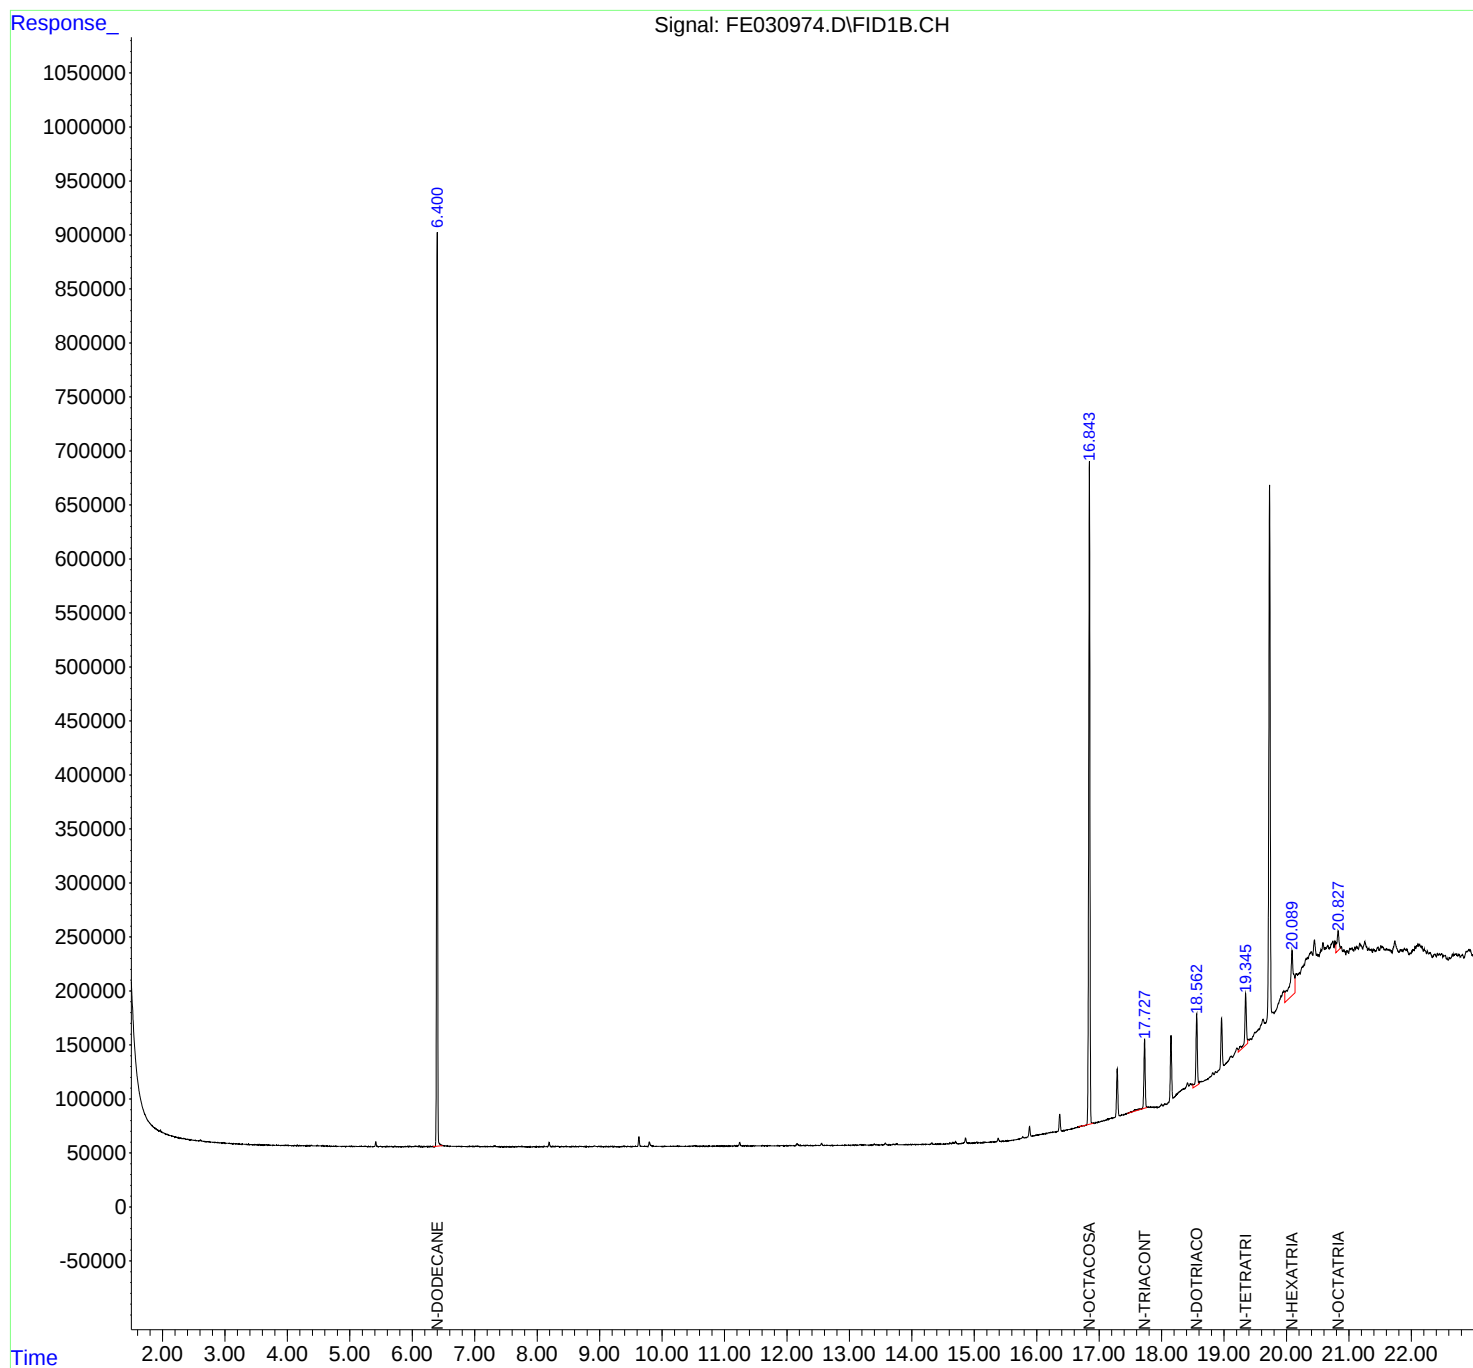


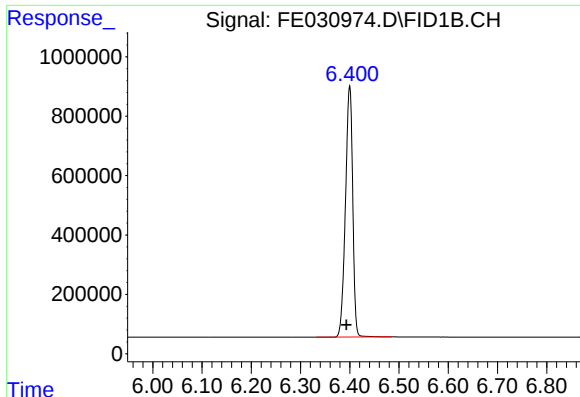

#3 N-DODECANE


R.T.: 6.400 min
Delta R.T.: 0.006 min
Response: 8664376
Conc: 23.60 ug/ml

Instrument :
FID_E
ClientSampleId :

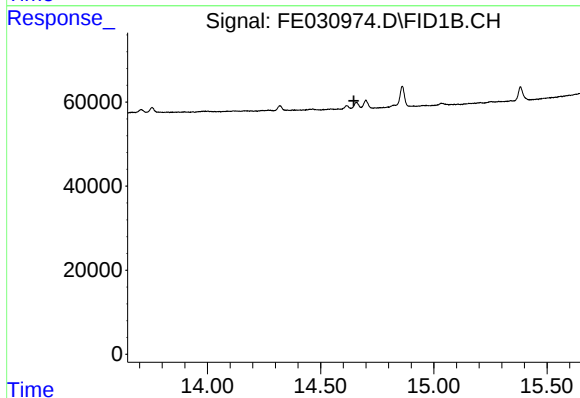


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.647 min
Response: 0
Conc: N.D.

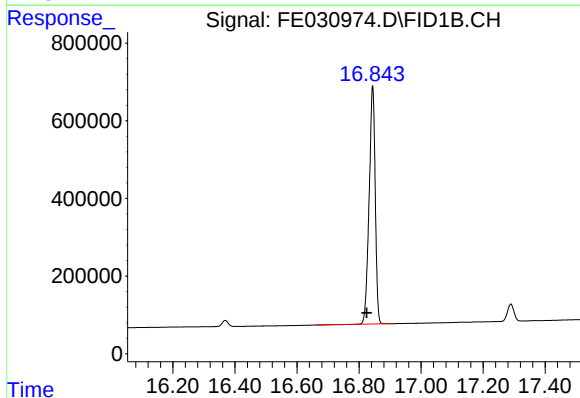


#12 N-OCTACOSANE

R.T.: 16.844 min
Delta R.T.: 0.018 min
Response: 8359654
Conc: 24.61 ug/ml

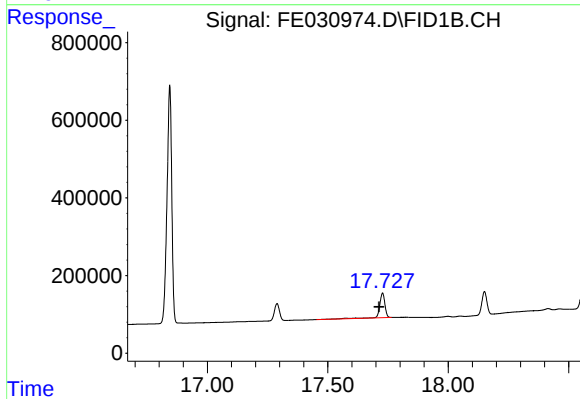

#13 N-TRIACONTANE


R.T.: 17.727 min
Delta R.T.: 0.014 min
Response: 974545
Conc: 2.91 ug/ml

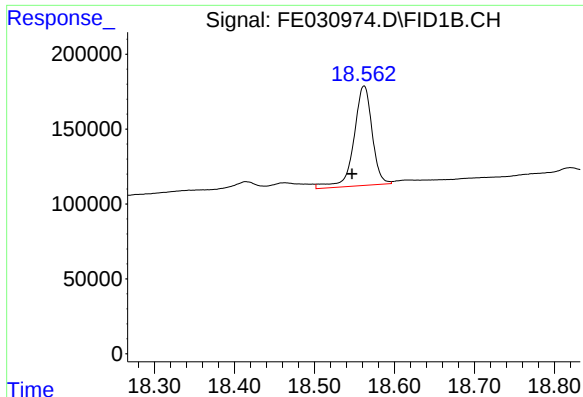

#14 N-DOTRIACONTANE


R.T.: 18.562 min
Delta R.T.: 0.015 min
Response: 1050733
Conc: 3.25 ug/ml

Instrument :
FID_E
ClientSampleId :

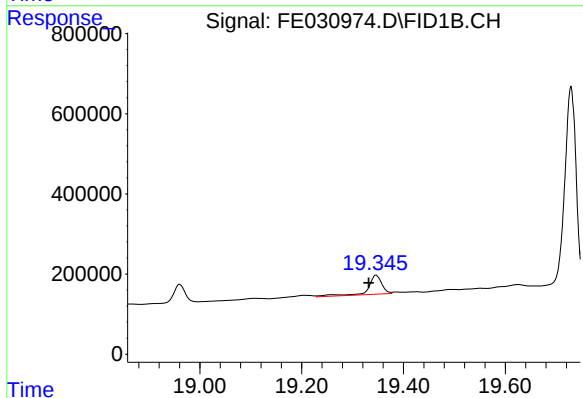


#15 N-TETRATRIACONTANE

R.T.: 19.346 min
Delta R.T.: 0.014 min
Response: 877917
Conc: 2.80 ug/ml

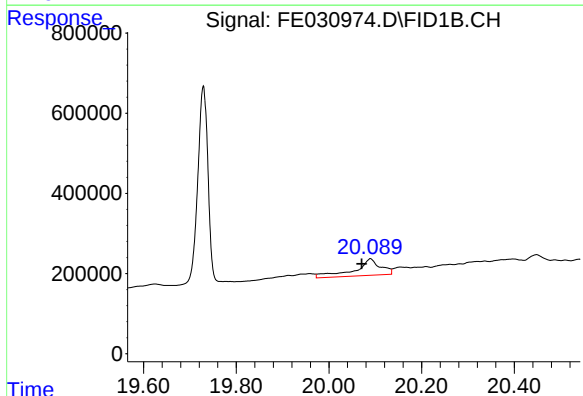

#16 N-HEXATRIACONTANE

R.T.: 20.089 min
Delta R.T.: 0.018 min
Response: 1596431
Conc: 5.37 ug/ml

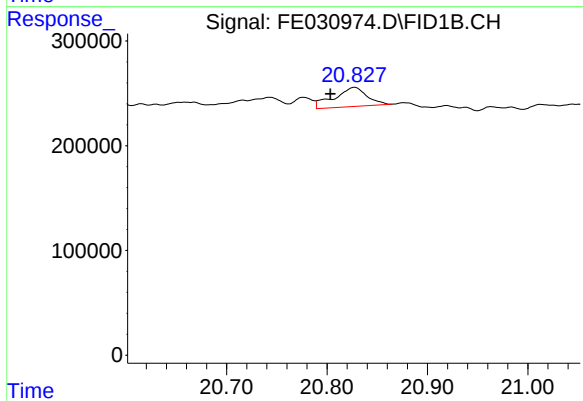

#17 N-OCTATRIACONTANE

R.T.: 20.827 min
Delta R.T.: 0.024 min
Response: 412780
Conc: 1.49 ug/ml