

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120622AL\
 Data File : FE039153.D
 Signal(s) : FID1B.ch
 Acq On : 06 Dec 2022 14:48
 Operator : YP\AJ
 Sample : N5863-01D
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 07 04:25:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.940	401773	2.568 ug/ml
Spiked Amount 50.000		Recovery =	5.14%
12) S 1-chlorooctadecane (S...	13.379	4273169	35.392 ug/ml
Spiked Amount 50.000		Recovery =	70.78%
Target Compounds			
4) T n-Dodecane (C12)	6.750	74575	0.529 ug/ml
6) T n-Tetradecane (C14)	8.575	90225	0.632 ug/ml
7) T n-Hexadecane (C16)	10.181	52812	0.361 ug/ml
17) T n-Tricontane (C30)	18.089	51931	0.393 ug/ml
18) T n-Dotriacontane (C32)	18.921	55694	0.418 ug/ml
21) T n-Octatriacontane (C38)	21.184	65939	0.503 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120622AL\
Data File : FE039153.D
Signal(s) : FID1B.ch
Acq On : 06 Dec 2022 14:48
Operator : YP\AJ
Sample : N5863-01D
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 07 04:25:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

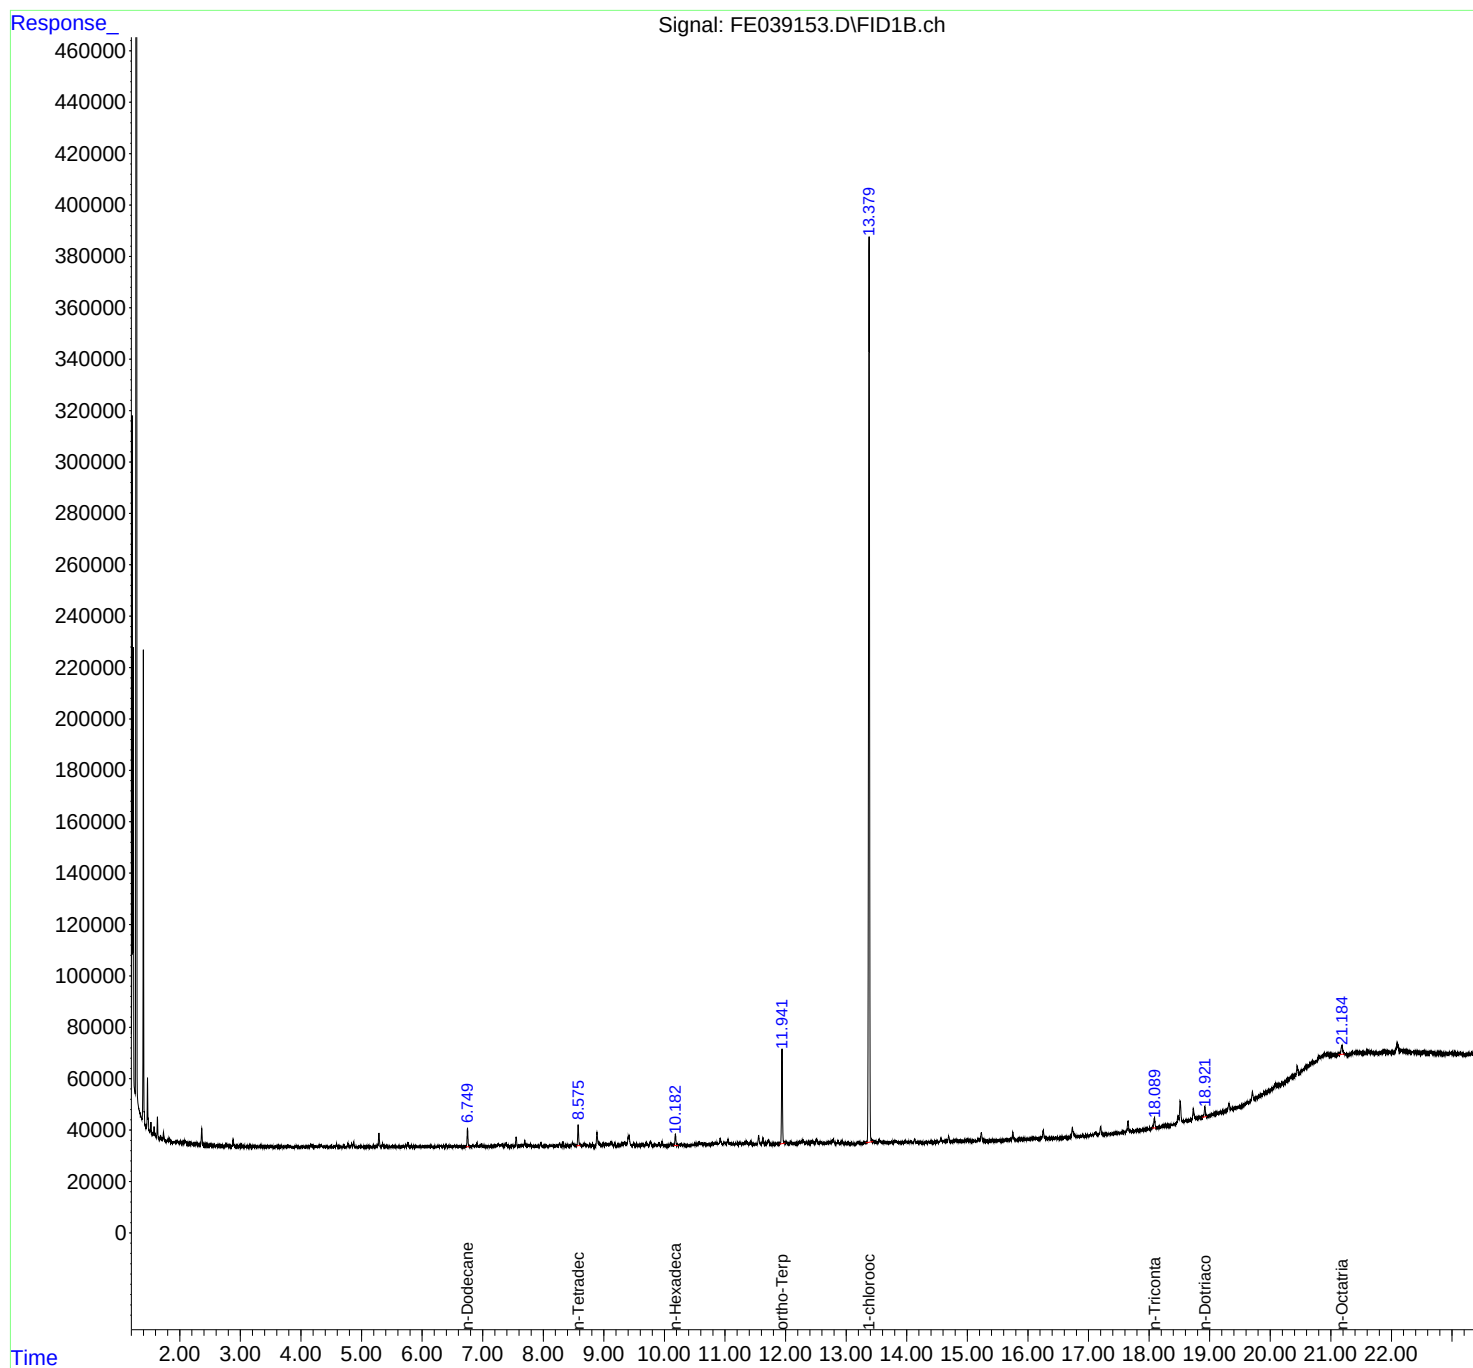


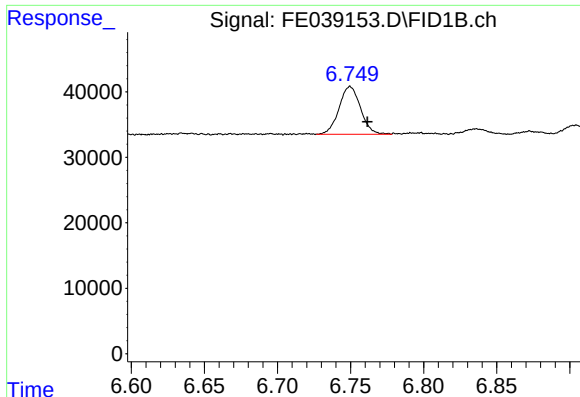

#4 n-Dodecane (C12)


R.T.: 6.750 min
Delta R.T.: -0.012 min
Response: 74575
Conc: 0.53 ug/ml

Instrument :
FID_E
ClientSampleId :

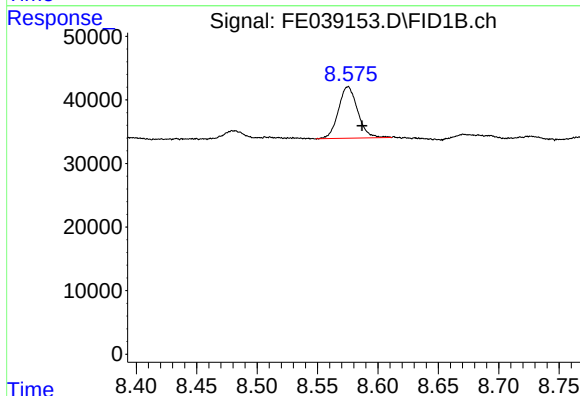


#6 n-Tetradecane (C14)

R.T.: 8.575 min
Delta R.T.: -0.012 min
Response: 90225
Conc: 0.63 ug/ml

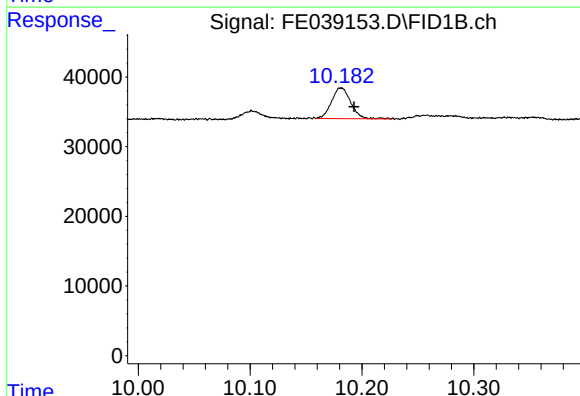


#7 n-Hexadecane (C16)

R.T.: 10.181 min
Delta R.T.: -0.011 min
Response: 52812
Conc: 0.36 ug/ml

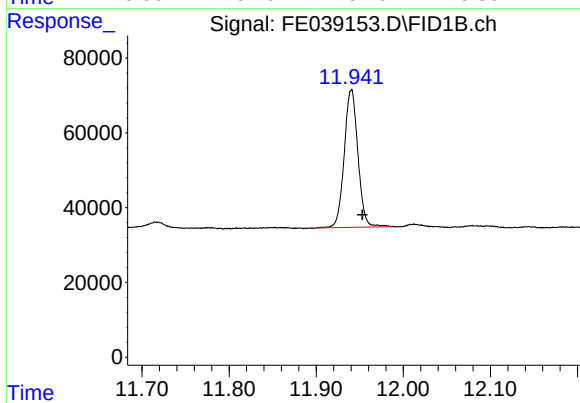

#9 ortho-Terphenyl (SURR)


R.T.: 11.940 min
Delta R.T.: -0.013 min
Response: 401773
Conc: 2.57 ug/ml

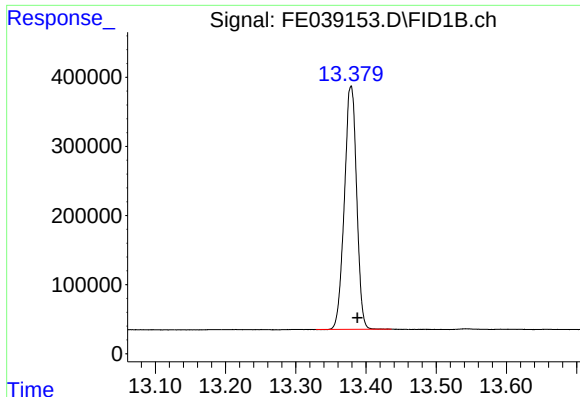

#12 1-chlorooctadecane (SURR)


R.T.: 13.379 min
Delta R.T.: -0.009 min
Response: 4273169
Conc: 35.39 ug/ml

Instrument :
FID_E
ClientSampleId :

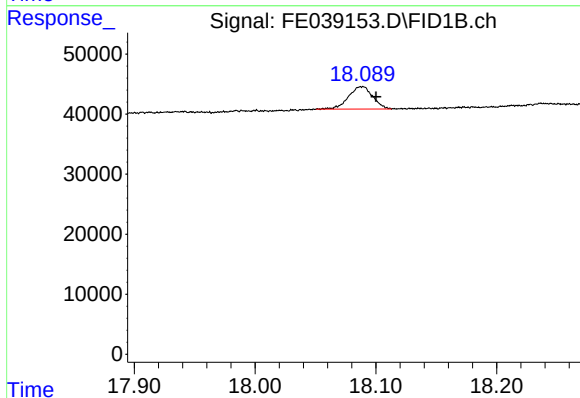


#17 n-Tricontane (C30)

R.T.: 18.089 min
Delta R.T.: -0.012 min
Response: 51931
Conc: 0.39 ug/ml

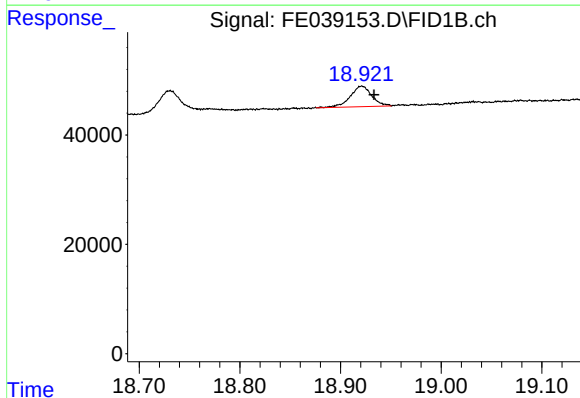

#18 n-Dotriacontane (C32)

R.T.: 18.921 min
Delta R.T.: -0.012 min
Response: 55694
Conc: 0.42 ug/ml

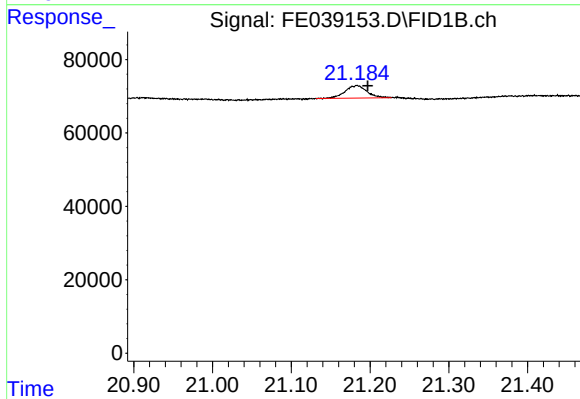

#21 n-Octatriacontane (C38)

R.T.: 21.184 min
Delta R.T.: -0.014 min
Response: 65939
Conc: 0.50 ug/ml