

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE120623AL\  
 Data File : FE045676.D  
 Signal(s) : FID1B.ch  
 Acq On : 06 Dec 2023 12:12  
 Operator : YP\AJ  
 Sample : 05620-01DL 5X  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 OILY-WATER-TOTEDL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 12/07/2023  
 Supervised By :Ankita Jodhani 12/07/2023

Integration File: autoint1.e  
 Quant Time: Dec 07 00:11:15 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 113023.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Nov 30 12:25:07 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 13.305 | 735620     | 4.675 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 9.35%        |
| Target Compounds               |        |            |              |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE120623AL\  
Data File : FE045676.D  
Signal(s) : FID1B.ch  
Acq On : 06 Dec 2023 12:12  
Operator : YP\AJ  
Sample : 05620-01DL 5X  
Misc :  
ALS Vial : 16 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
OILY-WATER-TOTEDL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 12/07/2023  
Supervised By :Ankita Jodhani 12/07/2023

Integration File: autoint1.e  
Quant Time: Dec 07 00:11:15 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 113023.M  
Quant Title : GC Extractables  
QLast Update : Thu Nov 30 12:25:07 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

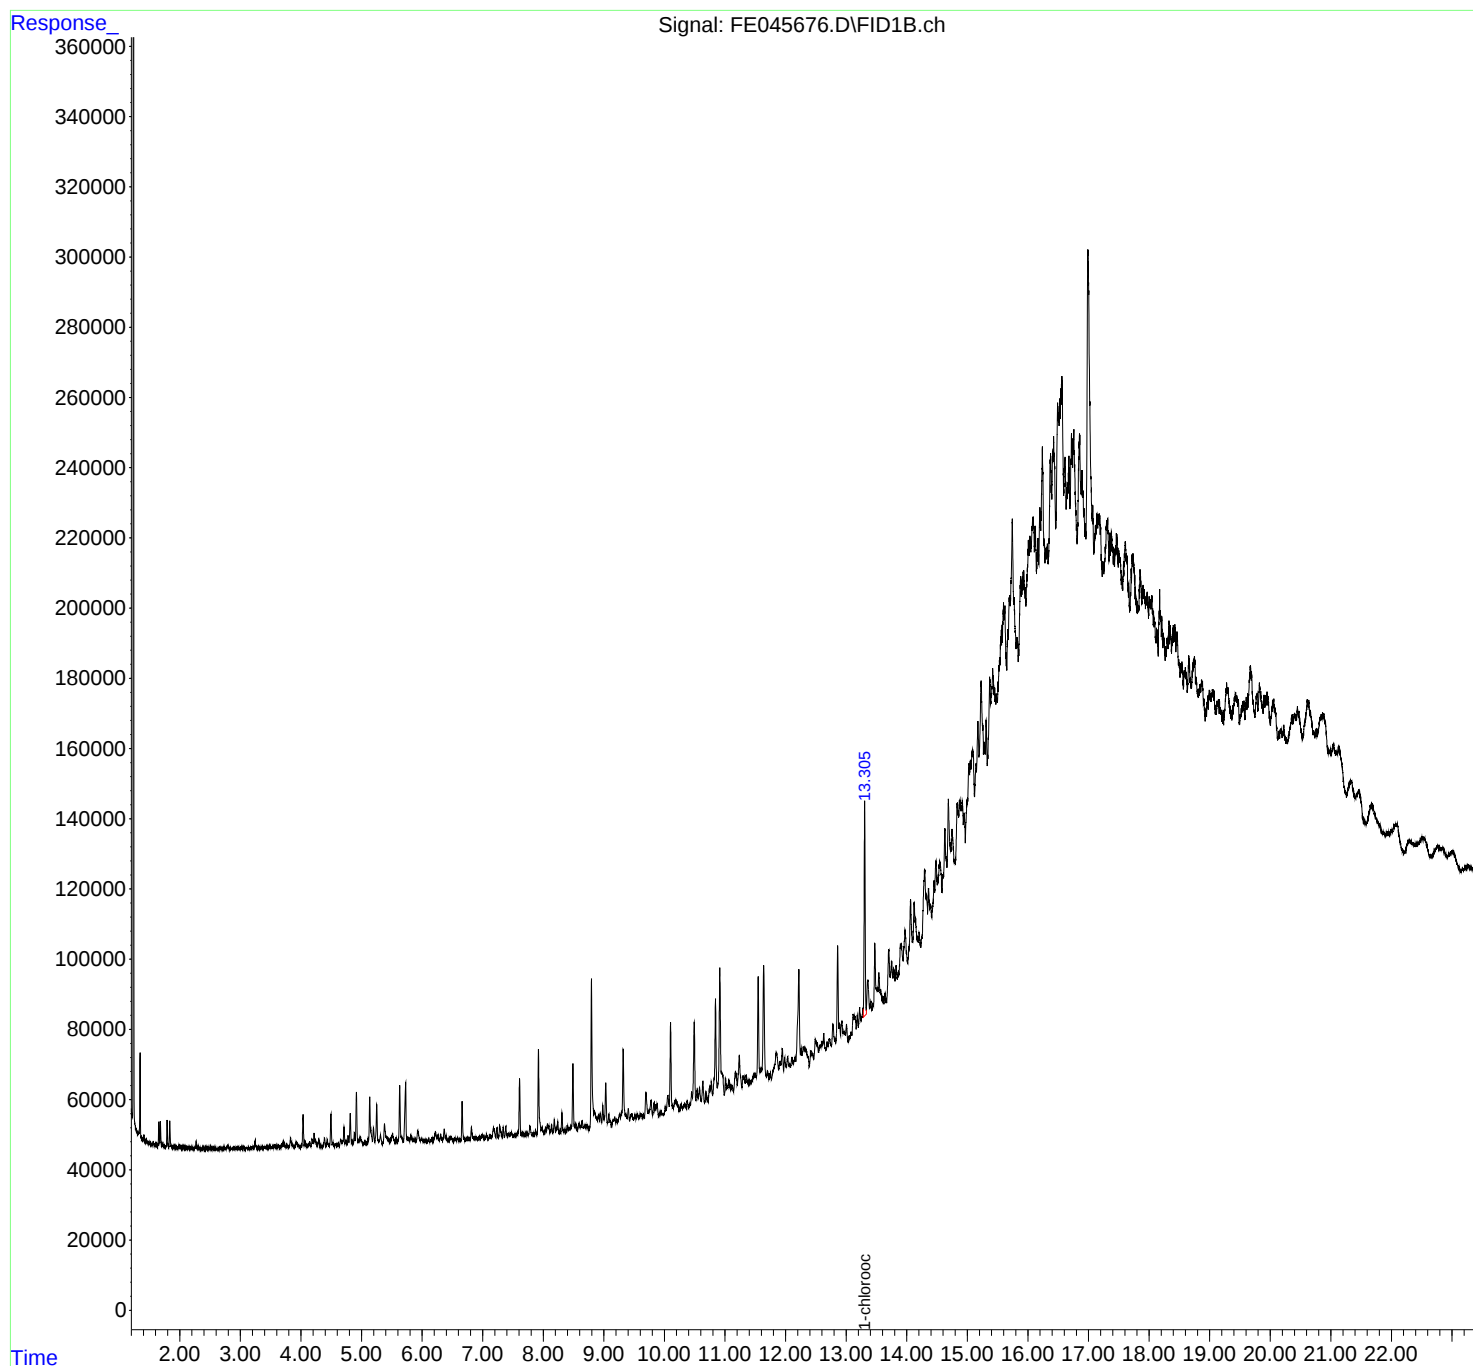

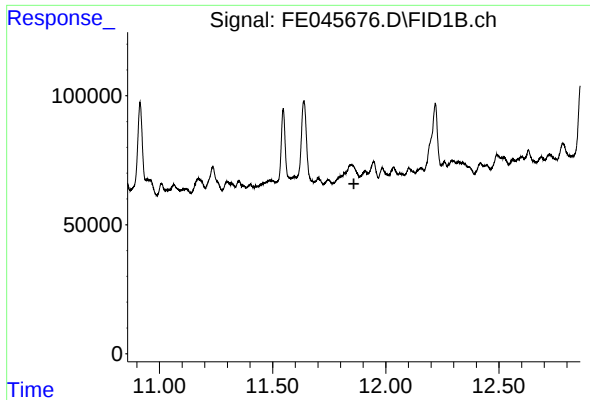


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.859 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :  
OILY-WATER-TOTEDL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 12/07/2023  
Supervised By :Ankita Jodhani 12/07/2023

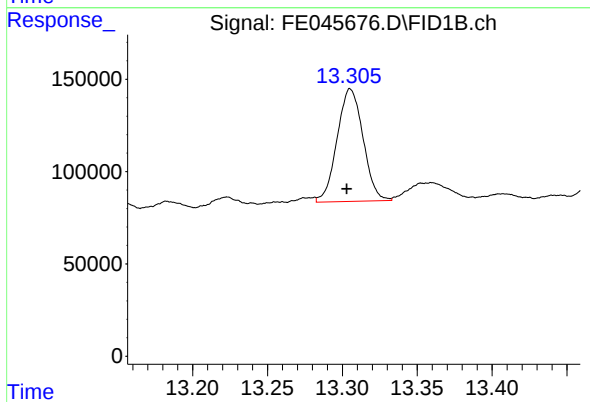

#12 1-chlorooctadecane (SURR)

R.T.: 13.305 min  
Delta R.T.: 0.002 min  
Response: 735620  
Conc: 4.68 ug/ml m