

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120718\
 Data File : FE029288.D
 Signal(s) : FID1B.CH
 Acq On : 07 Dec 2018 20:25
 Operator : AJ\SJ
 Sample : 1760 TRPH STD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File: sample.e
 Quant Time: Dec 07 23:44:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE120718.M
 Quant Title :
 QLast Update : Fri Dec 07 23:39:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.839	3641726	19.479 ug/ml
Target Compounds			
1) N-OCTANE	2.522	26381163	156.982 ug/ml
2) N-NONANE	3.519	26525028	156.554 ug/ml
3) N-DECANE	4.584	39483180	155.604 ug/ml
4) N-UNDECANE	5.618	41371092	233.453 ug/ml
5) N-DODECANE	6.601	41215995	234.612 ug/ml
6) N-TETRADECANE	8.404	40904446	234.758 ug/ml
7) N-HEXADECANE	10.007	35206162	196.201 ug/ml
8) N-OCTADECANE	11.440	17692019	97.786 ug/ml
9) N-EICOSANE	12.742	6975195	38.573 ug/ml
10) N-TETRACOSANE	15.049	7102190	38.920 ug/ml
11) N-OCTACOSANE	17.020	3523274	19.371 ug/ml
12) N-DOTRIACONTANE	18.743	3428302	19.484 ug/ml
14) N-HEXATRIACONTANE	20.268	3402608	19.641 ug/ml
15) N-TETRACONTANE	21.998	3103966	20.377 ug/ml
16) N-TETRATETRAOCTANE	24.927	2474289	21.528 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120718\
Data File : FE029288.D
Signal(s) : FID1B.CH
Acq On : 07 Dec 2018 20:25
Operator : AJ\SJ
Sample : 1760 TRPH STD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File: sample.e
Quant Time: Dec 07 23:44:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE120718.M
Quant Title :
QLast Update : Fri Dec 07 23:39:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

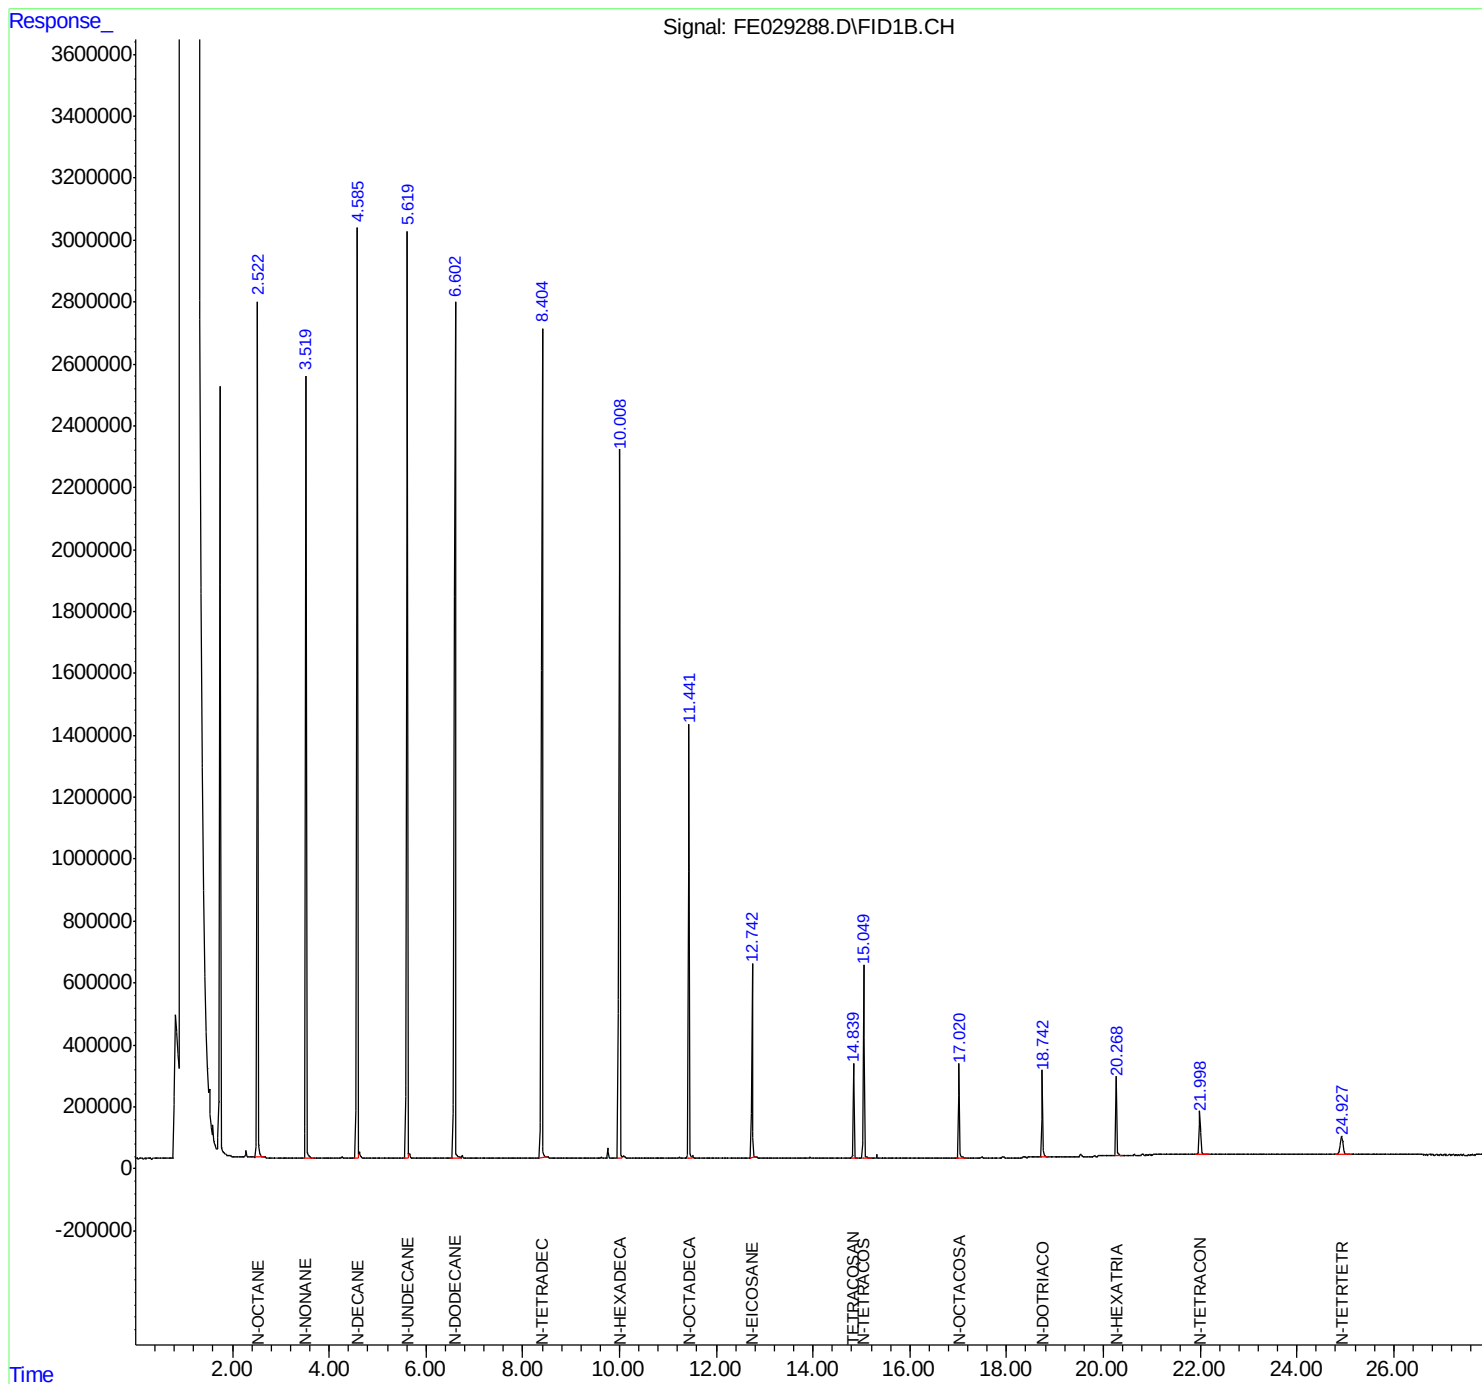

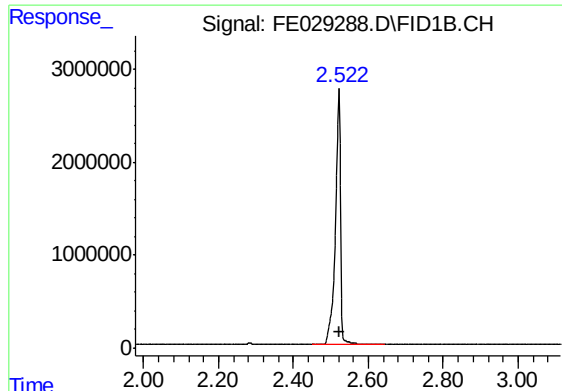


#1 N-OCTANE

R.T.: 2.522 min
Delta R.T.: 0.000 min
Response: 26381163
Conc: 156.98 ug/ml

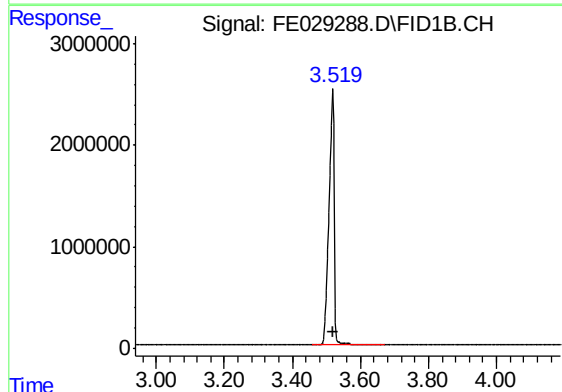


#2 N-NONANE

R.T.: 3.519 min
Delta R.T.: 0.000 min
Response: 26525028
Conc: 156.55 ug/ml

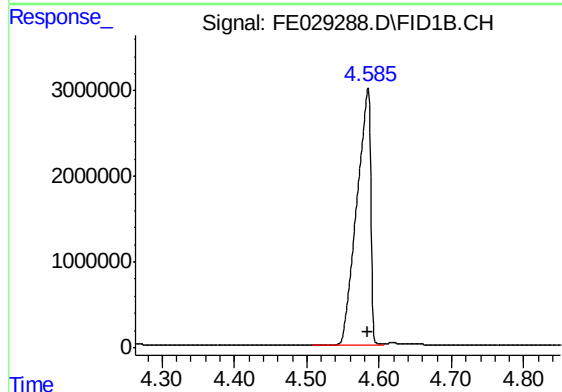


#3 N-DECANE

R.T.: 4.584 min
Delta R.T.: 0.000 min
Response: 39483180
Conc: 155.60 ug/ml

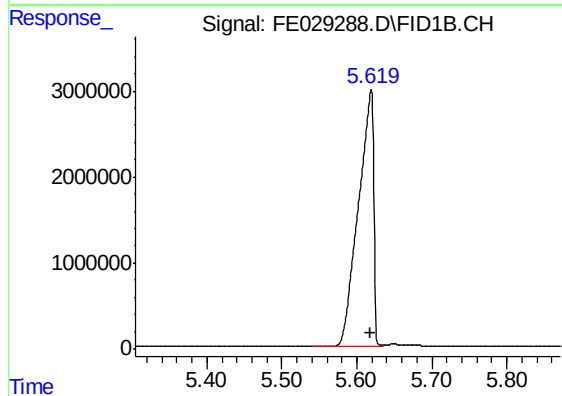


#4 N-UNDECANE

R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 41371092
Conc: 233.45 ug/ml

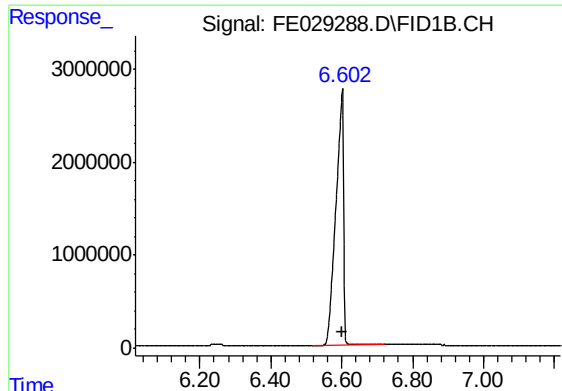


#5 N-DODECANE

R.T.: 6.601 min
Delta R.T.: 0.000 min
Response: 41215995
Conc: 234.61 ug/ml

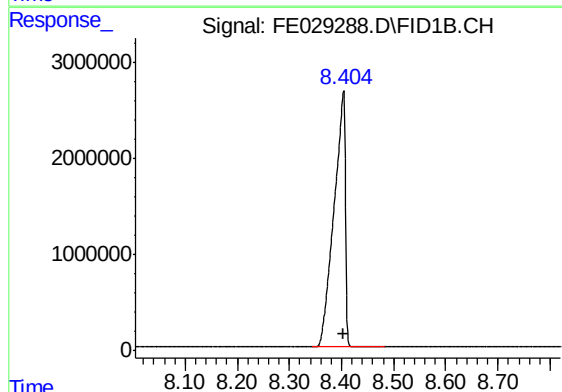


#6 N-TETRADECANE

R.T.: 8.404 min
Delta R.T.: 0.000 min
Response: 40904446
Conc: 234.76 ug/ml

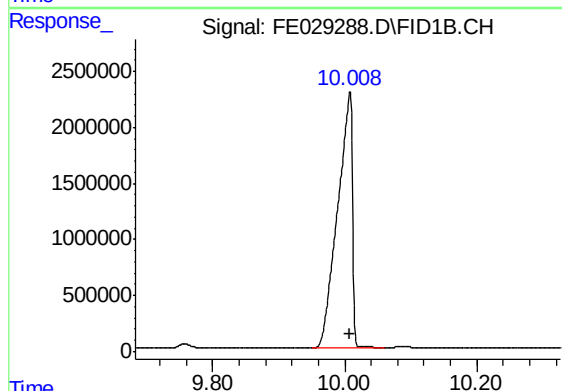


#7 N-HEXADECANE

R.T.: 10.007 min
Delta R.T.: 0.000 min
Response: 35206162
Conc: 196.20 ug/ml

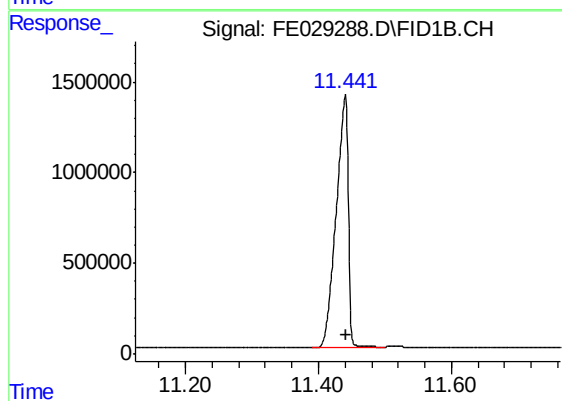


#8 N-OCTADECANE

R.T.: 11.440 min
Delta R.T.: 0.000 min
Response: 17692019
Conc: 97.79 ug/ml

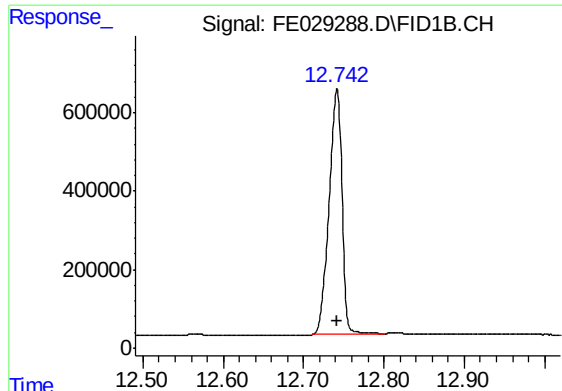


#9 N-EICOSANE

R.T.: 12.742 min
Delta R.T.: 0.000 min
Response: 6975195
Conc: 38.57 ug/ml

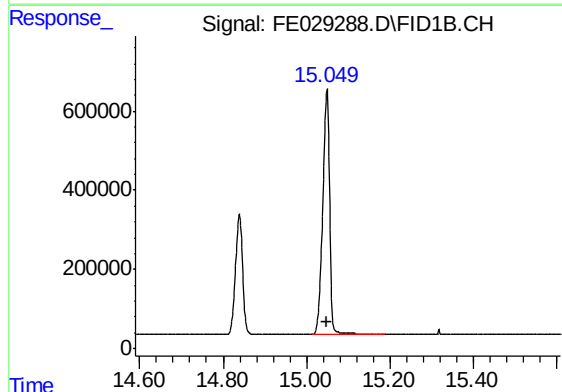


#10 N-TETRACOSANE

R.T.: 15.049 min
Delta R.T.: 0.000 min
Response: 7102190
Conc: 38.92 ug/ml

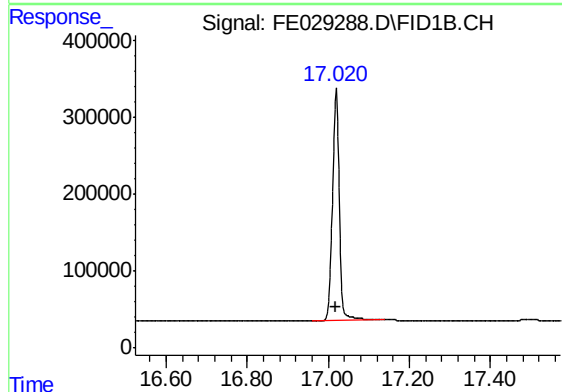


#11 N-OCTACOSANE

R.T.: 17.020 min
Delta R.T.: 0.000 min
Response: 3523274
Conc: 19.37 ug/ml

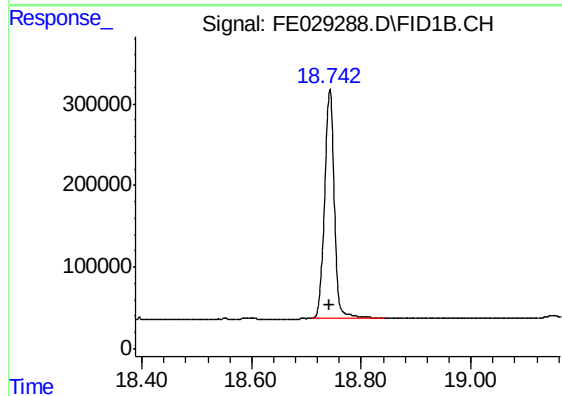


#12 N-DOTRIACONTANE

R.T.: 18.743 min
Delta R.T.: 0.000 min
Response: 3428302
Conc: 19.48 ug/ml

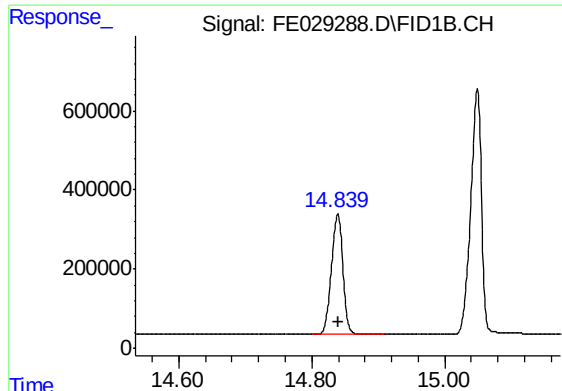


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.839 min
Delta R.T.: 0.000 min
Response: 3641726
Conc: 19.48 ug/ml

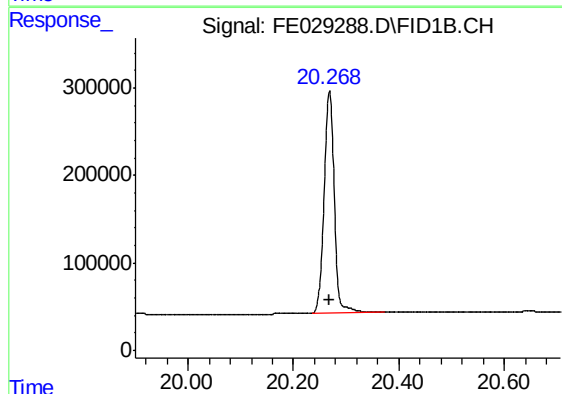


#14 N-HEXATRIACONTANE

R.T.: 20.268 min
Delta R.T.: 0.000 min
Response: 3402608
Conc: 19.64 ug/ml

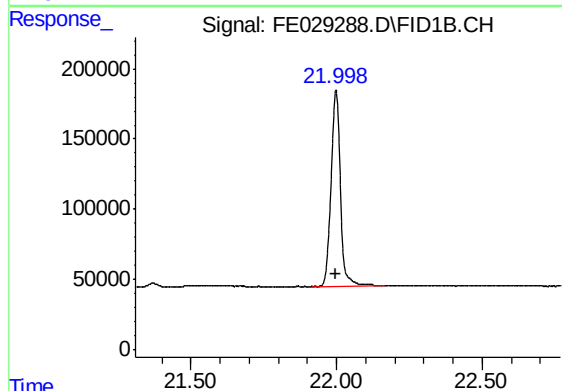

#15 N-TETRACONTANE

R.T.: 21.998 min
Delta R.T.: 0.000 min
Response: 3103966
Conc: 20.38 ug/ml

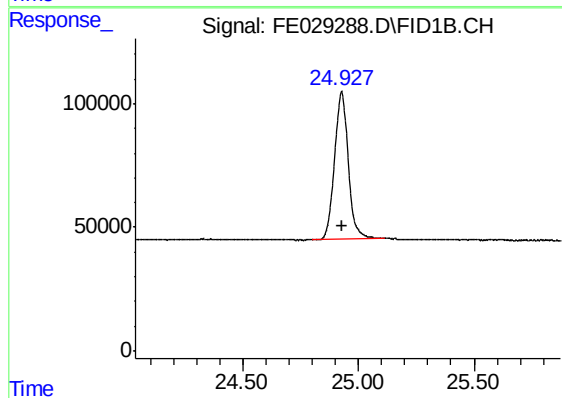

#16 N-TETRTETRACOOCTANE

R.T.: 24.927 min
Delta R.T.: 0.000 min
Response: 2474289
Conc: 21.53 ug/ml