

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120919\
Data File : FE030985.D
Signal(s) : FID1B.CH
Acq On : 09 Dec 2019 9:44
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 10 00:25:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE112619.M
Quant Title :
QLast Update : Tue Nov 26 14:51:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.563	125098	0.387 ug/ml
15)	N-TETRATRIACONTANE	19.378	105399	0.336 ug/ml
16)	N-HEXATRIACONTANE	20.113	317130	1.066 ug/ml
17)	N-OCTATRIACONTANE	20.750f	442323	1.597 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120919\
Data File : FE030985.D
Signal(s) : FID1B.CH
Acq On : 09 Dec 2019 9:44
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 10 00:25:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE112619.M
Quant Title :
QLast Update : Tue Nov 26 14:51:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

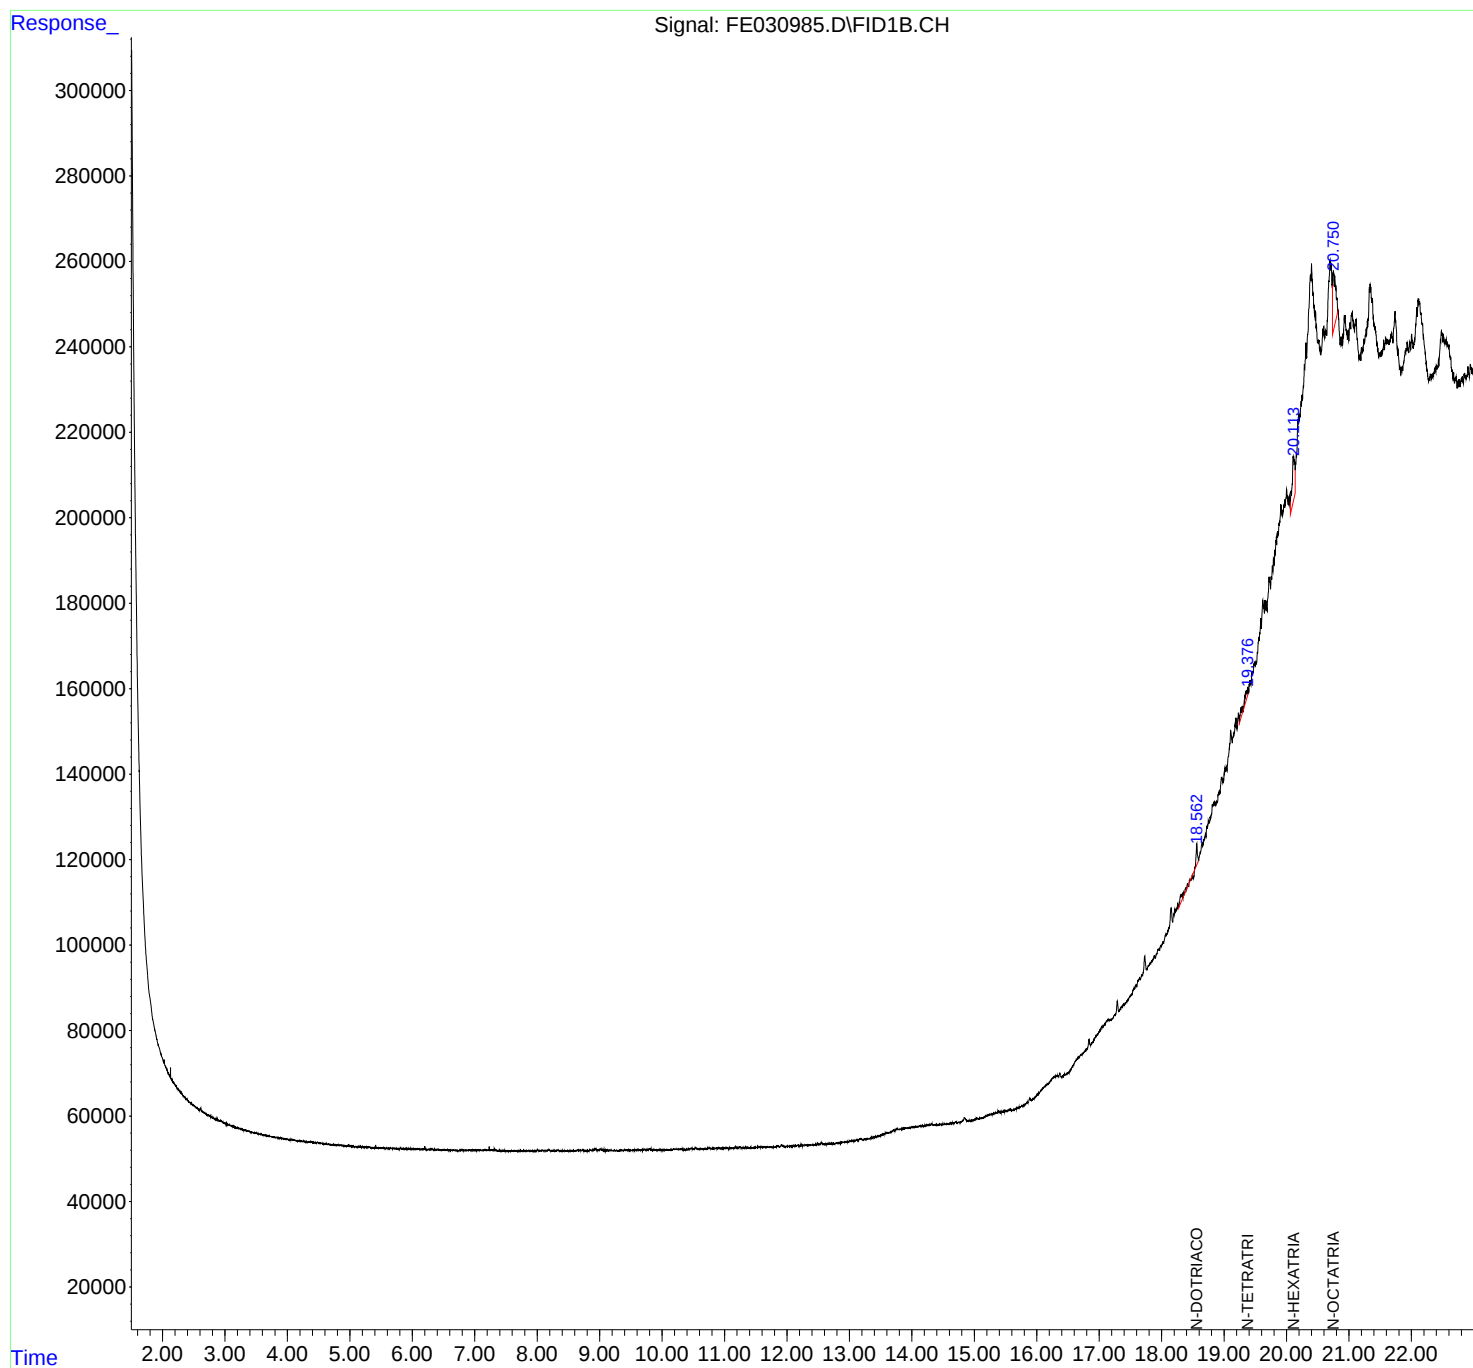

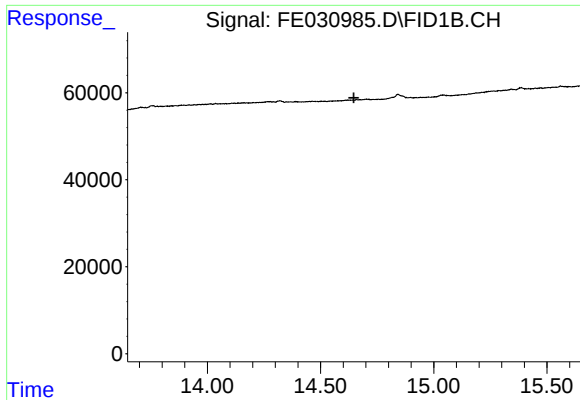


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.647 min
Response: 0
Conc: N.D.

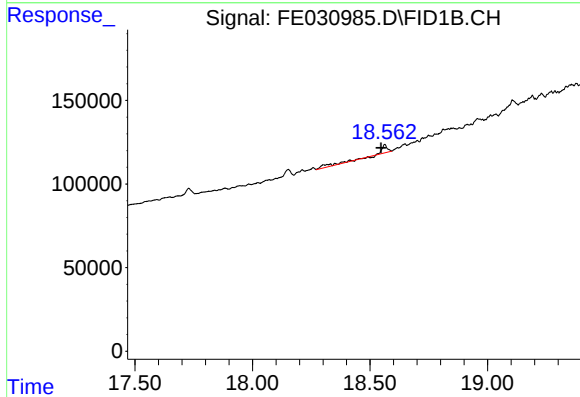


#14 N-DOTRIACONTANE

R.T.: 18.563 min
Delta R.T.: 0.015 min
Response: 125098
Conc: 0.39 ug/ml

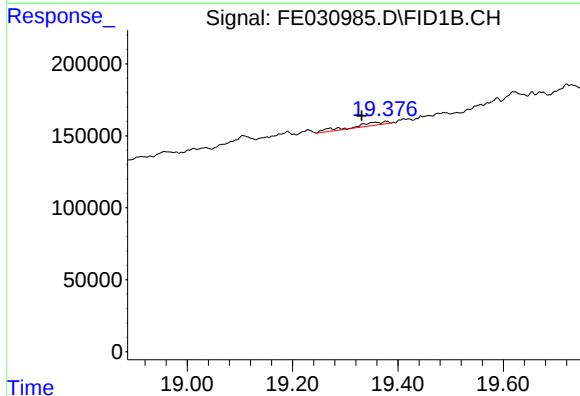


#15 N-TETRATRIACONTANE

R.T.: 19.378 min
Delta R.T.: 0.046 min
Response: 105399
Conc: 0.34 ug/ml

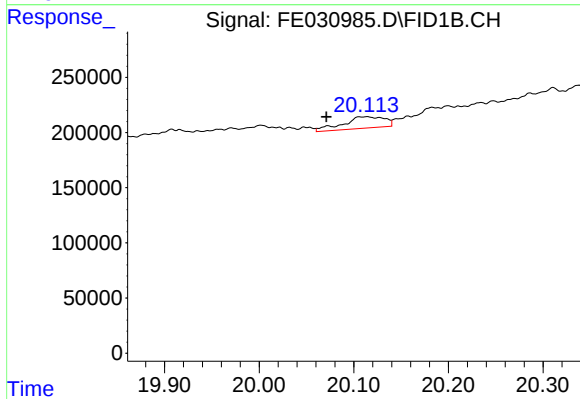

#16 N-HEXATRIACONTANE

R.T.: 20.113 min
Delta R.T.: 0.042 min
Response: 317130
Conc: 1.07 ug/ml

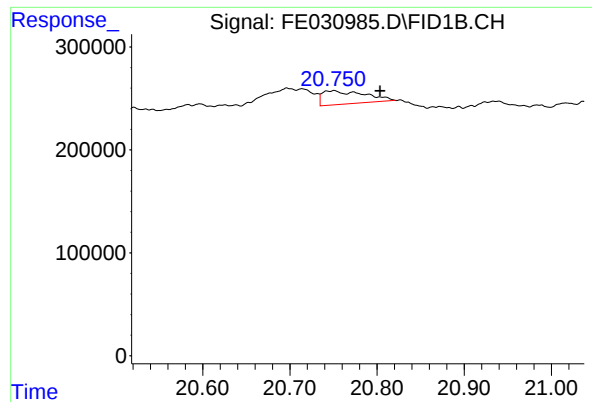

#17 N-OCTATRIACONTANE

R.T.: 20.750 min
Delta R.T.: -0.053 min
Response: 442323
Conc: 1.60 ug/ml