

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120922AL\
 Data File : FE039229.D
 Signal(s) : FID1B.ch
 Acq On : 09 Dec 2022 22:42
 Operator : YP\AJ
 Sample : N5965-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 11 03:04:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.940	5967306	38.145 ug/ml
Spiked Amount 50.000		Recovery =	76.29%
12) S 1-chlorooctadecane (S...	13.374	4688624	38.832 ug/ml
Spiked Amount 50.000		Recovery =	77.66%
Target Compounds			
10) T n-Eicosane (C20)	12.988	230838	1.626 ug/ml
14) T n-Tetracosane (C24)	15.206	112889	0.817 ug/ml
16) T n-Octacosane (C28)	17.201	96706	0.728 ug/ml
17) T n-Tricontane (C30)	18.086	76071	0.576 ug/ml
18) T n-Dotriacontane (C32)	18.913	127914	0.959 ug/ml
19) T n-Tetratriacontane (C34)	19.705	31650	0.239 ug/ml
20) T n-Hexatriacontane (C36)	20.515f	19391	0.151 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120922AL\
Data File : FE039229.D
Signal(s) : FID1B.ch
Acq On : 09 Dec 2022 22:42
Operator : YP\AJ
Sample : N5965-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 03:04:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

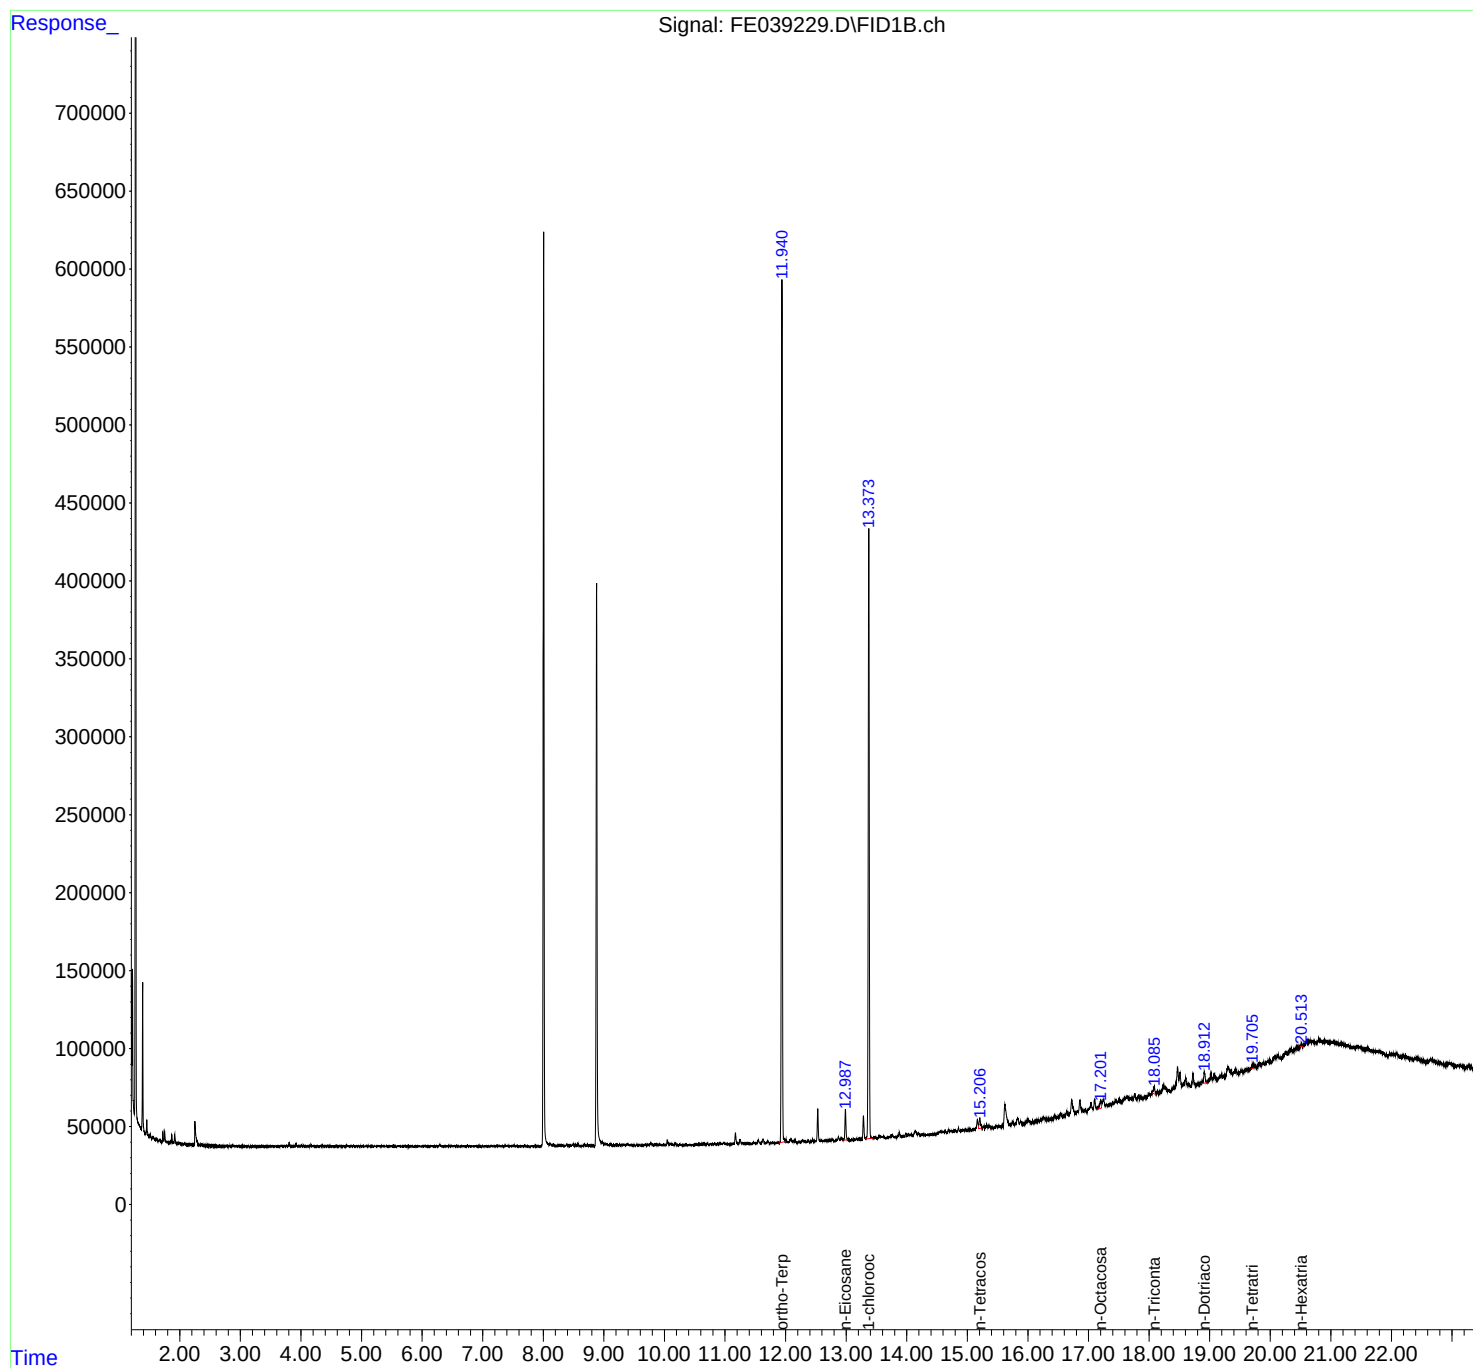


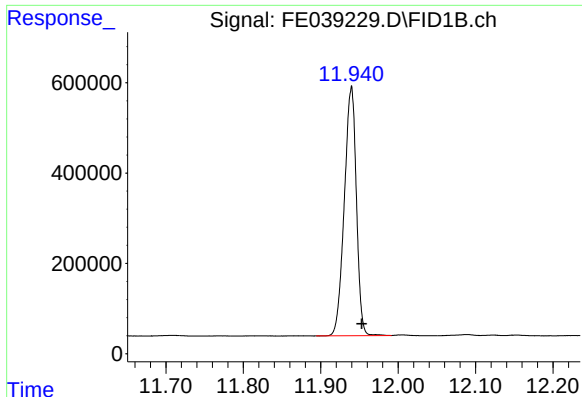

#9 ortho-Terphenyl (SURR)


R.T.: 11.940 min
Delta R.T.: -0.014 min
Response: 5967306
Conc: 38.14 ug/ml

Instrument :
FID_E
ClientSampleId :

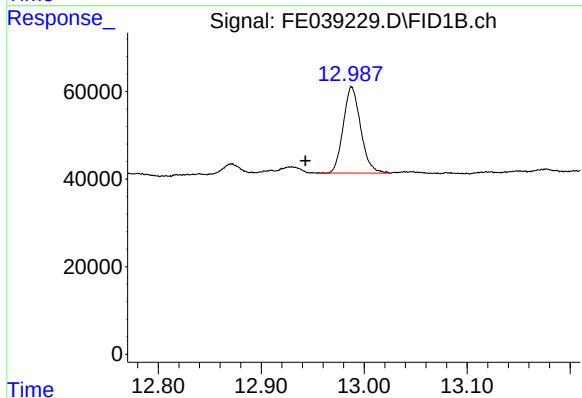


#10 n-Eicosane (C20)

R.T.: 12.988 min
Delta R.T.: 0.045 min
Response: 230838
Conc: 1.63 ug/ml

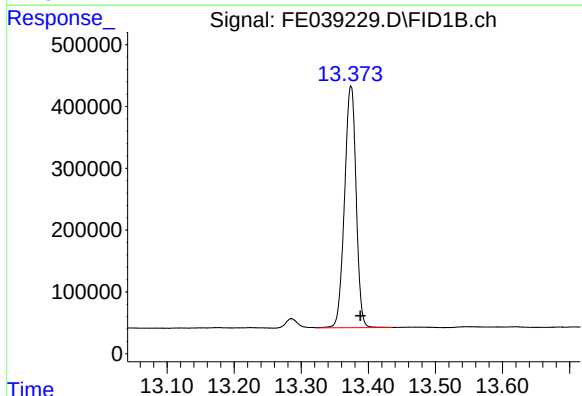


#12 1-chlorooctadecane (SURR)

R.T.: 13.374 min
Delta R.T.: -0.014 min
Response: 4688624
Conc: 38.83 ug/ml

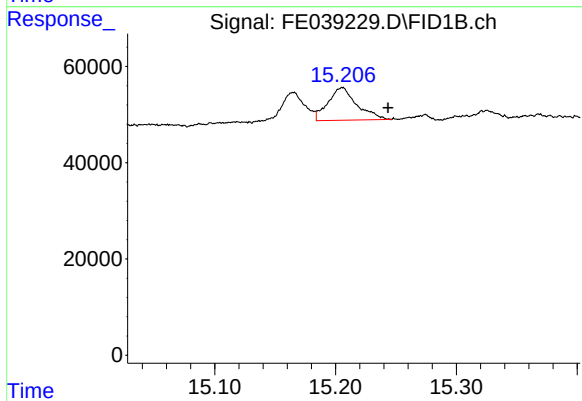

#14 n-Tetracosane (C24)


R.T.: 15.206 min
Delta R.T.: -0.038 min
Response: 112889
Conc: 0.82 ug/ml

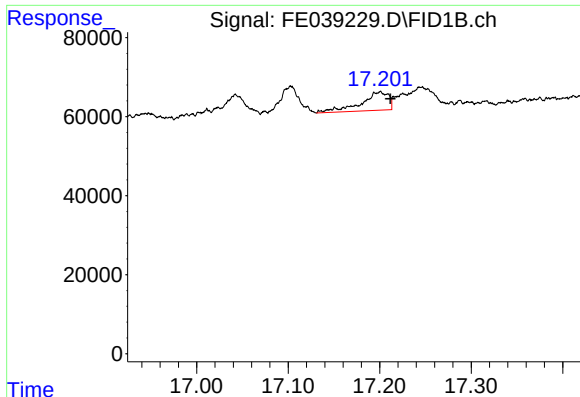

#16 n-Octacosane (C28)


R.T.: 17.201 min
Delta R.T.: -0.011 min
Response: 96706
Conc: 0.73 ug/ml

Instrument :
FID_E
ClientSampleId :

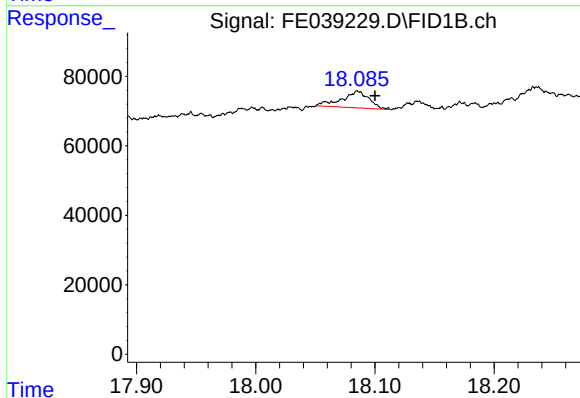


#17 n-Tricontane (C30)

R.T.: 18.086 min
Delta R.T.: -0.014 min
Response: 76071
Conc: 0.58 ug/ml

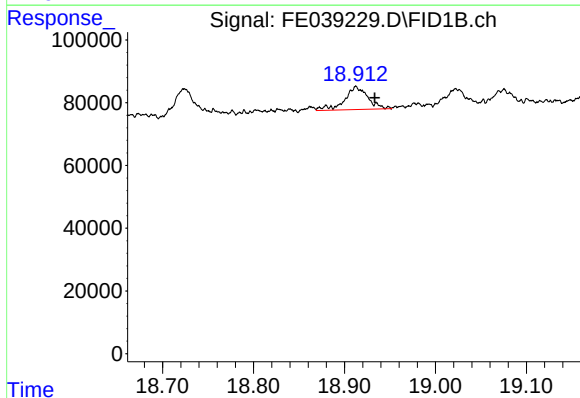


#18 n-Dotriacontane (C32)

R.T.: 18.913 min
Delta R.T.: -0.021 min
Response: 127914
Conc: 0.96 ug/ml

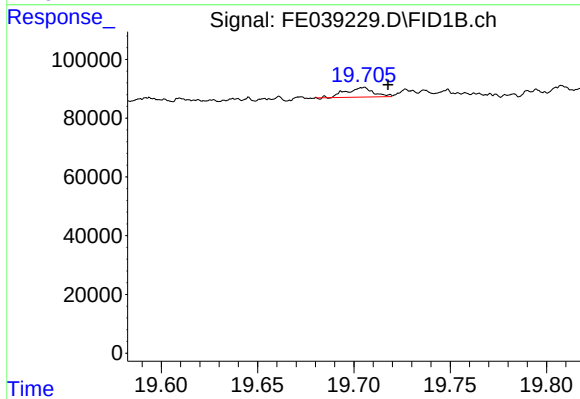

#19 n-Tetratriacontane (C34)

R.T.: 19.705 min
Delta R.T.: -0.013 min
Response: 31650
Conc: 0.24 ug/ml

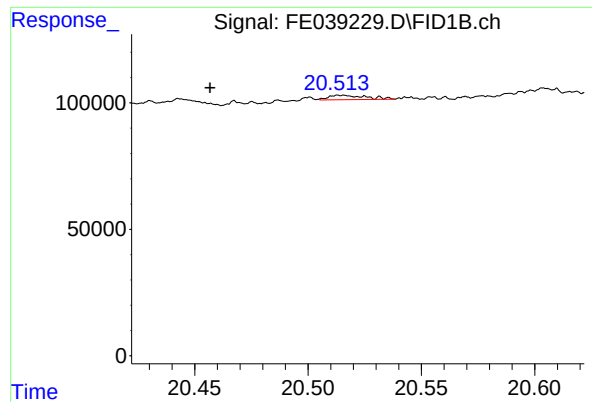

#20 n-Hexatriacontane (C36)

R.T.: 20.515 min
Delta R.T.: 0.058 min
Response: 19391
Conc: 0.15 ug/ml

Instrument :

FID_E

ClientSampleId :