

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120925AL\
Data File : FE057249.D
Signal(s) : FID1B.ch
Acq On : 09 Dec 2025 15:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 10 00:19:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 112725.M
Quant Title : GC Extractables
QLast Update : Mon Dec 01 08:04:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.927	117204	0.502 ug/ml
19) T	n-Tetratriacontane (C34)	19.713	65027	0.304 ug/ml
20) T	n-Hexatriacontane (C36)	20.455	80986	0.435 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE120925AL\
Data File : FE057249.D
Signal(s) : FID1B.ch
Acq On : 09 Dec 2025 15:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 10 00:19:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 112725.M
Quant Title : GC Extractables
QLast Update : Mon Dec 01 08:04:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

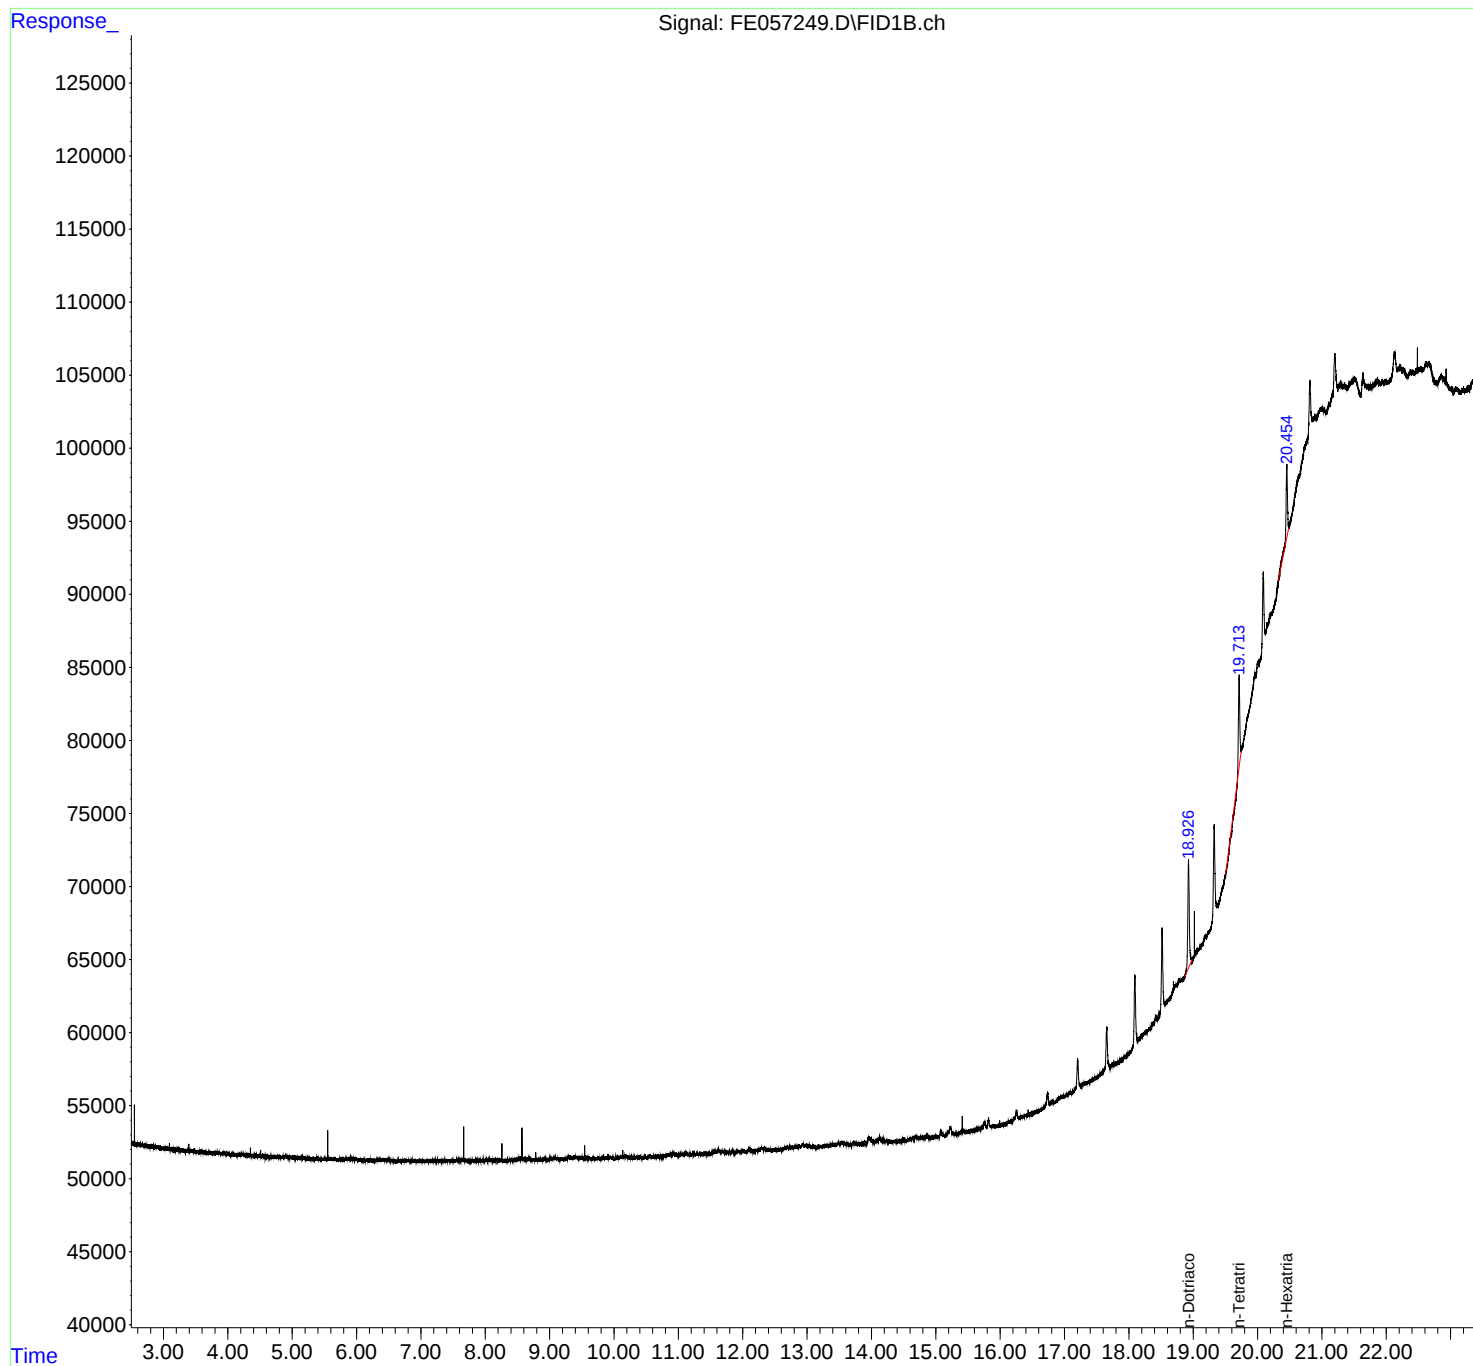


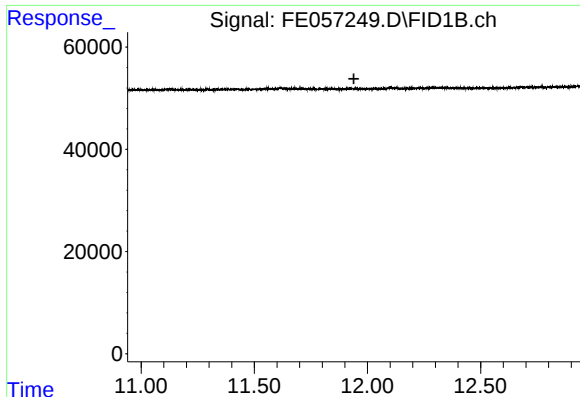

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.940 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

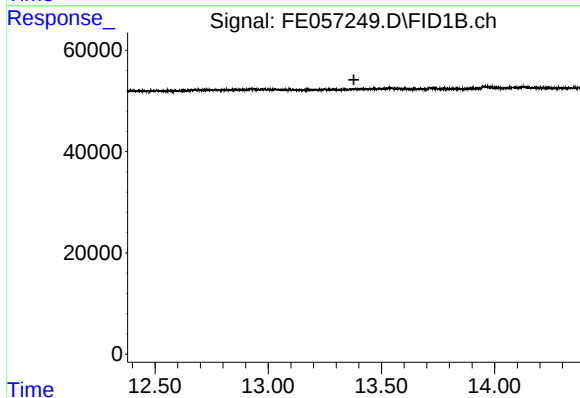


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.378 min
Response: 0
Conc: N.D.

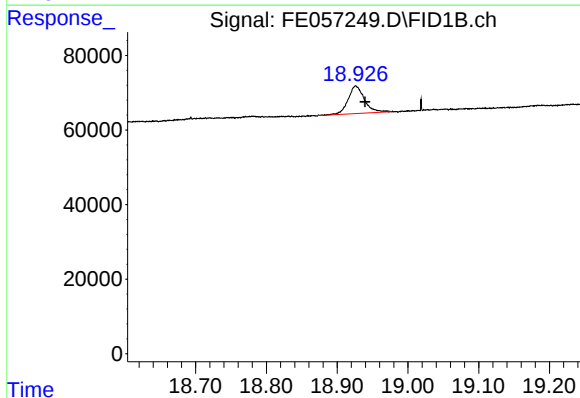


#18 n-Dotriacontane (C32)

R.T.: 18.927 min
Delta R.T.: -0.013 min
Response: 117204
Conc: 0.50 ug/ml

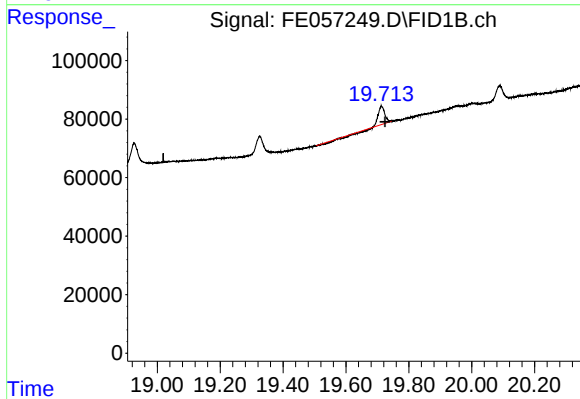

#19 n-Tetratriacontane (C34)

R.T.: 19.713 min
Delta R.T.: -0.011 min
Response: 65027
Conc: 0.30 ug/ml

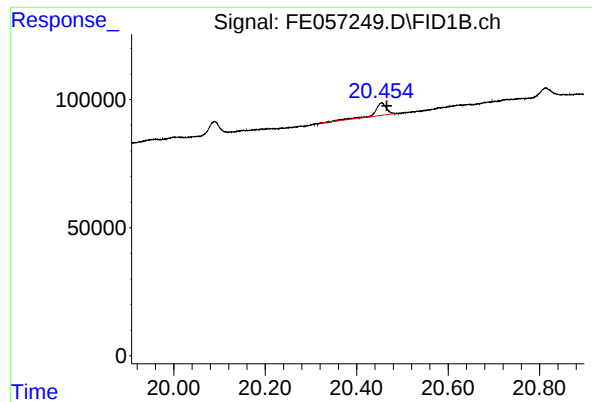

#20 n-Hexatriacontane (C36)

R.T.: 20.455 min
Delta R.T.: -0.011 min
Response: 80986
Conc: 0.44 ug/ml

Instrument :
FID_E
ClientSampleId :