

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121222AL\
 Data File : FE039241.D
 Signal(s) : FID1B.ch
 Acq On : 12 Dec 2022 12:30
 Operator : YP\AJ
 Sample : N5947-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 NYE-WATER-1208

Integration File: autoint1.e
 Quant Time: Dec 12 17:16:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.938	4614174	29.495 ug/ml
Spiked Amount 50.000		Recovery =	58.99%
12) S 1-chlorooctadecane (S...	13.372	3127824	25.905 ug/ml
Spiked Amount 50.000		Recovery =	51.81%

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121222AL\
Data File : FE039241.D
Signal(s) : FID1B.ch
Acq On : 12 Dec 2022 12:30
Operator : YP\AJ
Sample : N5947-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
NYE-WATER-1208

Integration File: autoint1.e
Quant Time: Dec 12 17:16:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

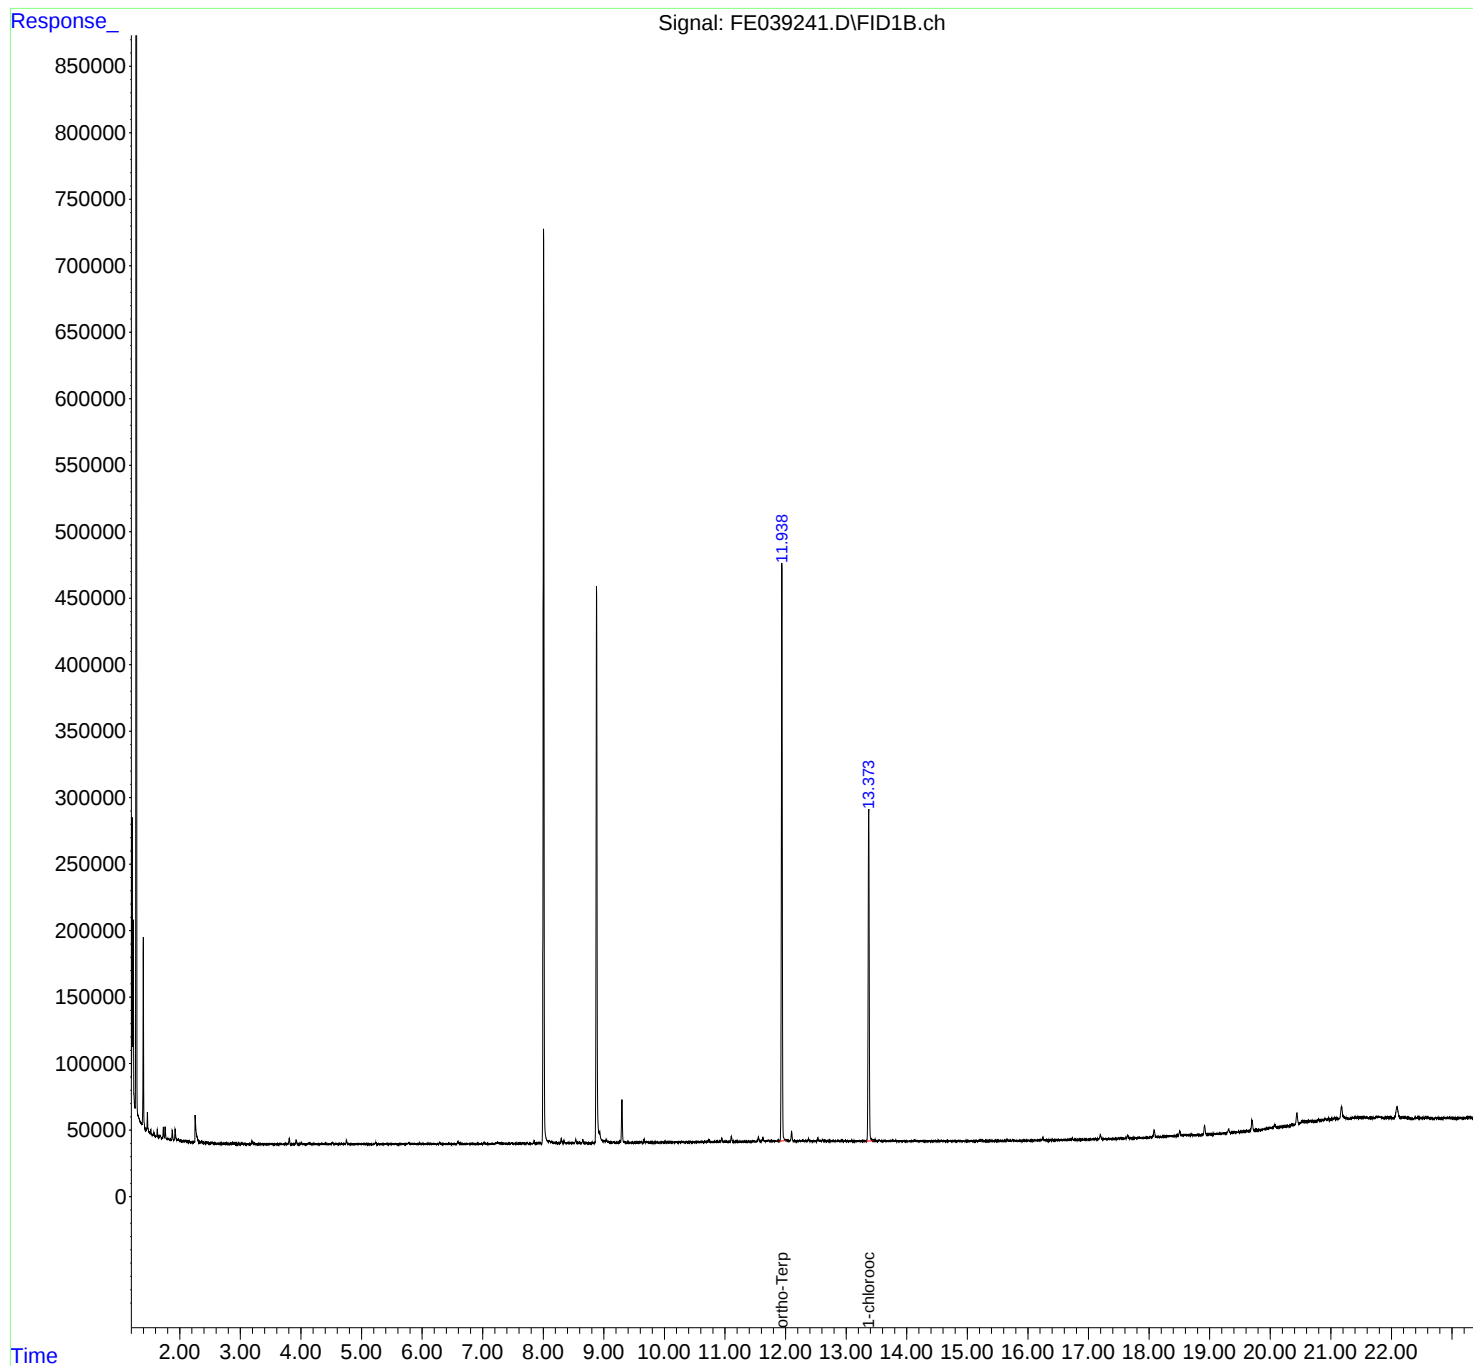


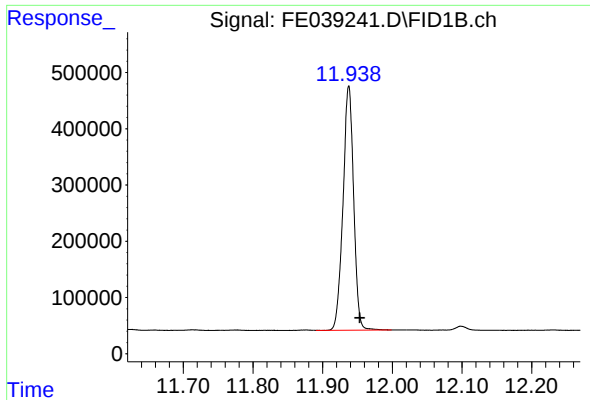

#9 ortho-Terphenyl (SURR)

R.T.: 11.938 min
Delta R.T.: -0.016 min
Response: 4614174
Conc: 29.50 ug/ml

Instrument :
FID_E
ClientSampleId :
NYE-WATER-1208

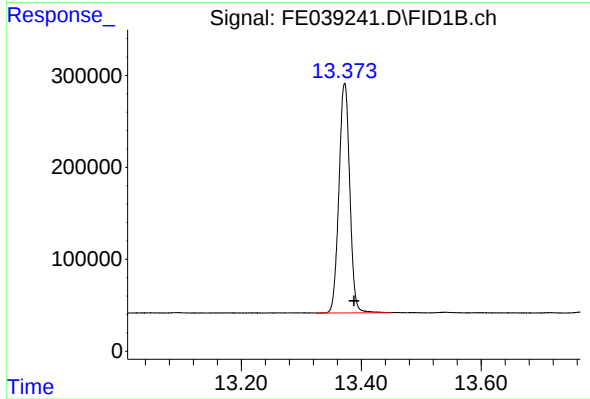

#12 1-chlorooctadecane (SURR)

R.T.: 13.372 min
Delta R.T.: -0.016 min
Response: 3127824
Conc: 25.91 ug/ml