

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121318\
 Data File : FE029325.D
 Signal(s) : FID1B.CH
 Acq On : 13 Dec 2018 16:00
 Operator : AJ\SJ
 Sample : J6344-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 14 00:39:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE120718.M
 Quant Title :
 QLast Update : Fri Dec 07 23:47:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.833	80674	0.421 ug/ml
Target Compounds			
4) N-UNDECANE	5.587	118957	0.655 ug/ml
5) N-DODECANE	6.592	44032	0.244 ug/ml
6) N-TETRADECANE	8.384	1771238	9.909 ug/ml
7) N-HEXADECANE	10.023	4906858	26.557 ug/ml
8) N-OCTADECANE	11.412	1036500	5.595 ug/ml
9) N-EICOSANE	12.737	421165	2.326 ug/ml
10) N-TETRACOSANE	15.022	249408	1.341 ug/ml
11) N-OCTACOSANE	17.013	923706	4.971 ug/ml
12) N-DOTRIACONTANE	18.750	603941	3.316 ug/ml
14) N-HEXATRIACONTANE	20.274	201198	1.123 ug/ml
15) N-TETRACONTANE	22.010	272643	1.749 ug/ml
16) N-TETRTETRACOOCTANE	24.952	209366	1.785 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121318\
Data File : FE029325.D
Signal(s) : FID1B.CH
Acq On : 13 Dec 2018 16:00
Operator : AJ\SJ
Sample : J6344-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 14 00:39:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE120718.M
Quant Title :
QLast Update : Fri Dec 07 23:47:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

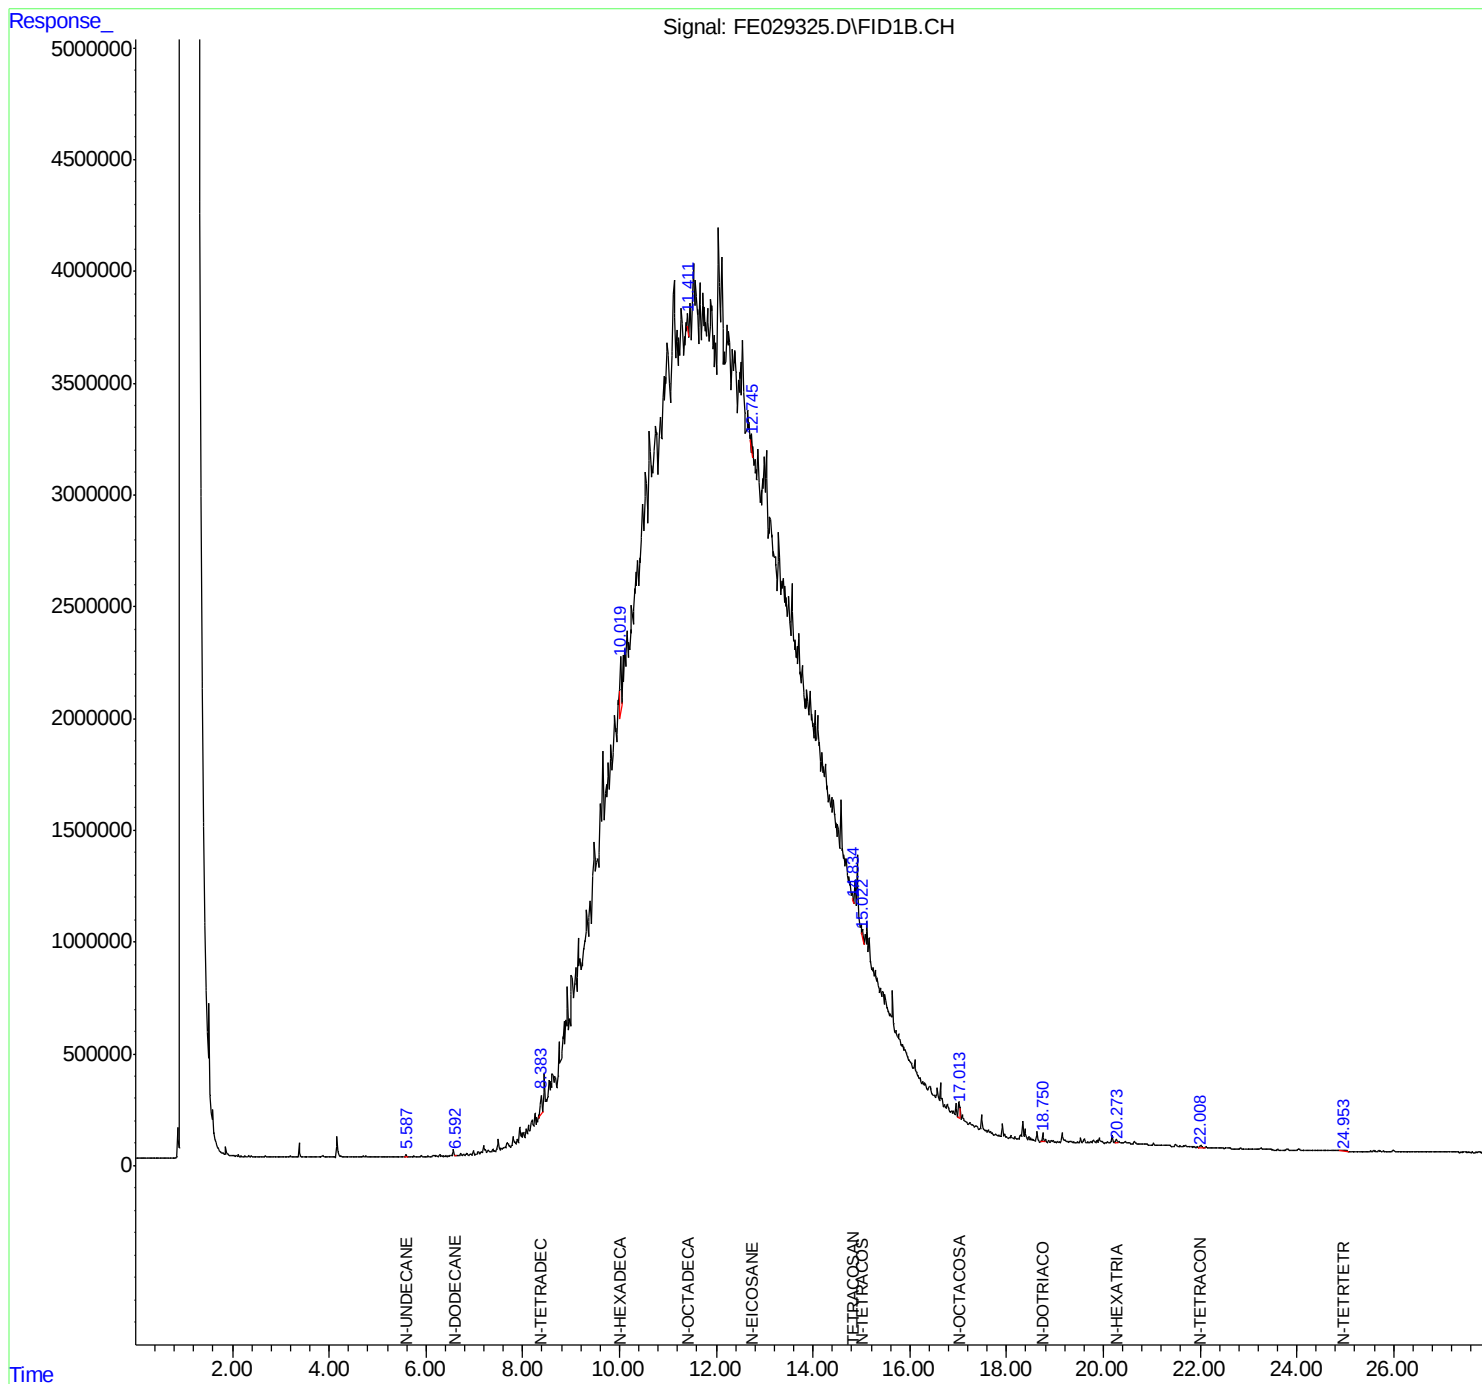

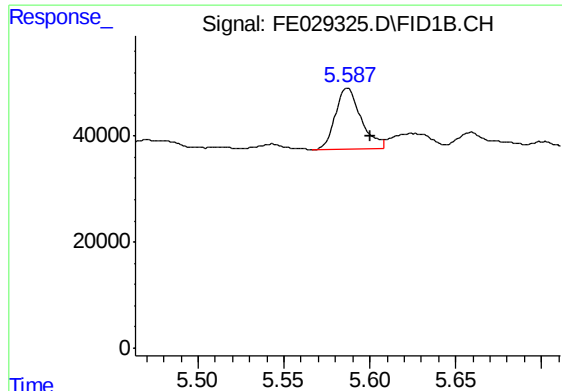


#4 N-UNDECANE

R.T.: 5.587 min
Delta R.T.: -0.014 min
Response: 118957
Conc: 0.66 ug/ml

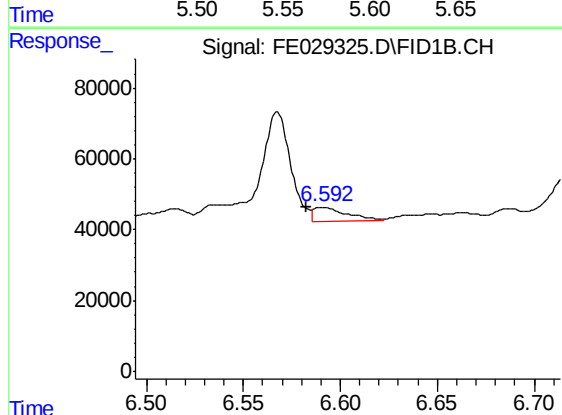


#5 N-DODECANE

R.T.: 6.592 min
Delta R.T.: 0.009 min
Response: 44032
Conc: 0.24 ug/ml

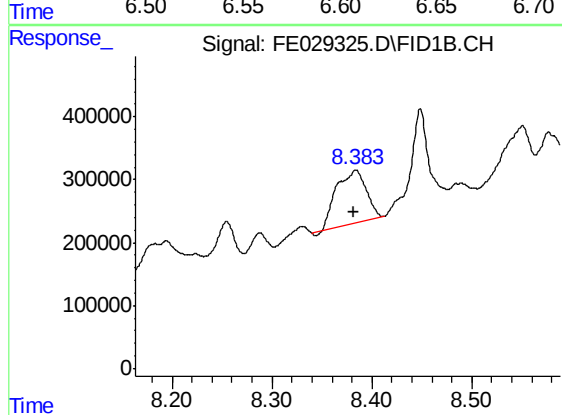


#6 N-TETRADECANE

R.T.: 8.384 min
Delta R.T.: 0.002 min
Response: 1771238
Conc: 9.91 ug/ml

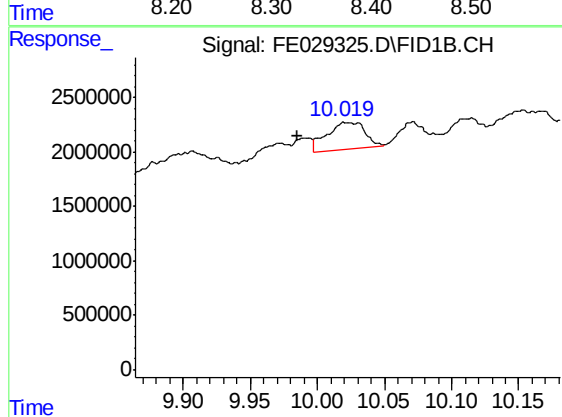


#7 N-HEXADECANE

R.T.: 10.023 min
Delta R.T.: 0.038 min
Response: 4906858
Conc: 26.56 ug/ml

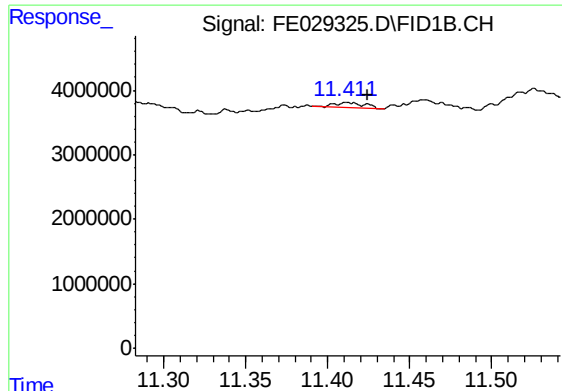


#8 N-OCTADECANE

R.T.: 11.412 min
Delta R.T.: -0.013 min
Response: 1036500
Conc: 5.60 ug/ml

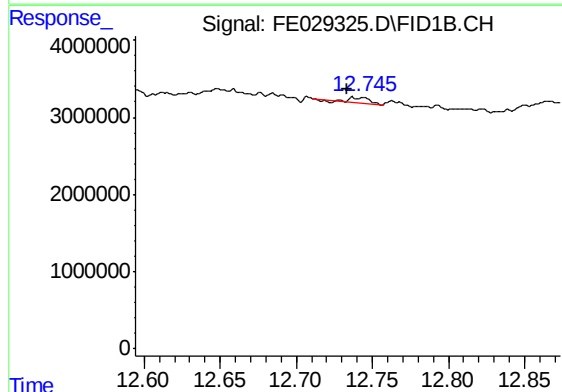


#9 N-EICOSANE

R.T.: 12.737 min
Delta R.T.: 0.004 min
Response: 421165
Conc: 2.33 ug/ml

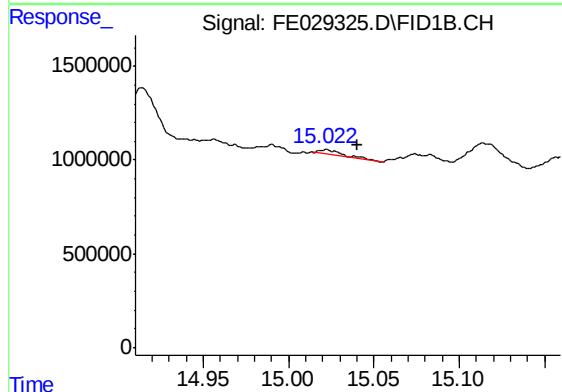


#10 N-TETRACOSANE

R.T.: 15.022 min
Delta R.T.: -0.019 min
Response: 249408
Conc: 1.34 ug/ml

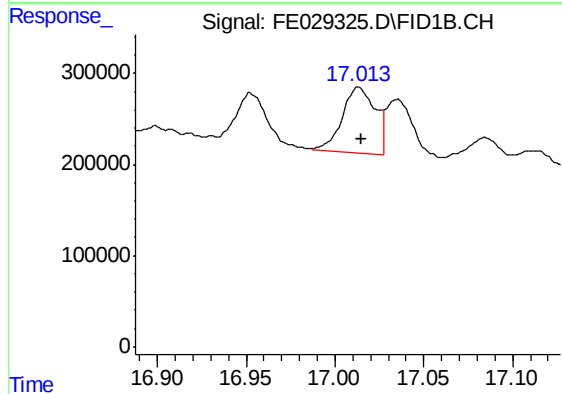


#11 N-OCTACOSANE

R.T.: 17.013 min
Delta R.T.: -0.001 min
Response: 923706
Conc: 4.97 ug/ml

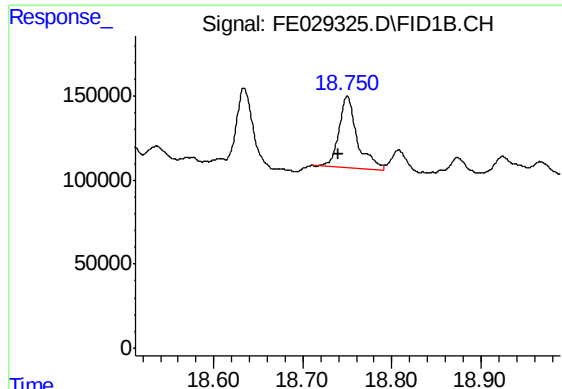


#12 N-DOTRIACONTANE

R.T.: 18.750 min
Delta R.T.: 0.010 min
Response: 603941
Conc: 3.32 ug/ml

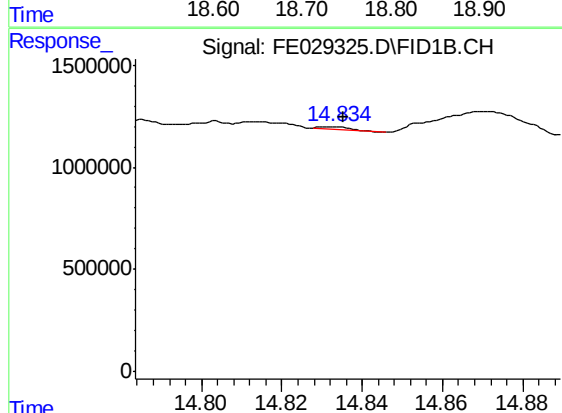


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.833 min
Delta R.T.: -0.003 min
Response: 80674
Conc: 0.42 ug/ml

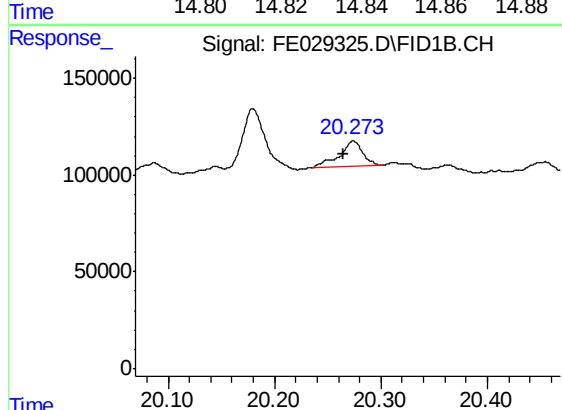


#14 N-HEXATRIACONTANE

R.T.: 20.274 min
Delta R.T.: 0.010 min
Response: 201198
Conc: 1.12 ug/ml

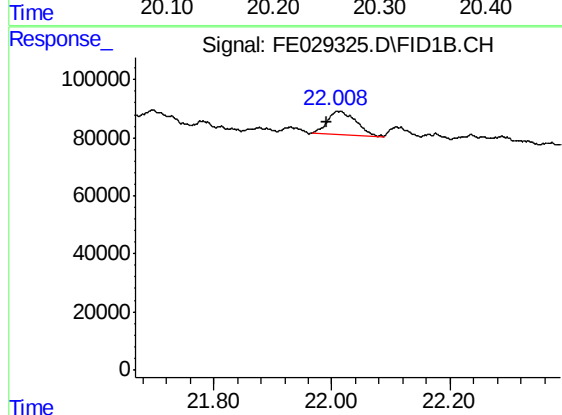

#15 N-TETRACONTANE

R.T.: 22.010 min
Delta R.T.: 0.019 min
Response: 272643
Conc: 1.75 ug/ml

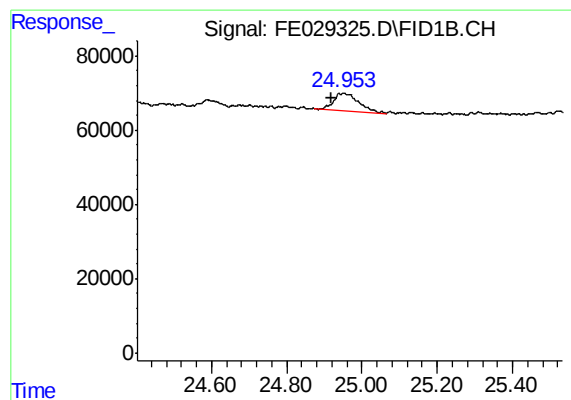

#16 N-TETRTETRACOEANE

R.T.: 24.952 min
Delta R.T.: 0.034 min
Response: 209366
Conc: 1.79 ug/ml