

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121318\
 Data File : FE029326.D
 Signal(s) : FID1B.CH
 Acq On : 13 Dec 2018 16:38
 Operator : AJ\SJ
 Sample : J6344-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 14 00:39:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE120718.M
 Quant Title :
 QLast Update : Fri Dec 07 23:47:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.857	1303930	6.805 ug/ml
Target Compounds			
6) N-TETRADECANE	8.366	440455	2.464 ug/ml
7) N-HEXADECANE	10.006	4224493	22.864 ug/ml
8) N-OCTADECANE	11.409	58502	0.316 ug/ml
9) N-EICOSANE	12.723	3016748	16.658 ug/ml
10) N-TETRACOSANE	15.058	357516	1.923 ug/ml
11) N-OCTACOSANE	17.023	121836	0.656 ug/ml
12) N-DOTRIACONTANE	18.742	157811	0.867 ug/ml
14) N-HEXATRIACONTANE	20.264	45850	0.256 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121318\
Data File : FE029326.D
Signal(s) : FID1B.CH
Acq On : 13 Dec 2018 16:38
Operator : AJ\SJ
Sample : J6344-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 14 00:39:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE120718.M
Quant Title :
QLast Update : Fri Dec 07 23:47:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

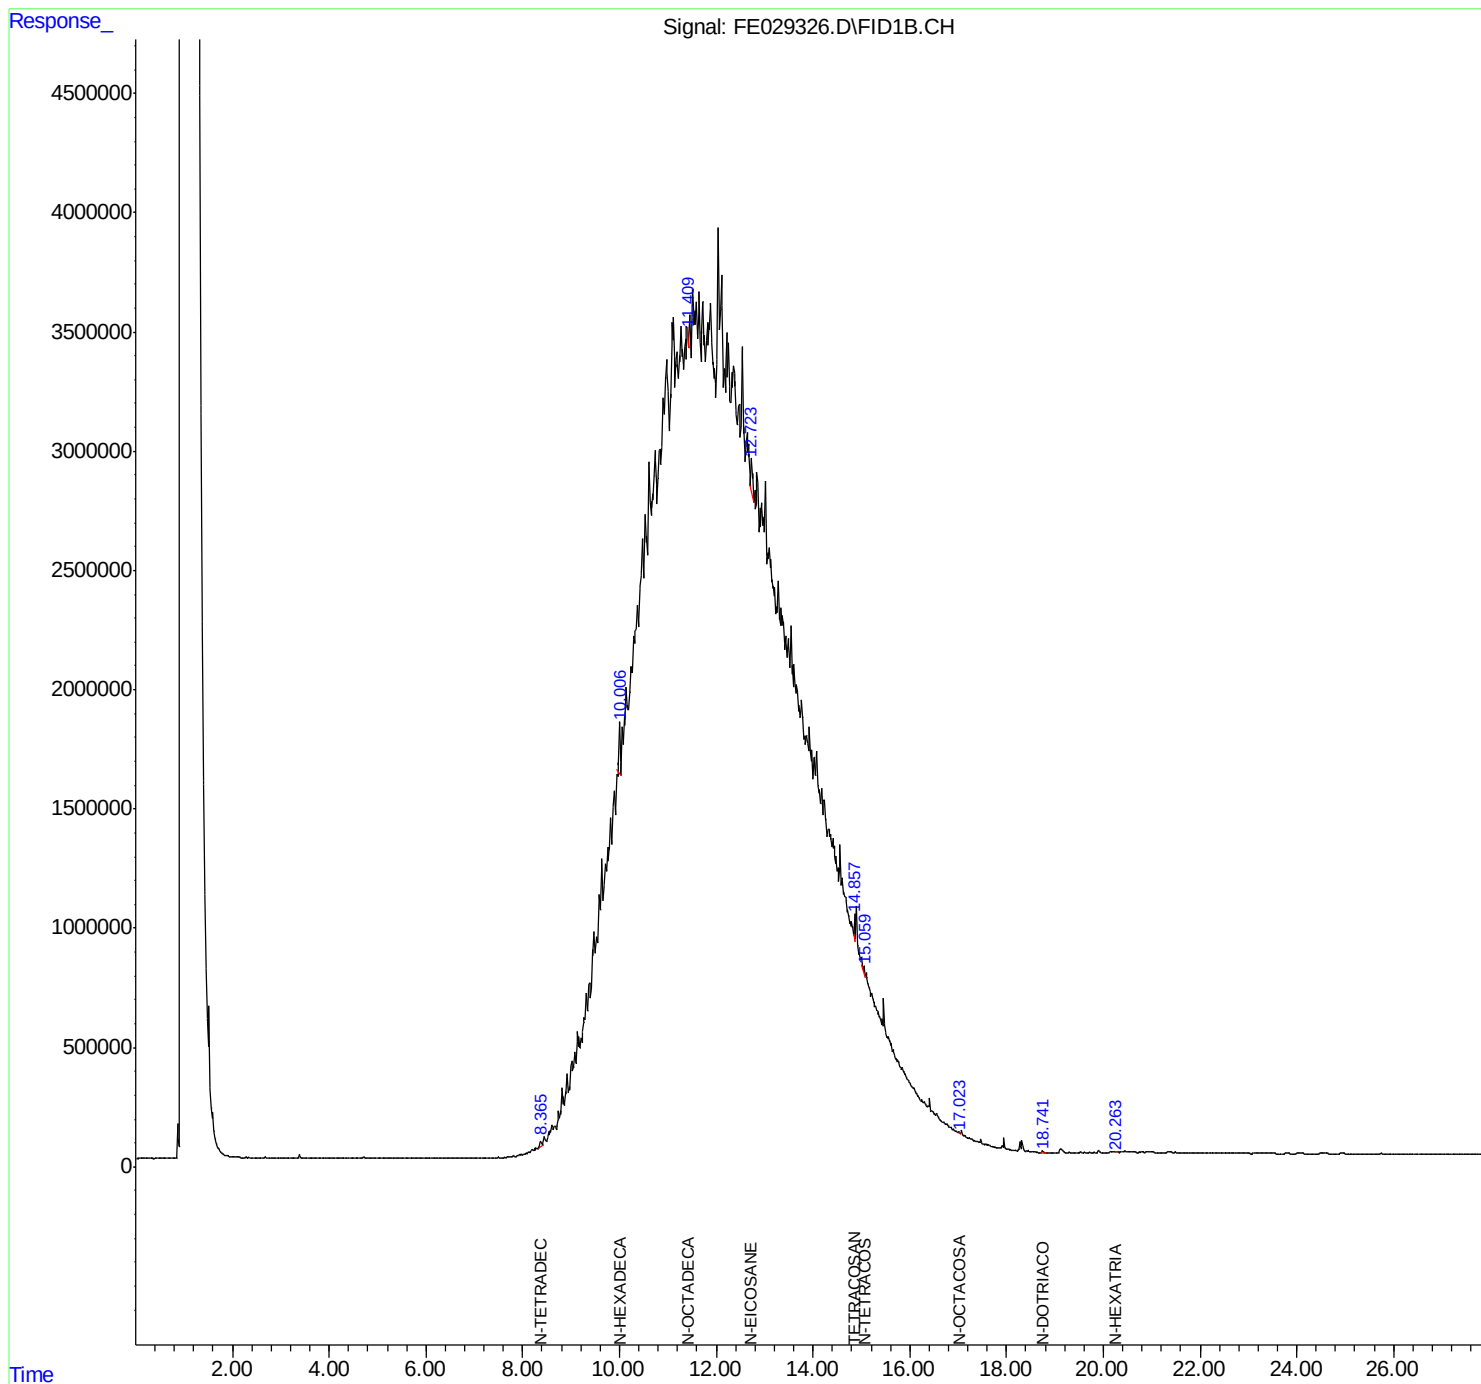

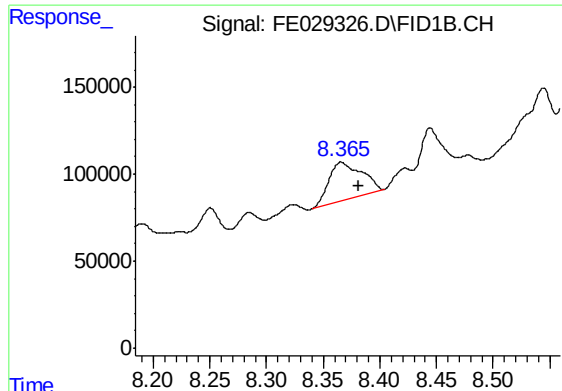


#6 N-TETRADECANE

R.T.: 8.366 min
Delta R.T.: -0.016 min
Response: 440455
Conc: 2.46 ug/ml

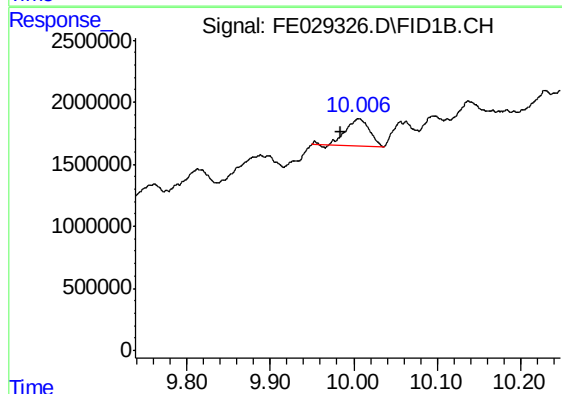


#7 N-HEXADECANE

R.T.: 10.006 min
Delta R.T.: 0.021 min
Response: 4224493
Conc: 22.86 ug/ml

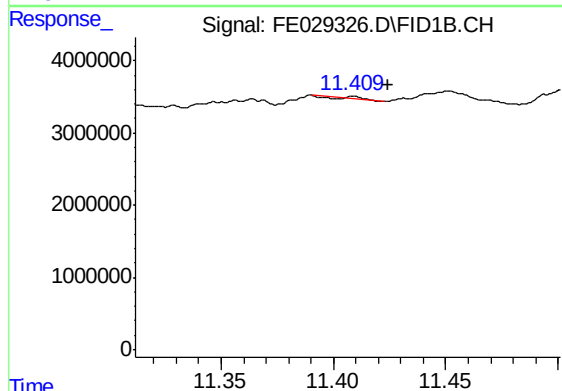


#8 N-OCTADECANE

R.T.: 11.409 min
Delta R.T.: -0.016 min
Response: 58502
Conc: 0.32 ug/ml

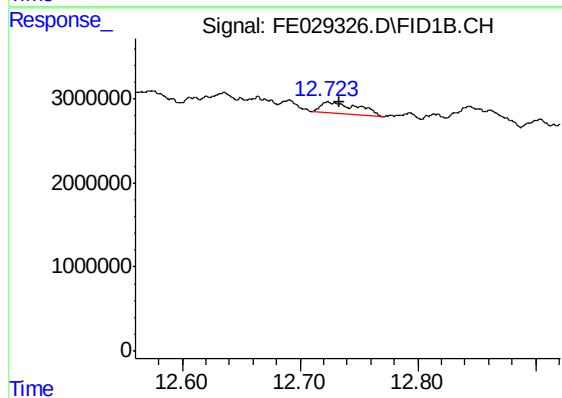


#9 N-EICOSANE

R.T.: 12.723 min
Delta R.T.: -0.010 min
Response: 3016748
Conc: 16.66 ug/ml

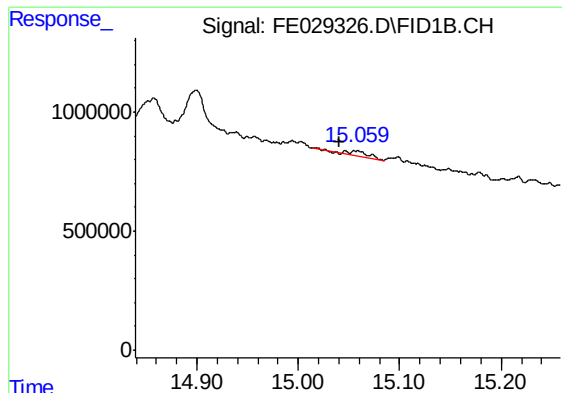


#10 N-TETRACOSANE

R.T.: 15.058 min
Delta R.T.: 0.018 min
Response: 357516
Conc: 1.92 ug/ml

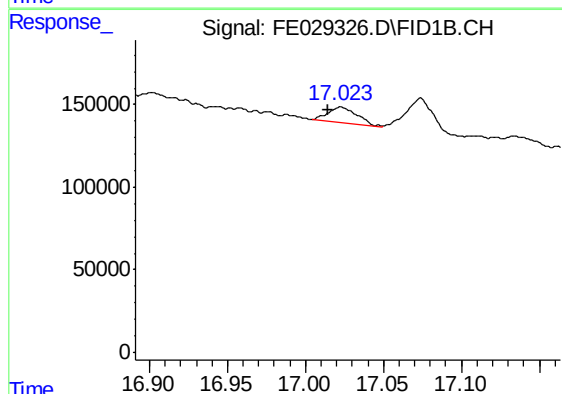


#11 N-OCTACOSANE

R.T.: 17.023 min
Delta R.T.: 0.008 min
Response: 121836
Conc: 0.66 ug/ml

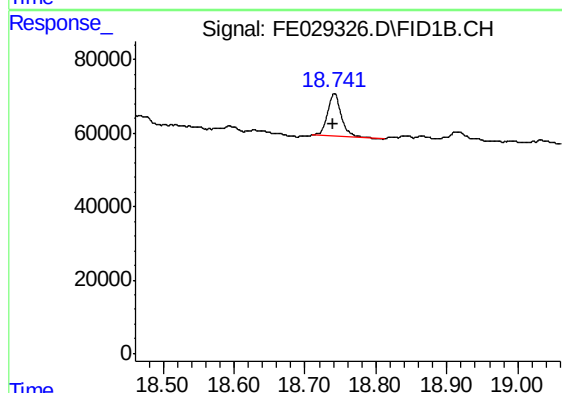


#12 N-DOTRIACONTANE

R.T.: 18.742 min
Delta R.T.: 0.002 min
Response: 157811
Conc: 0.87 ug/ml

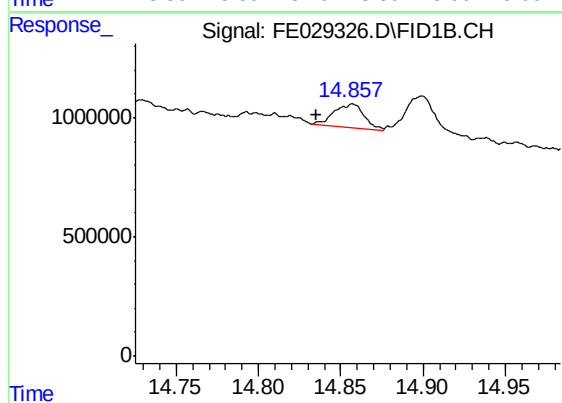

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.857 min
Delta R.T.: 0.022 min
Response: 1303930
Conc: 6.80 ug/ml

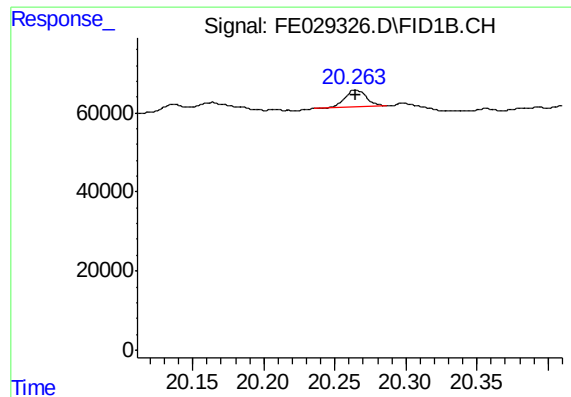

#14 N-HEXATRIACONTANE

R.T.: 20.264 min
Delta R.T.: 0.000 min
Response: 45850
Conc: 0.26 ug/ml