

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121322AL\
 Data File : FE039284.D
 Signal(s) : FID1B.ch
 Acq On : 13 Dec 2022 18:05
 Operator : YP\AJ
 Sample : N6025-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 14 02:16:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.940	4677211	29.898 ug/ml
Spiked Amount 50.000		Recovery =	59.80%
12) S 1-chlorooctadecane (S...	13.375	3758597	31.130 ug/ml
Spiked Amount 50.000		Recovery =	62.26%
Target Compounds			
10) T n-Eicosane (C20)	12.989	461972	3.254 ug/ml
14) T n-Tetracosane (C24)	15.207	297644	2.155 ug/ml
16) T n-Octacosane (C28)	17.204	89365	0.673 ug/ml
17) T n-Tricontane (C30)	18.087	52680	0.399 ug/ml
18) T n-Dotriacontane (C32)	18.919	51032	0.383 ug/ml
19) T n-Tetratriacontane (C34)	19.707	47363	0.358 ug/ml
20) T n-Hexatriacontane (C36)	20.517f	612	0.005 ug/ml
21) T n-Octatriacontane (C38)	21.180	50411	0.385 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121322AL\
Data File : FE039284.D
Signal(s) : FID1B.ch
Acq On : 13 Dec 2022 18:05
Operator : YP\AJ
Sample : N6025-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 02:16:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

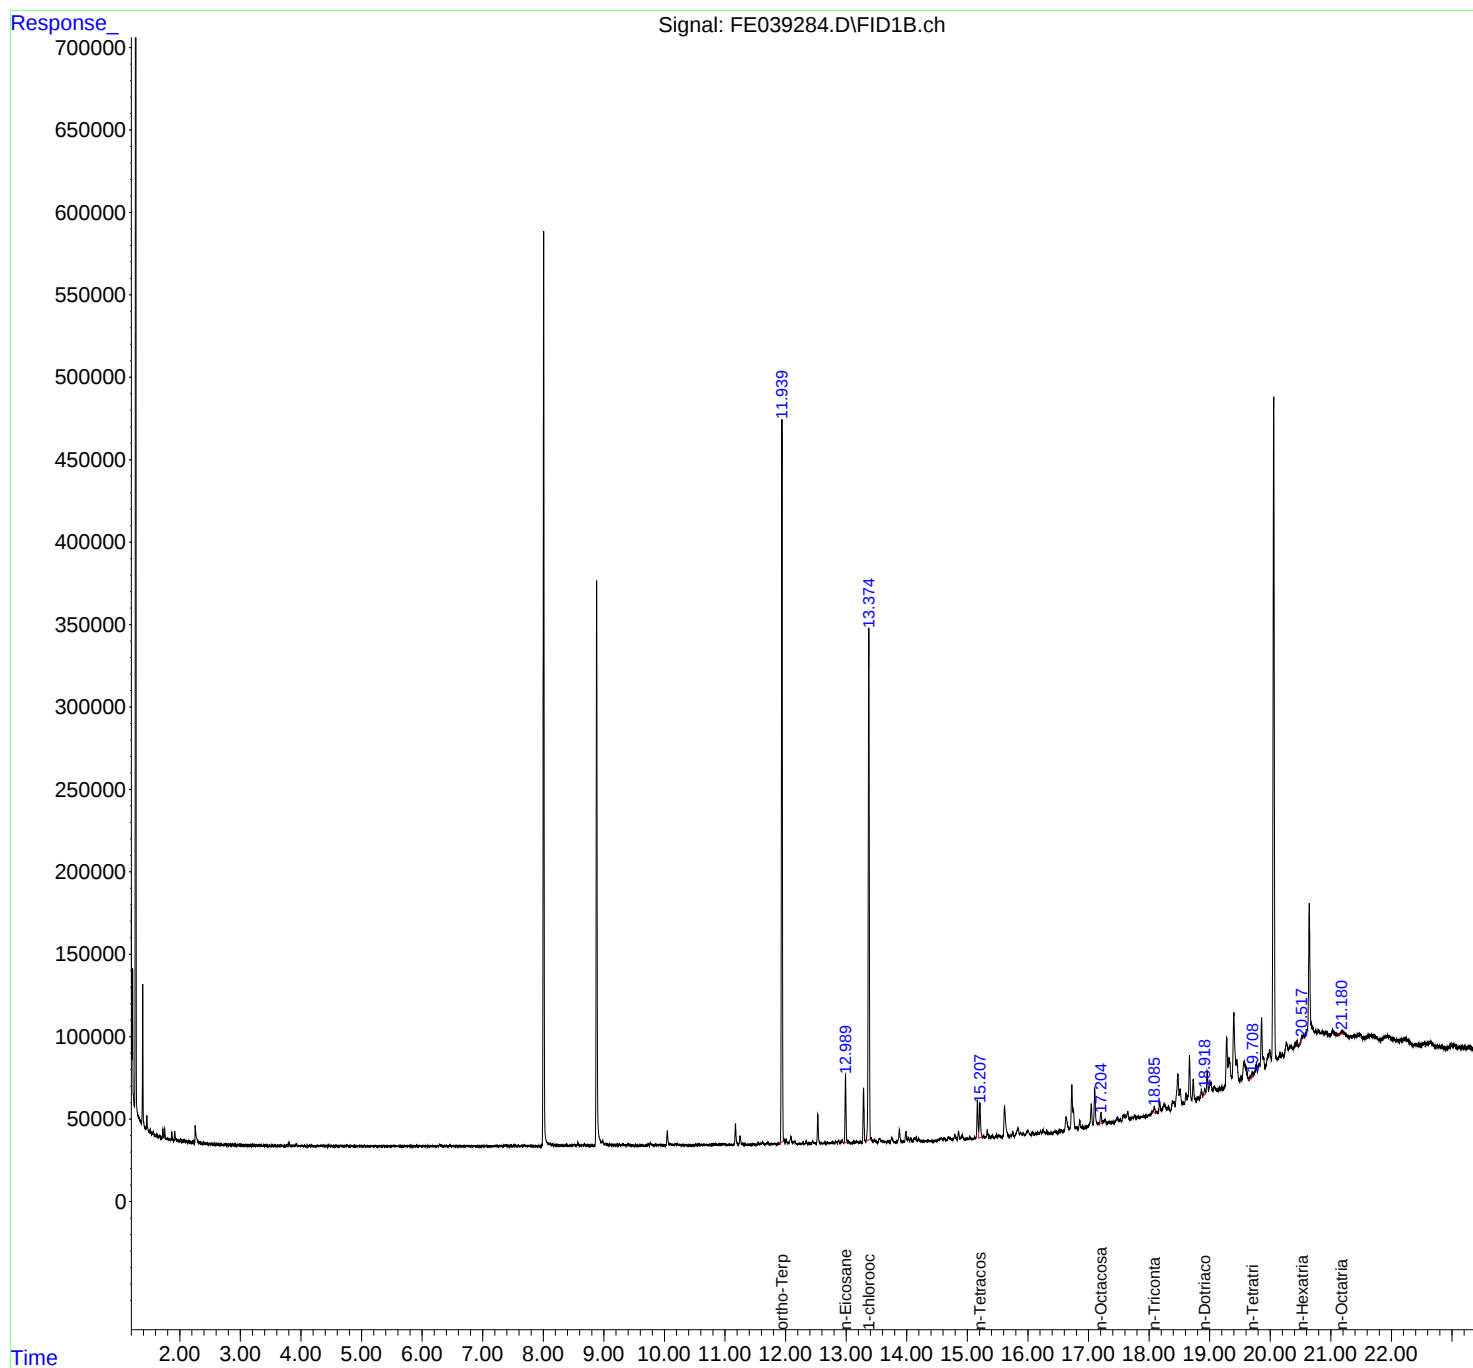


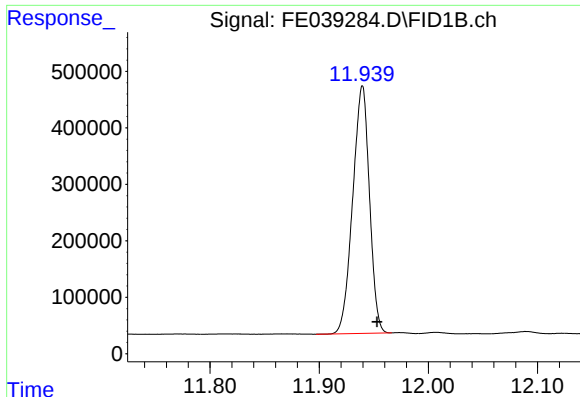

#9 ortho-Terphenyl (SURR)


R.T.: 11.940 min
Delta R.T.: -0.014 min
Response: 4677211
Conc: 29.90 ug/ml

Instrument :
FID_E
ClientSampleId :

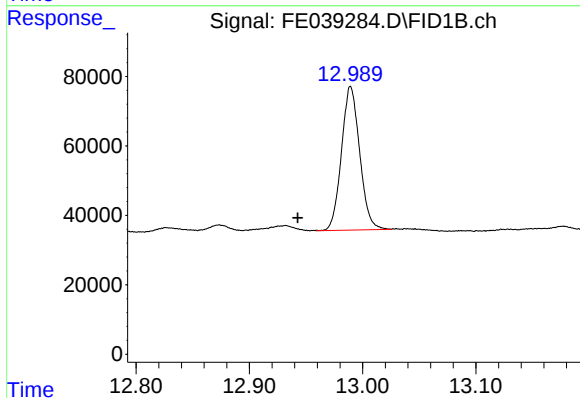


#10 n-Eicosane (C20)

R.T.: 12.989 min
Delta R.T.: 0.047 min
Response: 461972
Conc: 3.25 ug/ml

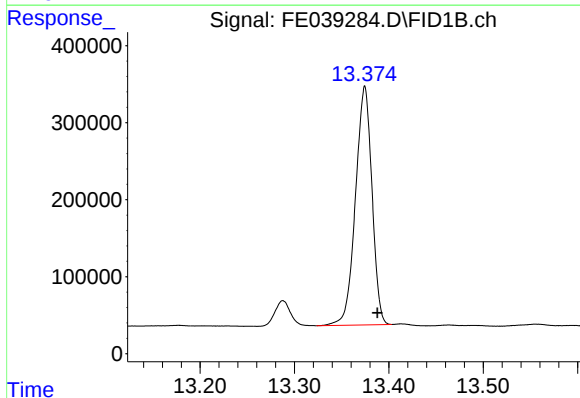


#12 1-chlorooctadecane (SURR)

R.T.: 13.375 min
Delta R.T.: -0.014 min
Response: 3758597
Conc: 31.13 ug/ml

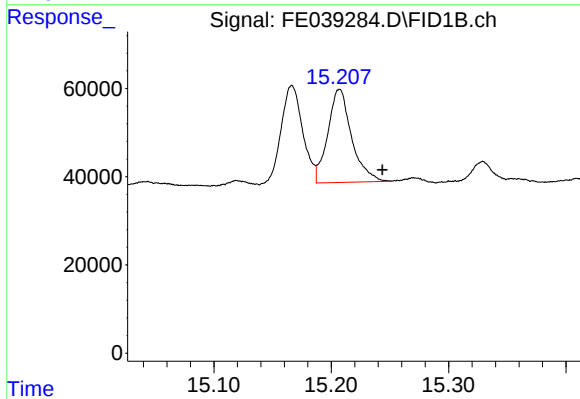

#14 n-Tetracosane (C24)


R.T.: 15.207 min
Delta R.T.: -0.036 min
Response: 297644
Conc: 2.16 ug/ml

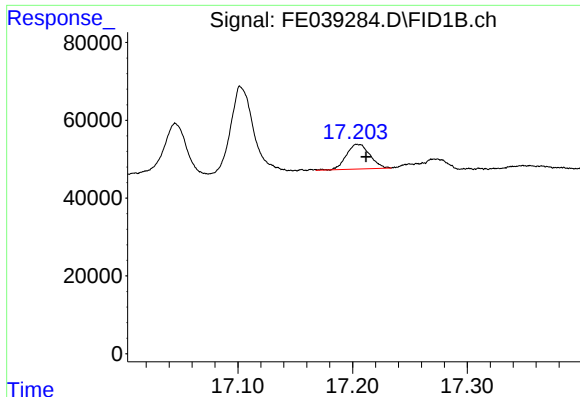

#16 n-Octacosane (C28)


R.T.: 17.204 min
Delta R.T.: -0.008 min
Response: 89365
Conc: 0.67 ug/ml

Instrument :
FID_E
ClientSampleId :

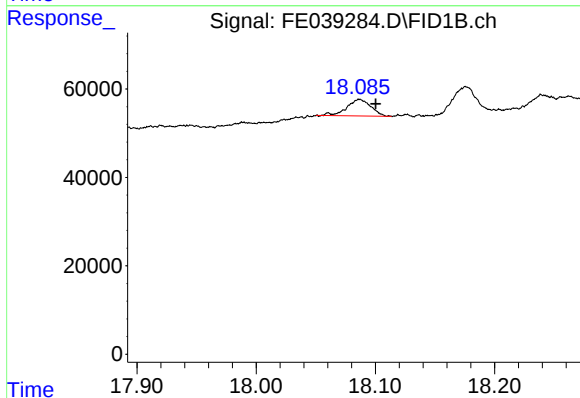


#17 n-Tricontane (C30)

R.T.: 18.087 min
Delta R.T.: -0.014 min
Response: 52680
Conc: 0.40 ug/ml

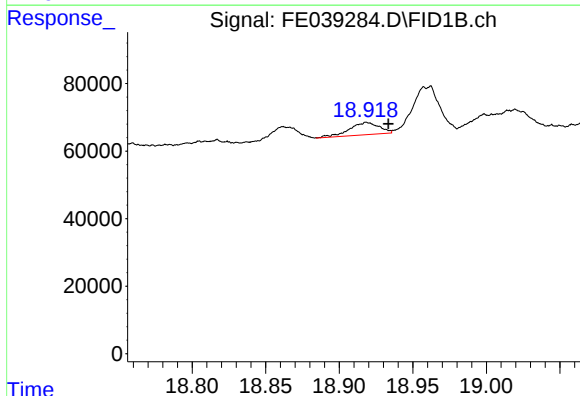


#18 n-Dotriacontane (C32)

R.T.: 18.919 min
Delta R.T.: -0.014 min
Response: 51032
Conc: 0.38 ug/ml

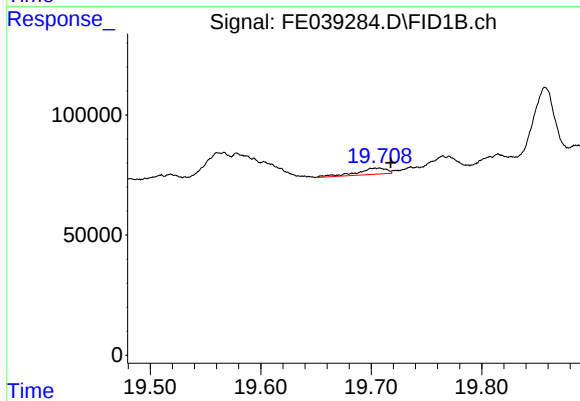

#19 n-Tetratriacontane (C34)


R.T.: 19.707 min
Delta R.T.: -0.010 min
Response: 47363
Conc: 0.36 ug/ml

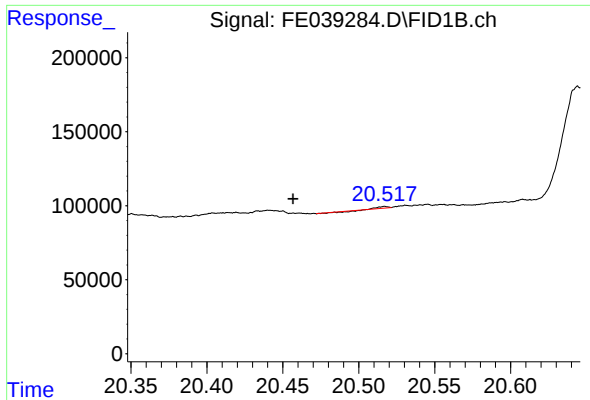

#20 n-Hexatriacontane (C36)

R.T.: 20.517 min
Delta R.T.: 0.060 min
Response: 612
Conc: 0.00 ug/ml

Instrument :
FID_E
ClientSampleId :

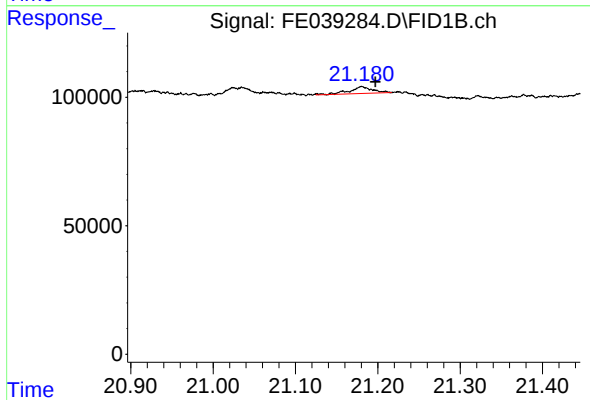

#21 n-Octatriacontane (C38)

R.T.: 21.180 min
Delta R.T.: -0.017 min
Response: 50411
Conc: 0.38 ug/ml