

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121322AL\
Data File : FE039292.D
Signal(s) : FID1B.ch
Acq On : 13 Dec 2022 23:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 02:17:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.720	89879	0.679 ug/ml
20) T	n-Hexatriacontane (C36)	20.449	49727	0.387 ug/ml
21) T	n-Octatriacontane (C38)	21.210	297549	2.271 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121322AL\
Data File : FE039292.D
Signal(s) : FID1B.ch
Acq On : 13 Dec 2022 23:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 02:17:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

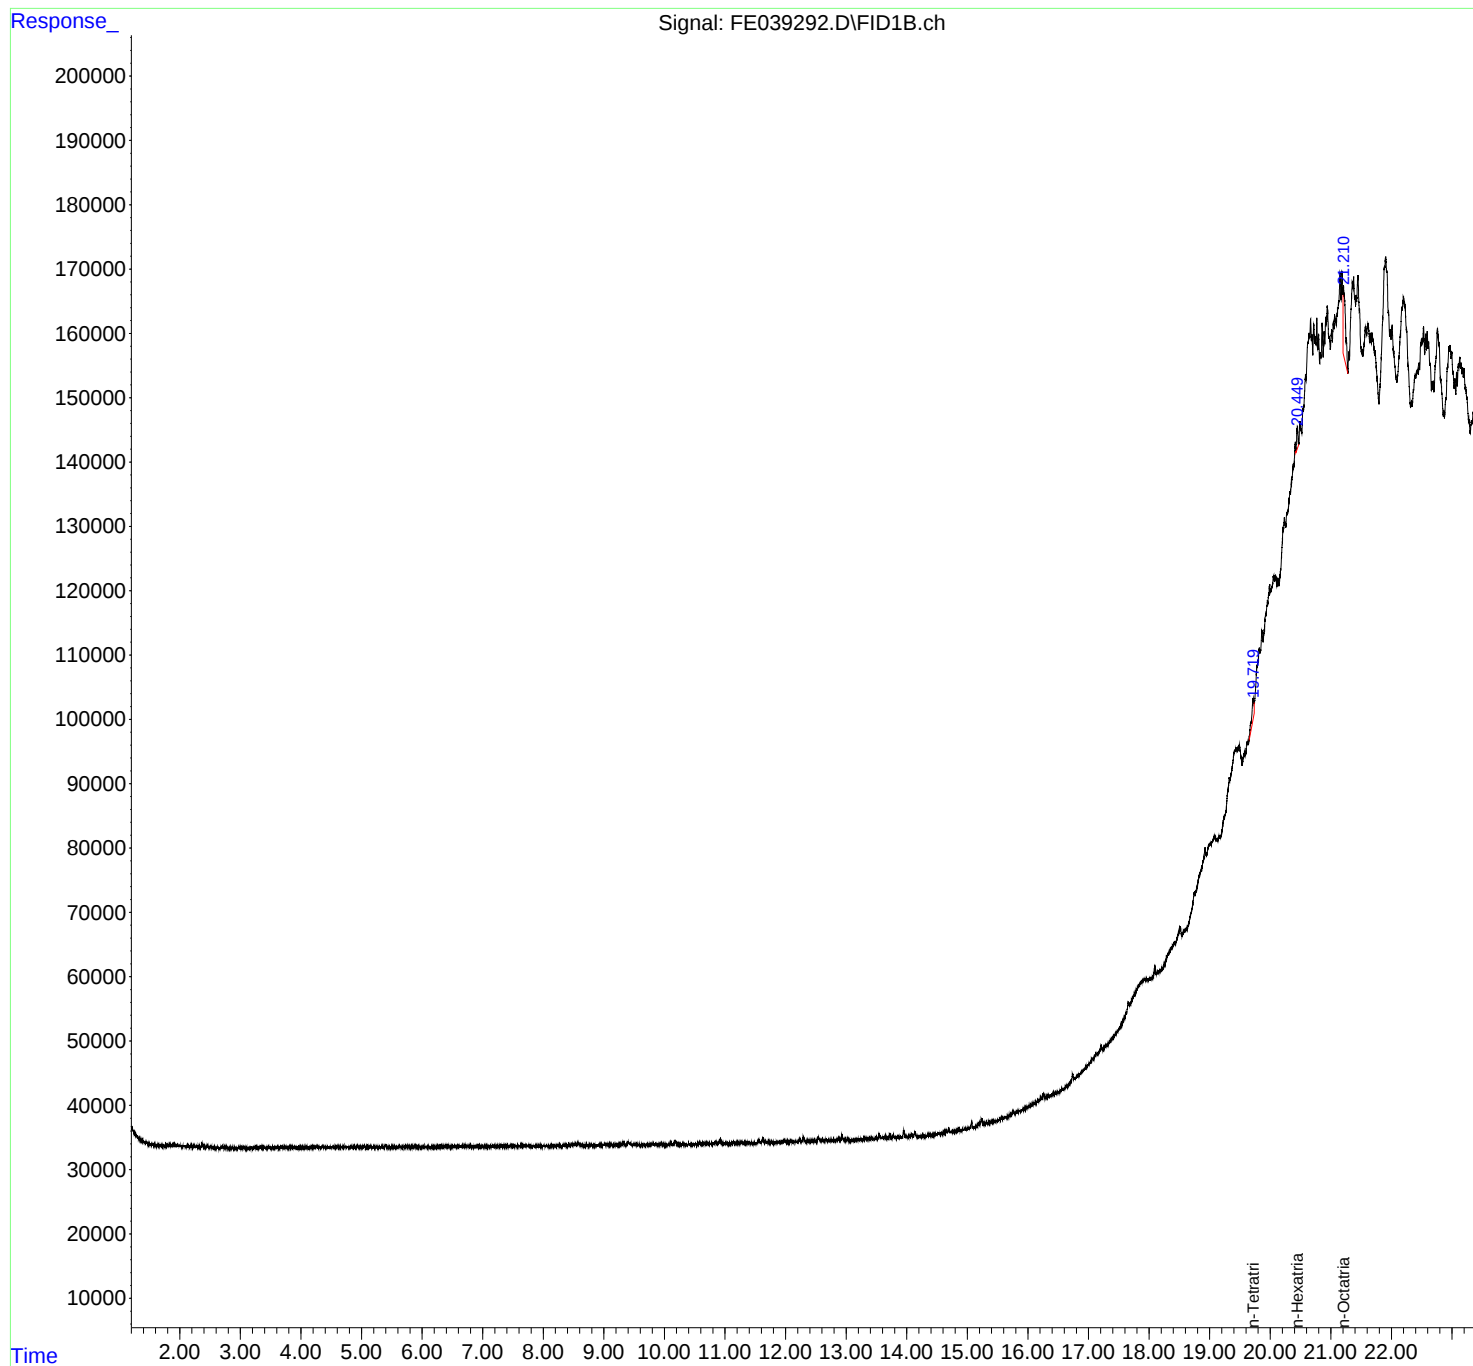


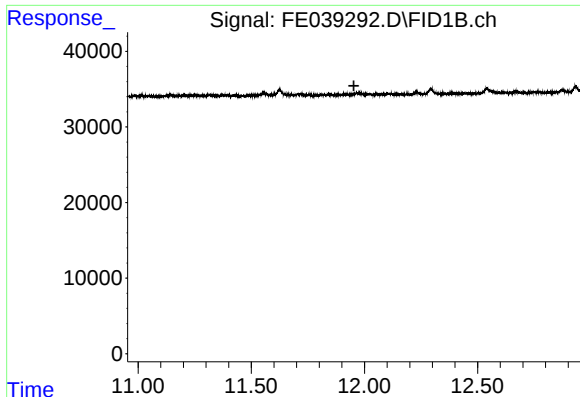

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.953 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

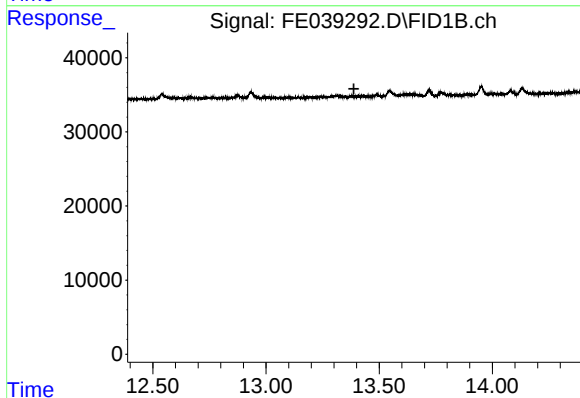


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.388 min
Response: 0
Conc: N.D.

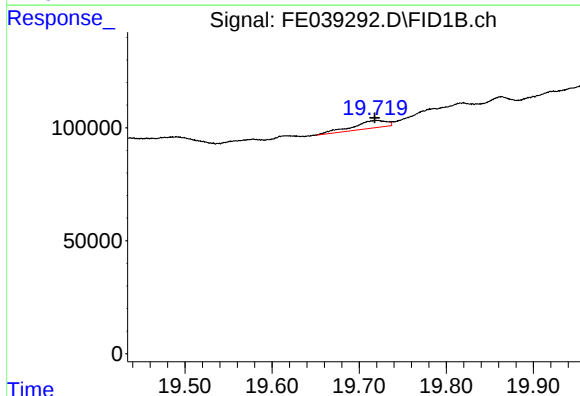


#19 n-Tetratriacontane (C34)

R.T.: 19.720 min
Delta R.T.: 0.002 min
Response: 89879
Conc: 0.68 ug/ml

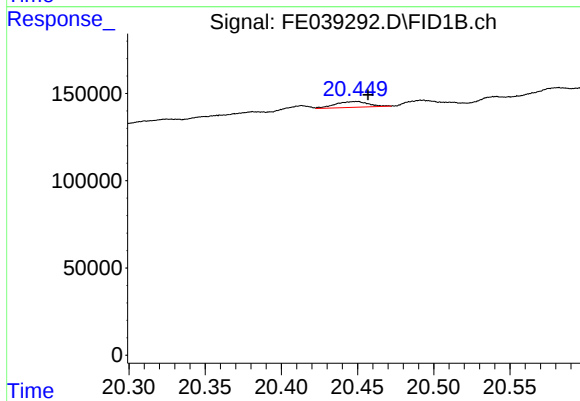

#20 n-Hexatriacontane (C36)

R.T.: 20.449 min
Delta R.T.: -0.008 min
Response: 49727
Conc: 0.39 ug/ml

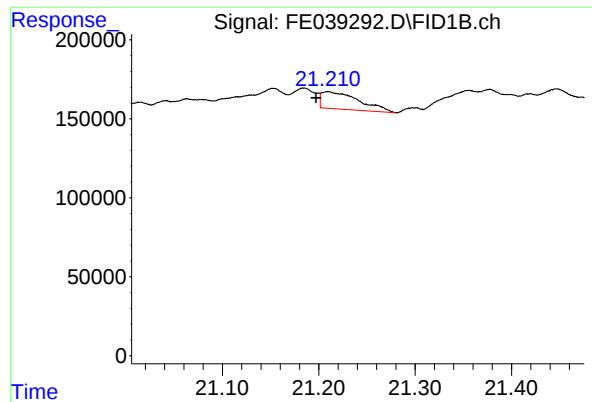

#21 n-Octatriacontane (C38)

R.T.: 21.210 min
Delta R.T.: 0.012 min
Response: 297549
Conc: 2.27 ug/ml

Instrument :

FID_E

ClientSampleId :