

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121422AL\
 Data File : FE039301.D
 Signal(s) : FID1B.ch
 Acq On : 14 Dec 2022 15:08
 Operator : YP\AJ
 Sample : PB149634BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 14 16:41:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.942	7975839	50.984 ug/ml
Spiked Amount 50.000		Recovery =	101.97%
12) S 1-chlorooctadecane (S...	13.378	6311748	52.276 ug/ml
Spiked Amount 50.000		Recovery =	104.55%
Target Compounds			
14) T n-Tetracosane (C24)	15.210	235929	1.708 ug/ml
17) T n-Tricontane (C30)	18.090	43637	0.330 ug/ml
18) T n-Dotriacontane (C32)	18.924	59697	0.448 ug/ml
19) T n-Tetratriacontane (C34)	19.707	58895	0.445 ug/ml
20) T n-Hexatriacontane (C36)	20.448	47592	0.370 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121422AL\
Data File : FE039301.D
Signal(s) : FID1B.ch
Acq On : 14 Dec 2022 15:08
Operator : YP\AJ
Sample : PB149634BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 16:41:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

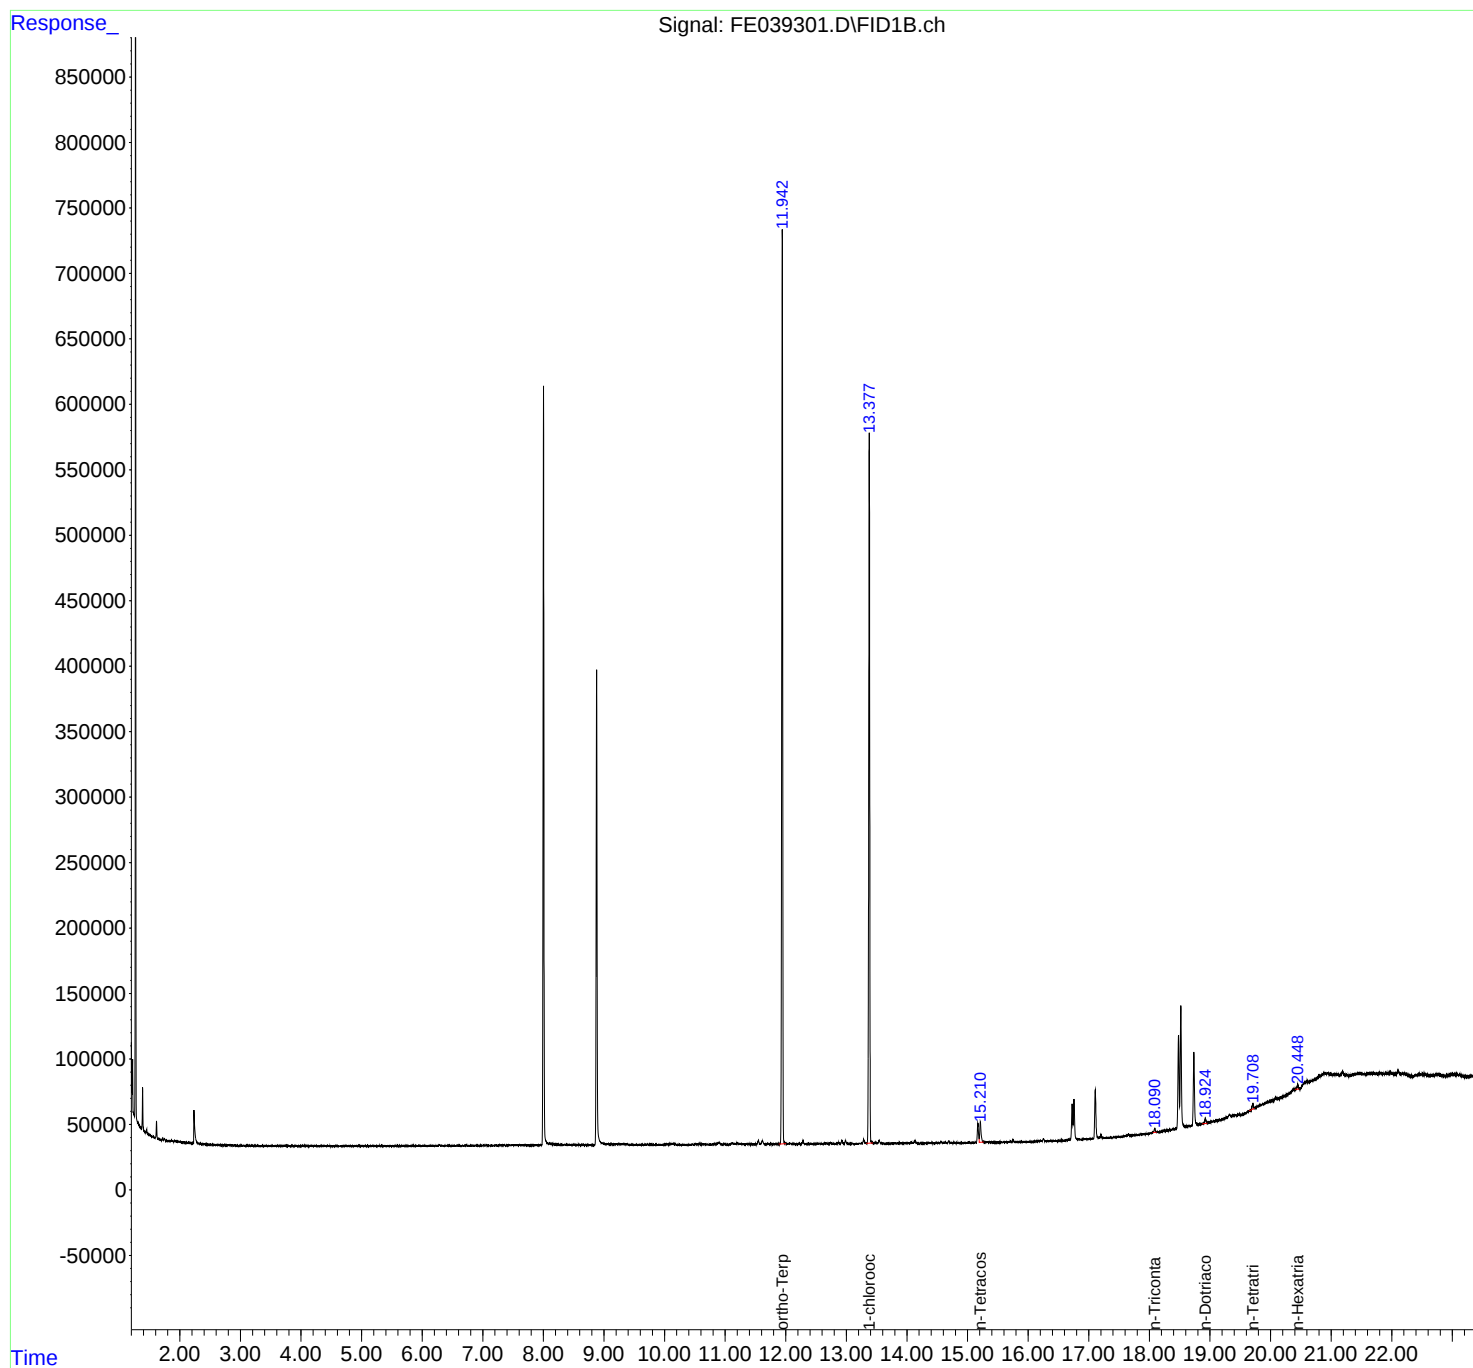


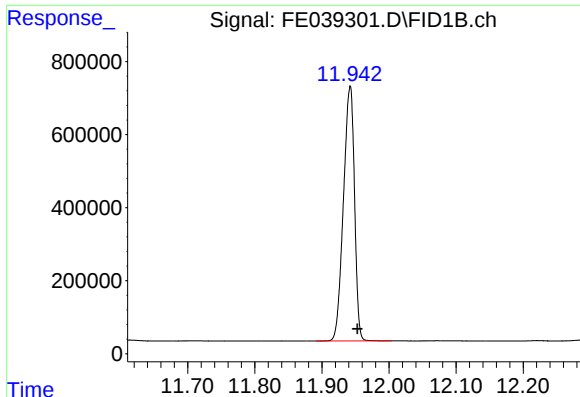

#9 ortho-Terphenyl (SURR)


R.T.: 11.942 min
Delta R.T.: -0.011 min
Response: 7975839
Conc: 50.98 ug/ml

Instrument :
FID_E
ClientSampleId :

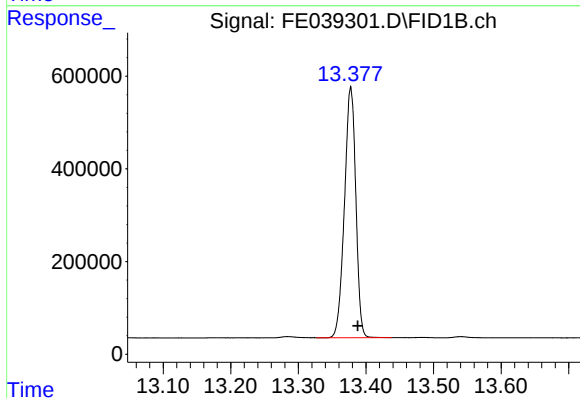


#12 1-chlorooctadecane (SURR)

R.T.: 13.378 min
Delta R.T.: -0.011 min
Response: 6311748
Conc: 52.28 ug/ml

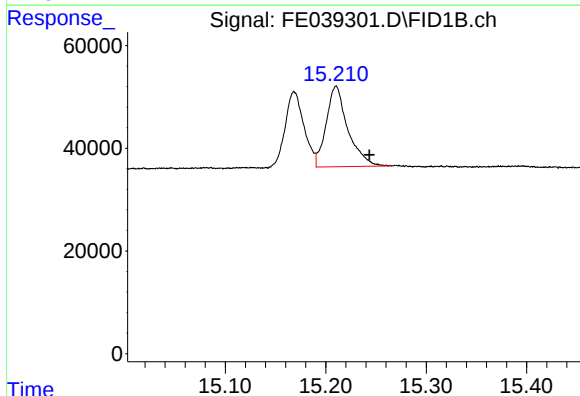


#14 n-Tetracosane (C24)

R.T.: 15.210 min
Delta R.T.: -0.033 min
Response: 235929
Conc: 1.71 ug/ml

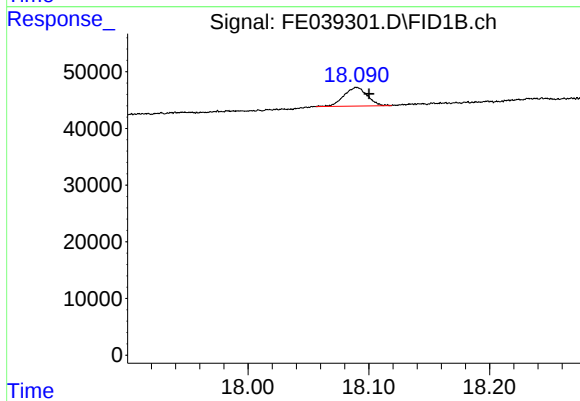

#17 n-Tricontane (C30)


R.T.: 18.090 min
Delta R.T.: -0.010 min
Response: 43637
Conc: 0.33 ug/ml

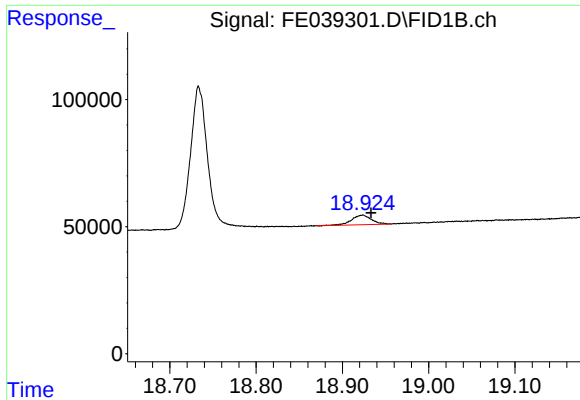

#18 n-Dotriacontane (C32)


R.T.: 18.924 min
Delta R.T.: -0.010 min
Response: 59697
Conc: 0.45 ug/ml

Instrument :
FID_E
ClientSampleId :

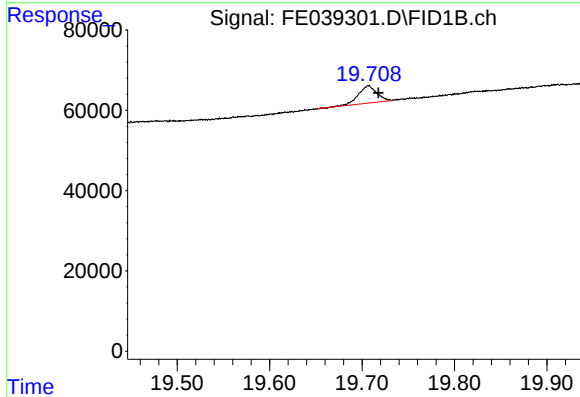

#19 n-Tetratriacontane (C34)

R.T.: 19.707 min
Delta R.T.: -0.011 min
Response: 58895
Conc: 0.45 ug/ml

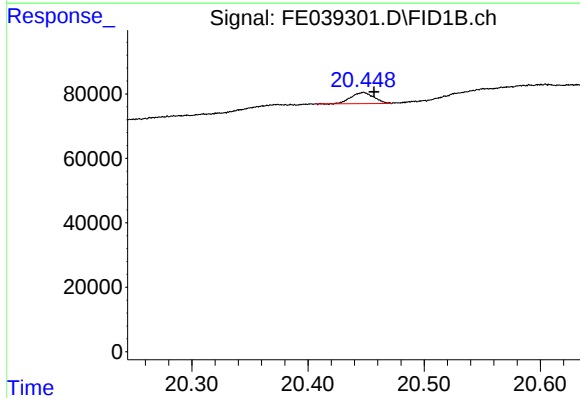

#20 n-Hexatriacontane (C36)

R.T.: 20.448 min
Delta R.T.: -0.009 min
Response: 47592
Conc: 0.37 ug/ml