

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121522AL\
 Data File : FE039324.D
 Signal(s) : FID1B.ch
 Acq On : 15 Dec 2022 11:46
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 15 15:07:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.917	59721	0.448 ug/ml
20) T n-Hexatriacontane (C36)	20.503	23735	0.185 ug/ml
21) T n-Octatriacontane (C38)	21.197	64708	0.494 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121522AL\
Data File : FE039324.D
Signal(s) : FID1B.ch
Acq On : 15 Dec 2022 11:46
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 15 15:07:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

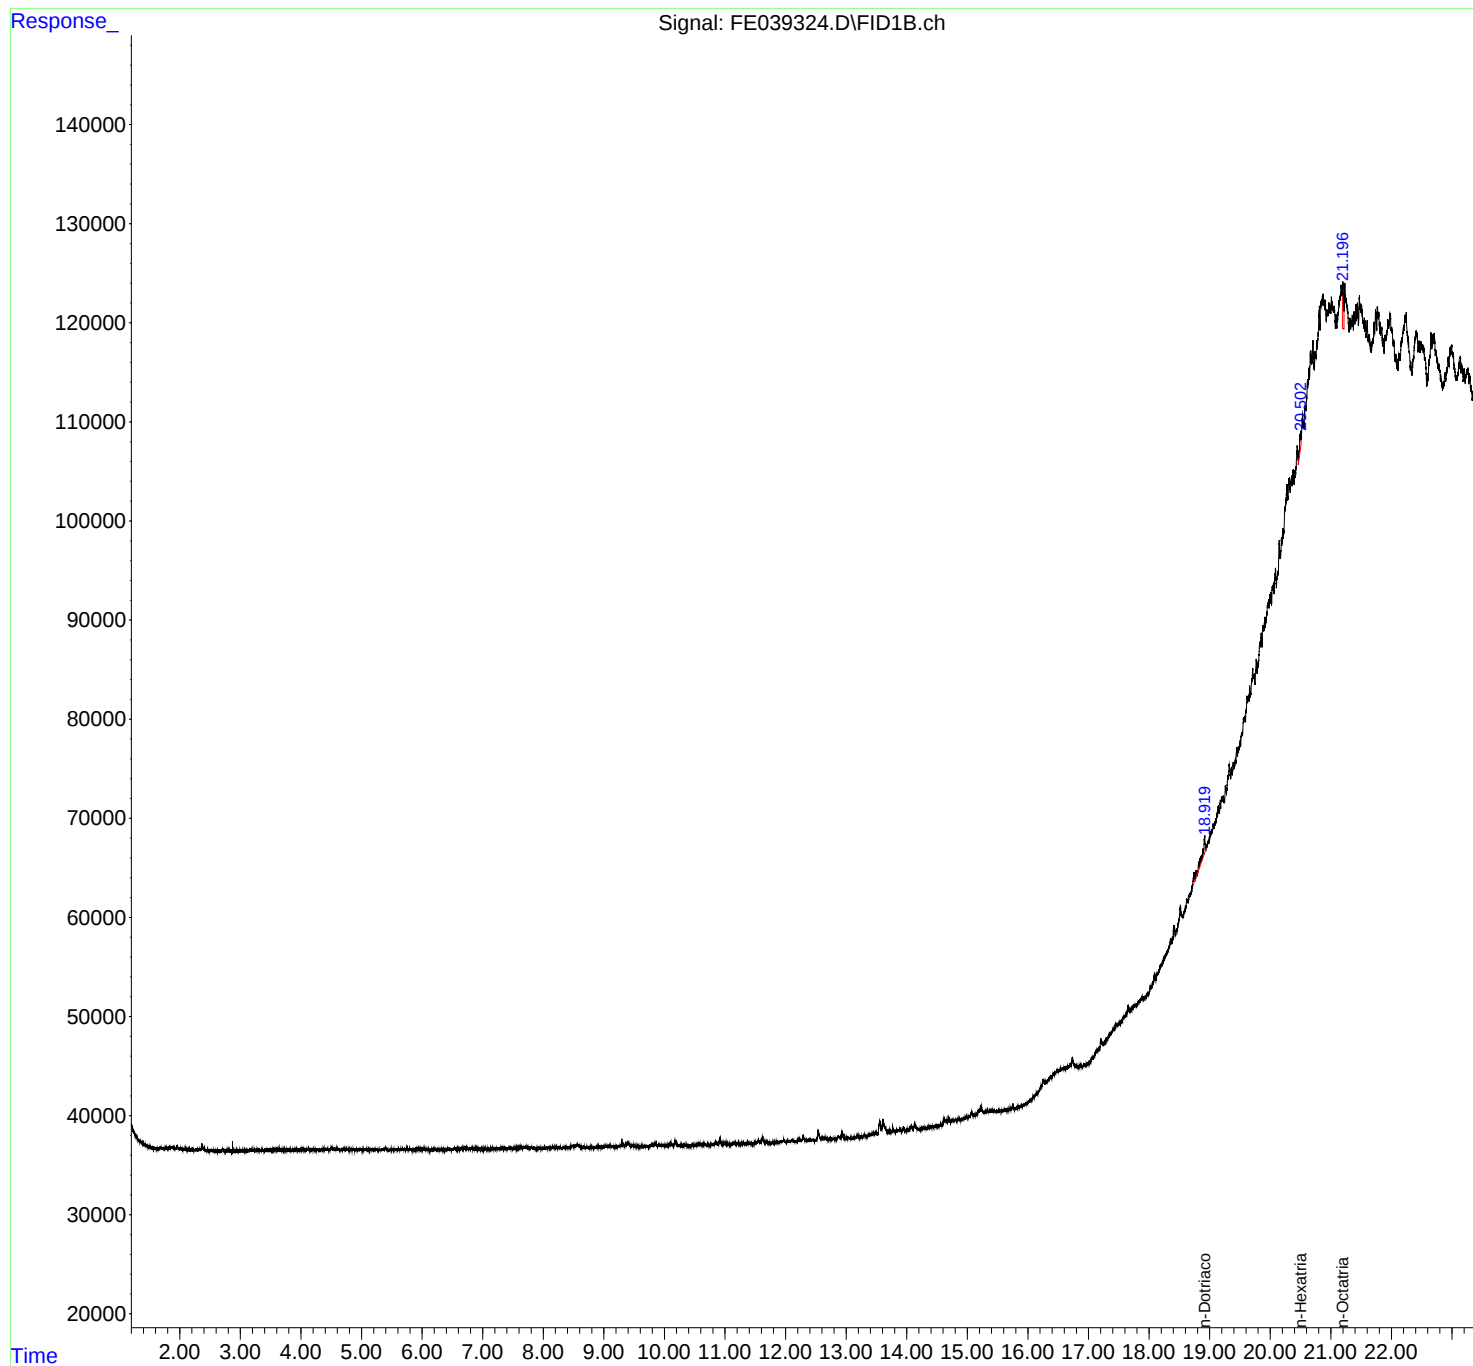


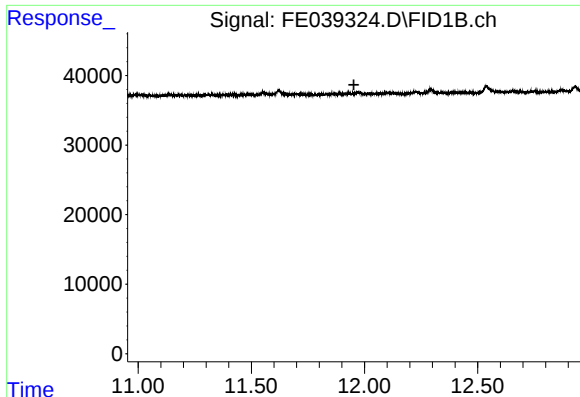

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.953 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

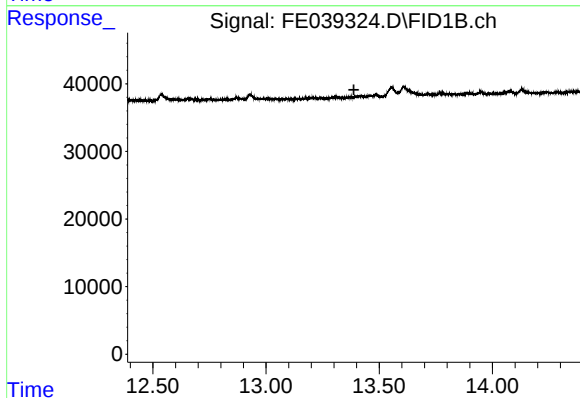


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.388 min
Response: 0
Conc: N.D.

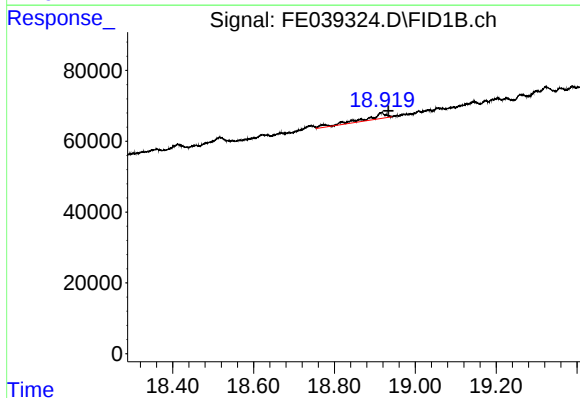


#18 n-Dotriacontane (C32)

R.T.: 18.917 min
Delta R.T.: -0.016 min
Response: 59721
Conc: 0.45 ug/ml

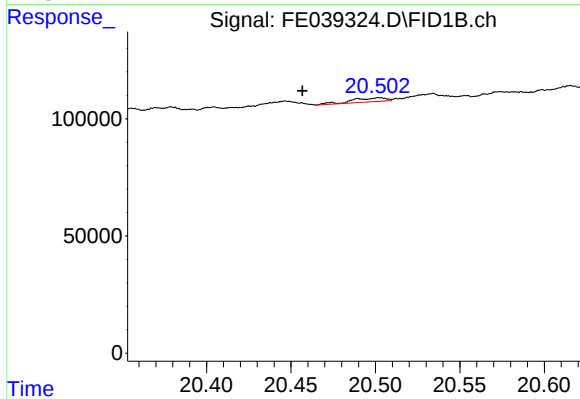

#20 n-Hexatriacontane (C36)

R.T.: 20.503 min
Delta R.T.: 0.046 min
Response: 23735
Conc: 0.18 ug/ml

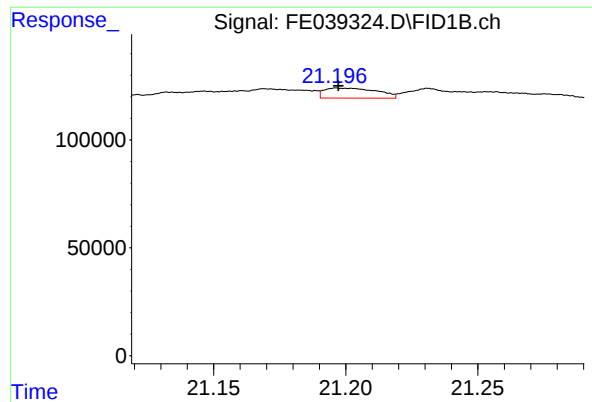

#21 n-Octatriacontane (C38)

R.T.: 21.197 min
Delta R.T.: 0.000 min
Response: 64708
Conc: 0.49 ug/ml

Instrument :
FID_E
ClientSampleId :