

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121622AL\
 Data File : FE039340.D
 Signal(s) : FID1B.ch
 Acq On : 16 Dec 2022 08:21
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 11:50:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 19 05:37:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.921	195681	1.378 ug/ml
11) T	n-Heneicosane (C21)	13.539	183303	1.290 ug/ml
13) T	n-Docosane (C22)	14.128	182509	1.306 ug/ml
14) T	n-Tetracosane (C24)	15.233	144951	1.050 ug/ml
15) T	n-Hexacosane (C26)	16.253	104703	0.780 ug/ml
16) T	n-Octacosane (C28)	17.207	93033	0.701 ug/ml
17) T	n-Tricontane (C30)	18.093	89507	0.678 ug/ml
18) T	n-Dotriacontane (C32)	18.927	144467	1.083 ug/ml
19) T	n-Tetratriacontane (C34)	19.713	54110	0.409 ug/ml
20) T	n-Hexatriacontane (C36)	20.452	59582	0.464 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121622AL\
Data File : FE039340.D
Signal(s) : FID1B.ch
Acq On : 16 Dec 2022 08:21
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 11:50:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 111922.M
Quant Title : GC Extractables
QLast Update : Sat Nov 19 05:37:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

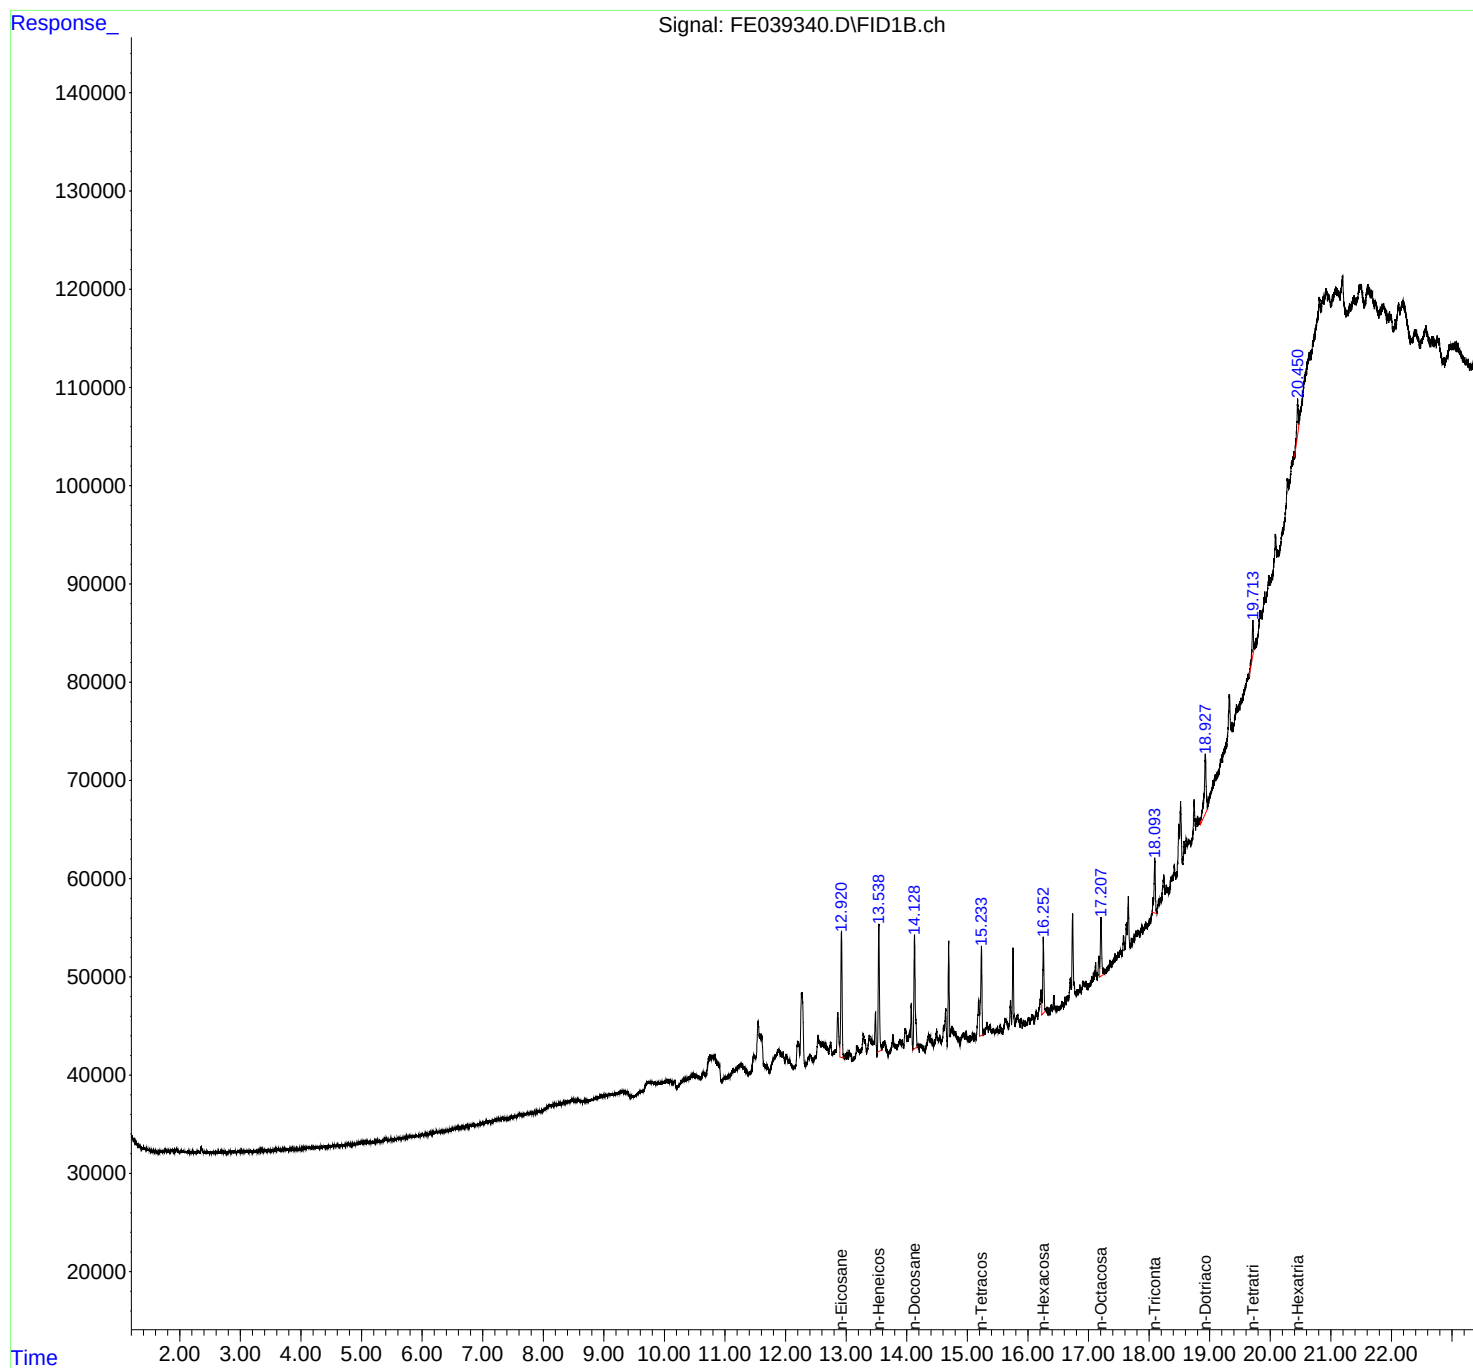


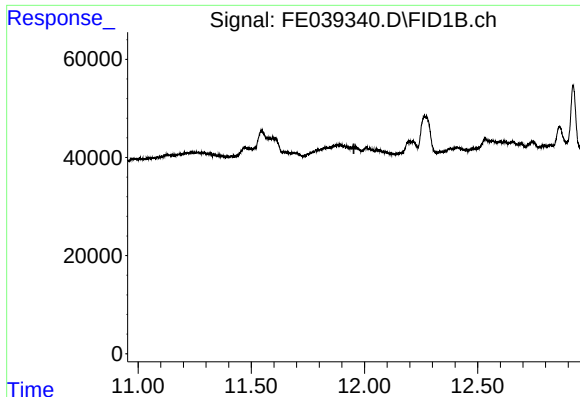

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.953 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

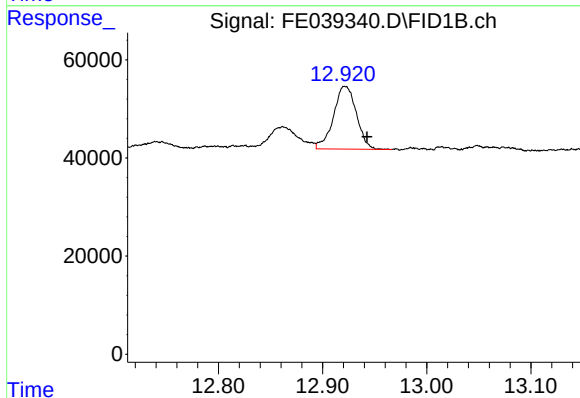


#10 n-Eicosane (C20)

R.T.: 12.921 min
Delta R.T.: -0.021 min
Response: 195681
Conc: 1.38 ug/ml

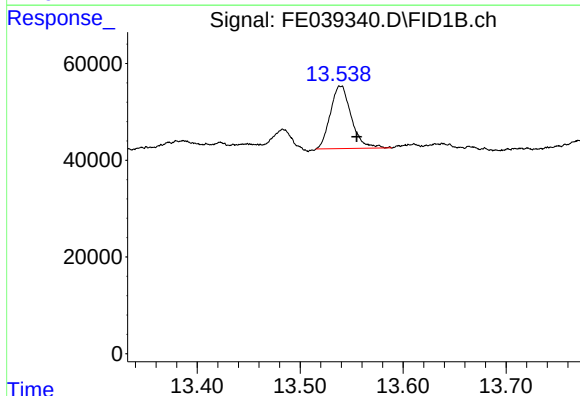


#11 n-Heneicosane (C21)

R.T.: 13.539 min
Delta R.T.: -0.015 min
Response: 183303
Conc: 1.29 ug/ml

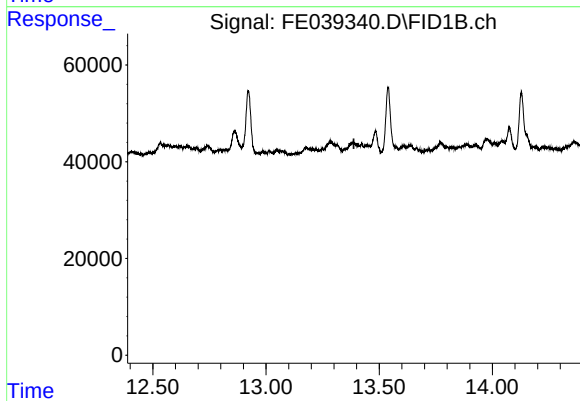

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.388 min
Response: 0
Conc: N.D.

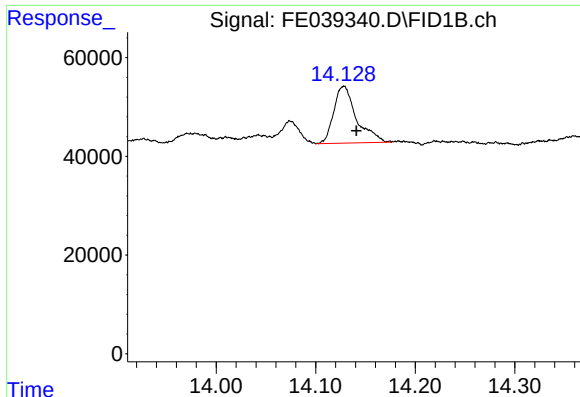

#13 n-Docosane (C22)


R.T.: 14.128 min
Delta R.T.: -0.013 min
Response: 182509
Conc: 1.31 ug/ml

Instrument :
FID_E
ClientSampleId :

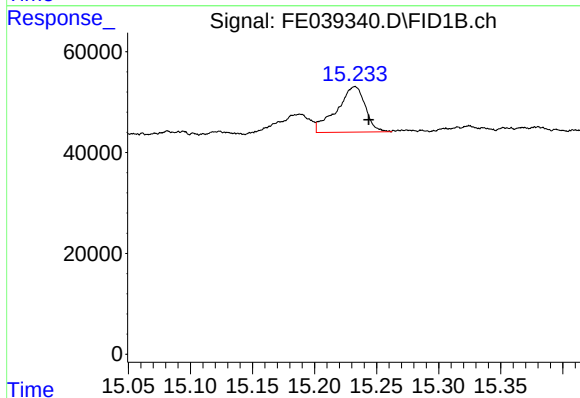


#14 n-Tetracosane (C24)

R.T.: 15.233 min
Delta R.T.: -0.011 min
Response: 144951
Conc: 1.05 ug/ml

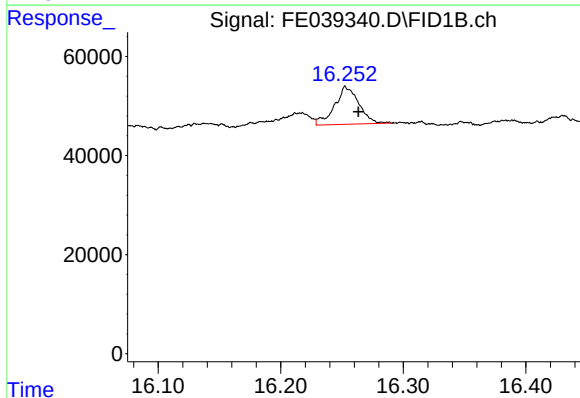


#15 n-Hexacosane (C26)

R.T.: 16.253 min
Delta R.T.: -0.010 min
Response: 104703
Conc: 0.78 ug/ml

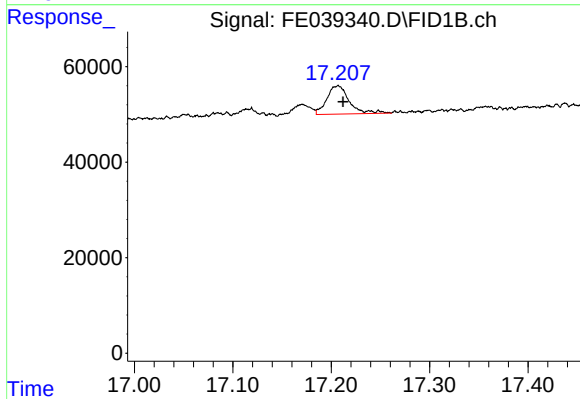

#16 n-Octacosane (C28)


R.T.: 17.207 min
Delta R.T.: -0.005 min
Response: 93033
Conc: 0.70 ug/ml

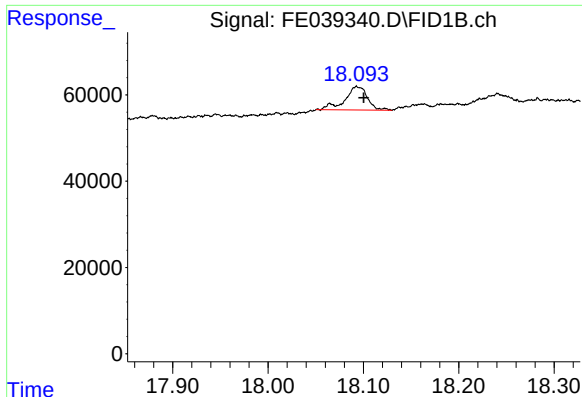

#17 n-Tricontane (C30)


R.T.: 18.093 min
Delta R.T.: -0.007 min
Response: 89507
Conc: 0.68 ug/ml

Instrument :
FID_E
ClientSampleId :

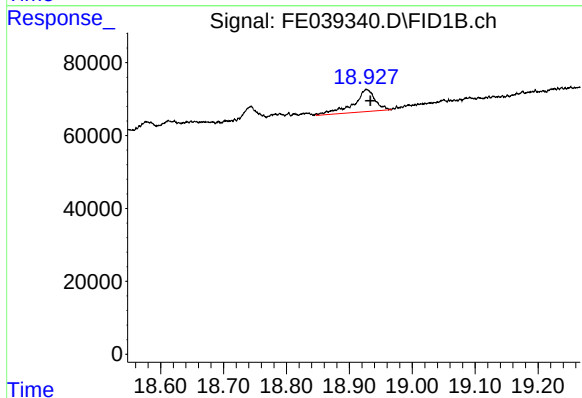


#18 n-Dotriacontane (C32)

R.T.: 18.927 min
Delta R.T.: -0.006 min
Response: 144467
Conc: 1.08 ug/ml

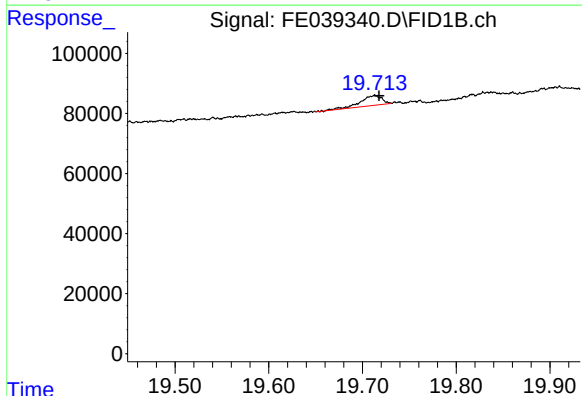

#19 n-Tetratriacontane (C34)

R.T.: 19.713 min
Delta R.T.: -0.005 min
Response: 54110
Conc: 0.41 ug/ml

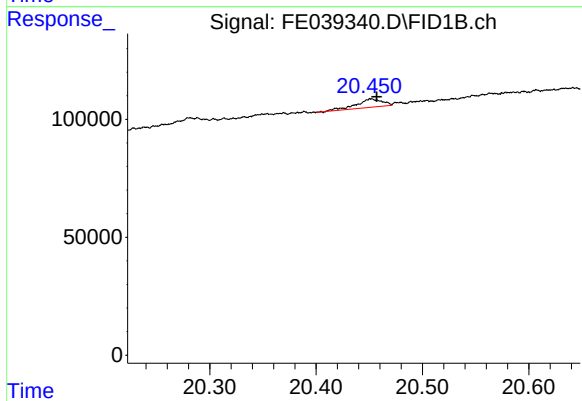

#20 n-Hexatriacontane (C36)

R.T.: 20.452 min
Delta R.T.: -0.005 min
Response: 59582
Conc: 0.46 ug/ml