

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121922AL\
 Data File : FE039387.D
 Signal(s) : FID1B.ch
 Acq On : 19 Dec 2022 18:50
 Operator : YP\AJ
 Sample : N6098-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 20 04:47:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 17 15:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.937	4327421	28.998 ug/ml
Spiked Amount 50.000		Recovery =	58.00%
12) S 1-chlorooctadecane (S...	13.372	3358271	29.177 ug/ml
Spiked Amount 50.000		Recovery =	58.35%
Target Compounds			
10) T n-Eicosane (C20)	12.989f	144057	1.055 ug/ml
14) T n-Tetracosane (C24)	15.210	67077	0.500 ug/ml
16) T n-Octacosane (C28)	17.244	76113	0.591 ug/ml
17) T n-Tricontane (C30)	18.085	52849	0.410 ug/ml
18) T n-Dotriacontane (C32)	18.916	112734	0.871 ug/ml
19) T n-Tetratriacontane (C34)	19.702	59270	0.470 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121922AL\
Data File : FE039387.D
Signal(s) : FID1B.ch
Acq On : 19 Dec 2022 18:50
Operator : YP\AJ
Sample : N6098-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 20 04:47:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
Quant Title : GC Extractables
QLast Update : Sat Dec 17 15:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

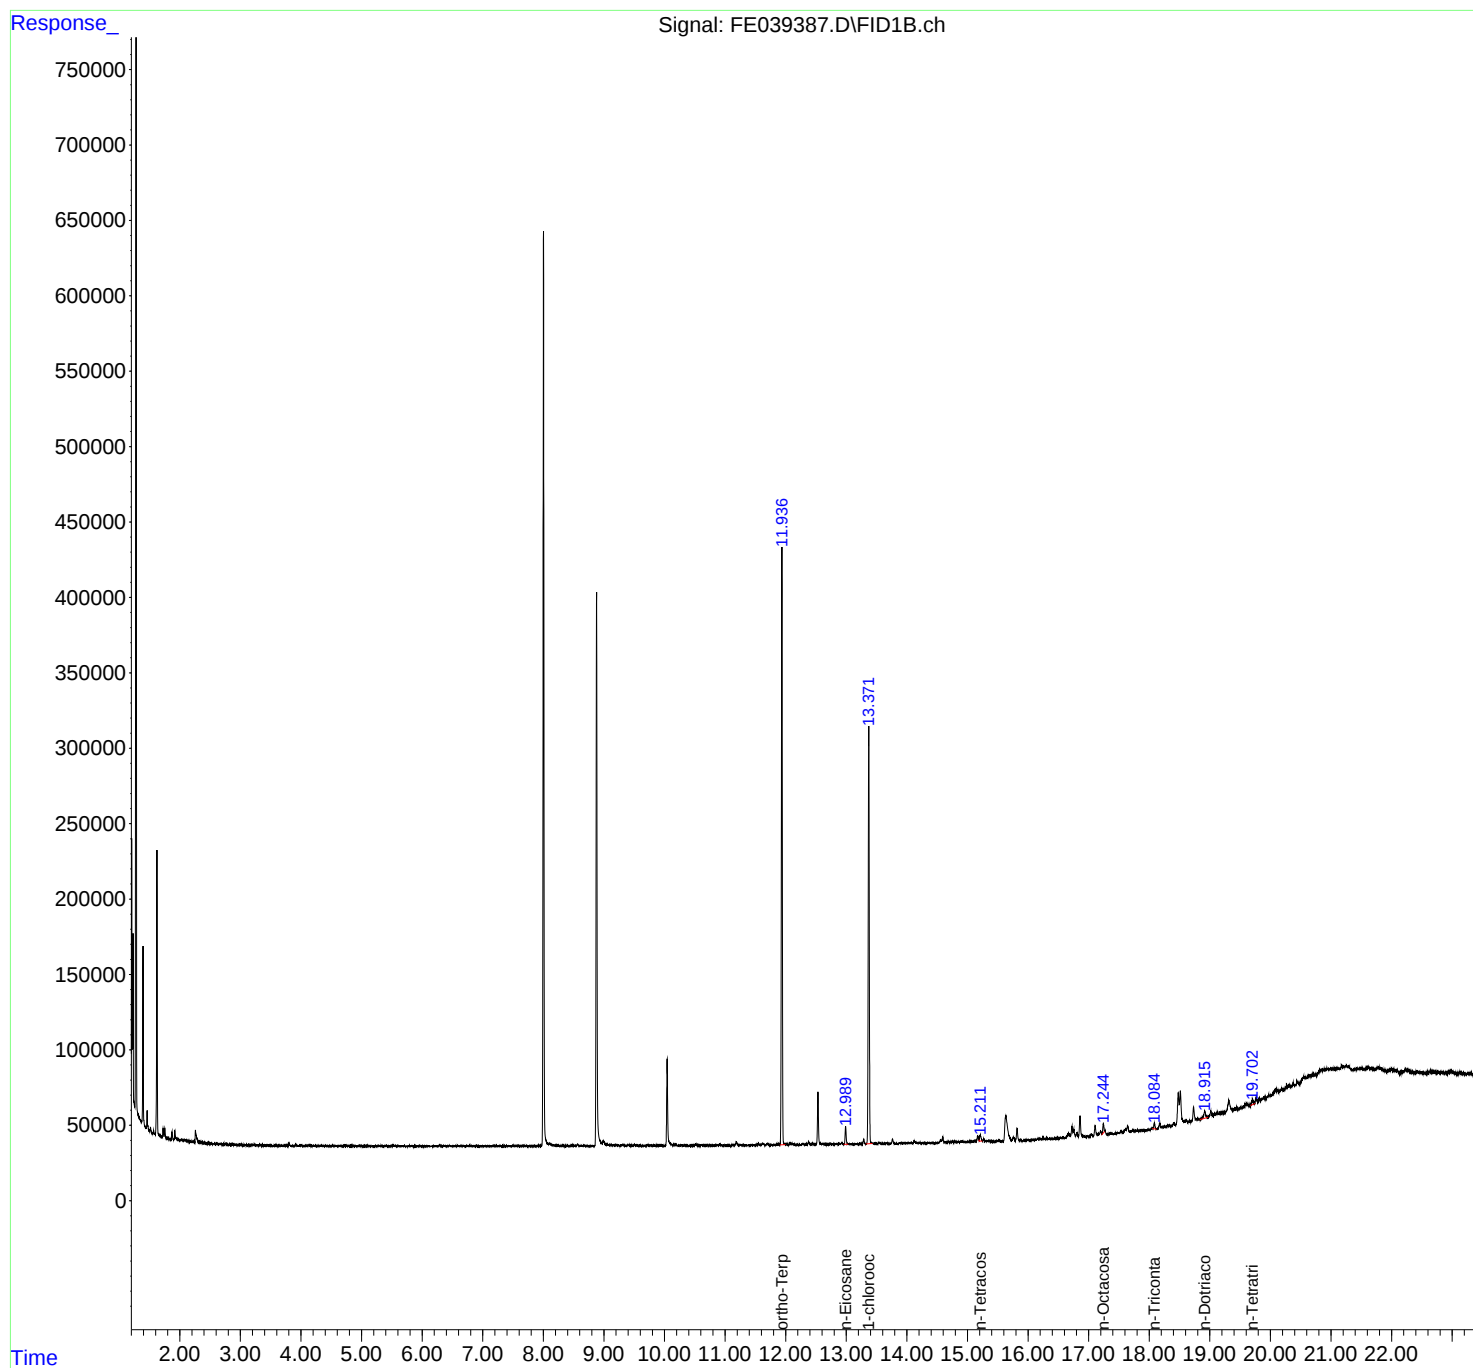


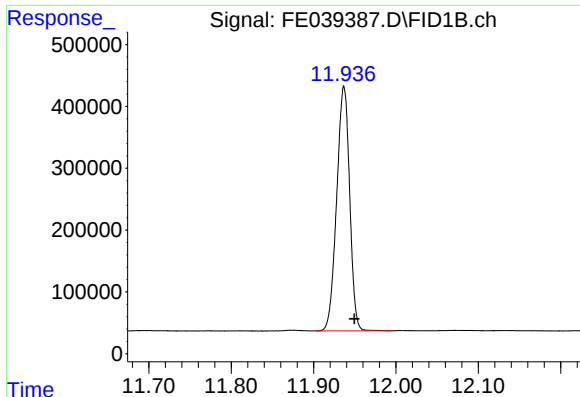

#9 ortho-Terphenyl (SURR)


R.T.: 11.937 min
Delta R.T.: -0.013 min
Response: 4327421
Conc: 29.00 ug/ml

Instrument :
FID_E
ClientSampleId :

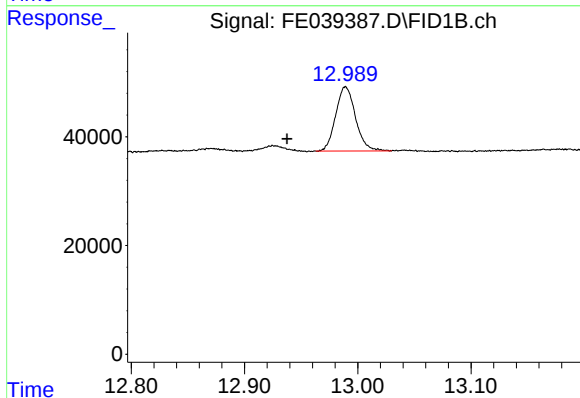


#10 n-Eicosane (C20)

R.T.: 12.989 min
Delta R.T.: 0.052 min
Response: 144057
Conc: 1.06 ug/ml

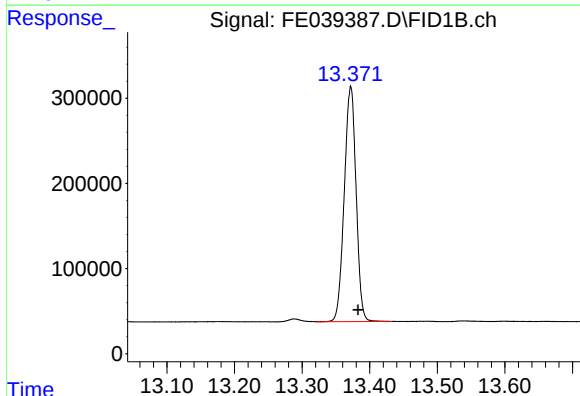


#12 1-chlorooctadecane (SURR)

R.T.: 13.372 min
Delta R.T.: -0.011 min
Response: 3358271
Conc: 29.18 ug/ml

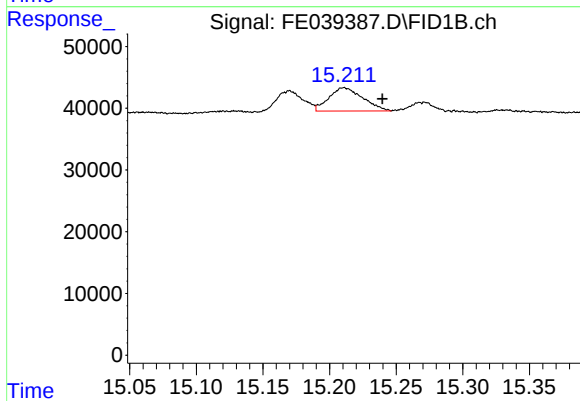

#14 n-Tetracosane (C24)


R.T.: 15.210 min
Delta R.T.: -0.029 min
Response: 67077
Conc: 0.50 ug/ml

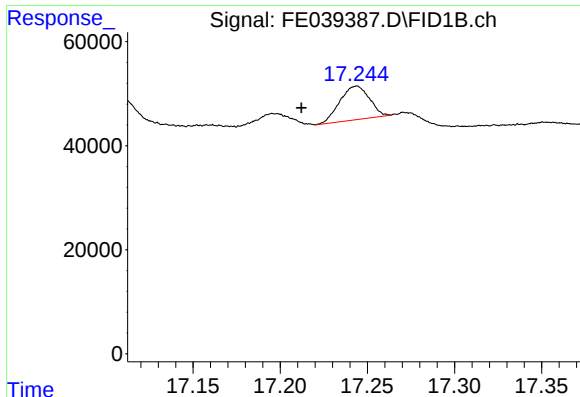

#16 n-Octacosane (C28)


R.T.: 17.244 min
Delta R.T.: 0.032 min
Response: 76113
Conc: 0.59 ug/ml

Instrument :
FID_E
ClientSampleId :

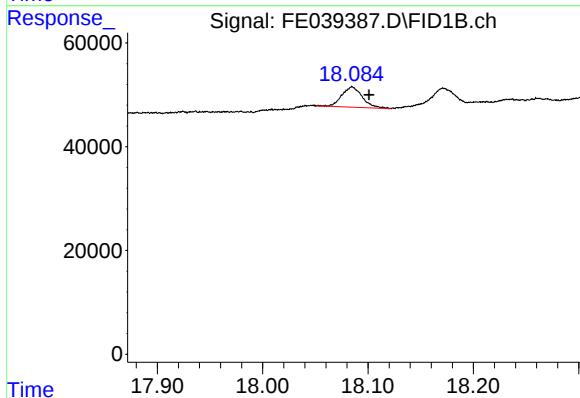


#17 n-Tricontane (C30)

R.T.: 18.085 min
Delta R.T.: -0.016 min
Response: 52849
Conc: 0.41 ug/ml

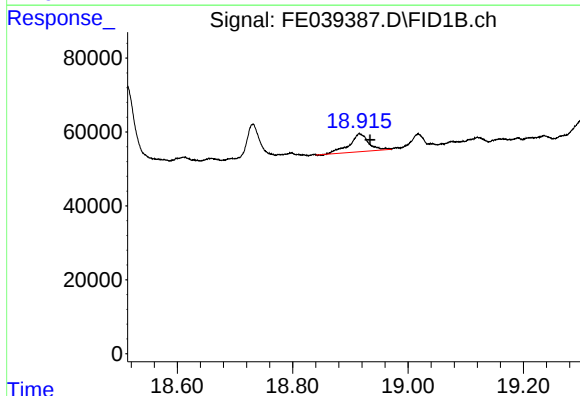

#18 n-Dotriacontane (C32)

R.T.: 18.916 min
Delta R.T.: -0.018 min
Response: 112734
Conc: 0.87 ug/ml

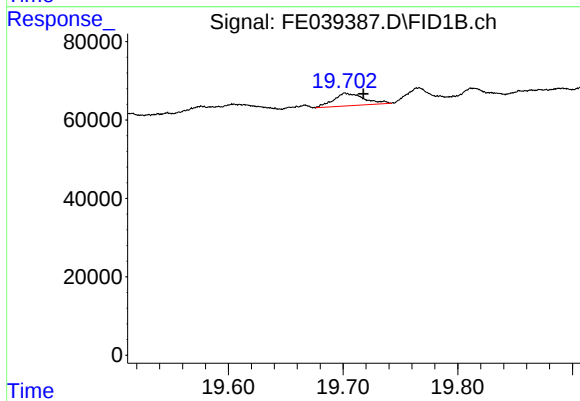

#19 n-Tetratriacontane (C34)

R.T.: 19.702 min
Delta R.T.: -0.016 min
Response: 59270
Conc: 0.47 ug/ml