

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121922AL\
 Data File : FE039388.D
 Signal(s) : FID1B.ch
 Acq On : 19 Dec 2022 19:21
 Operator : YP\AJ
 Sample : N6098-01D
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 20 04:48:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 17 15:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.936	4277110	28.661 ug/ml
Spiked Amount 50.000		Recovery =	57.32%
12) S 1-chlorooctadecane (S...	13.372	3308380	28.744 ug/ml
Spiked Amount 50.000		Recovery =	57.49%
Target Compounds			
10) T n-Eicosane (C20)	12.989f	139652	1.023 ug/ml
16) T n-Octacosane (C28)	17.244	71543	0.556 ug/ml
17) T n-Tricontane (C30)	18.084	63158	0.491 ug/ml
18) T n-Dotriacontane (C32)	18.915	116067	0.896 ug/ml
19) T n-Tetratriacontane (C34)	19.701	55740	0.442 ug/ml
20) T n-Hexatriacontane (C36)	20.441	40527	0.335 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121922AL\
Data File : FE039388.D
Signal(s) : FID1B.ch
Acq On : 19 Dec 2022 19:21
Operator : YP\AJ
Sample : N6098-01D
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 20 04:48:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
Quant Title : GC Extractables
QLast Update : Sat Dec 17 15:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

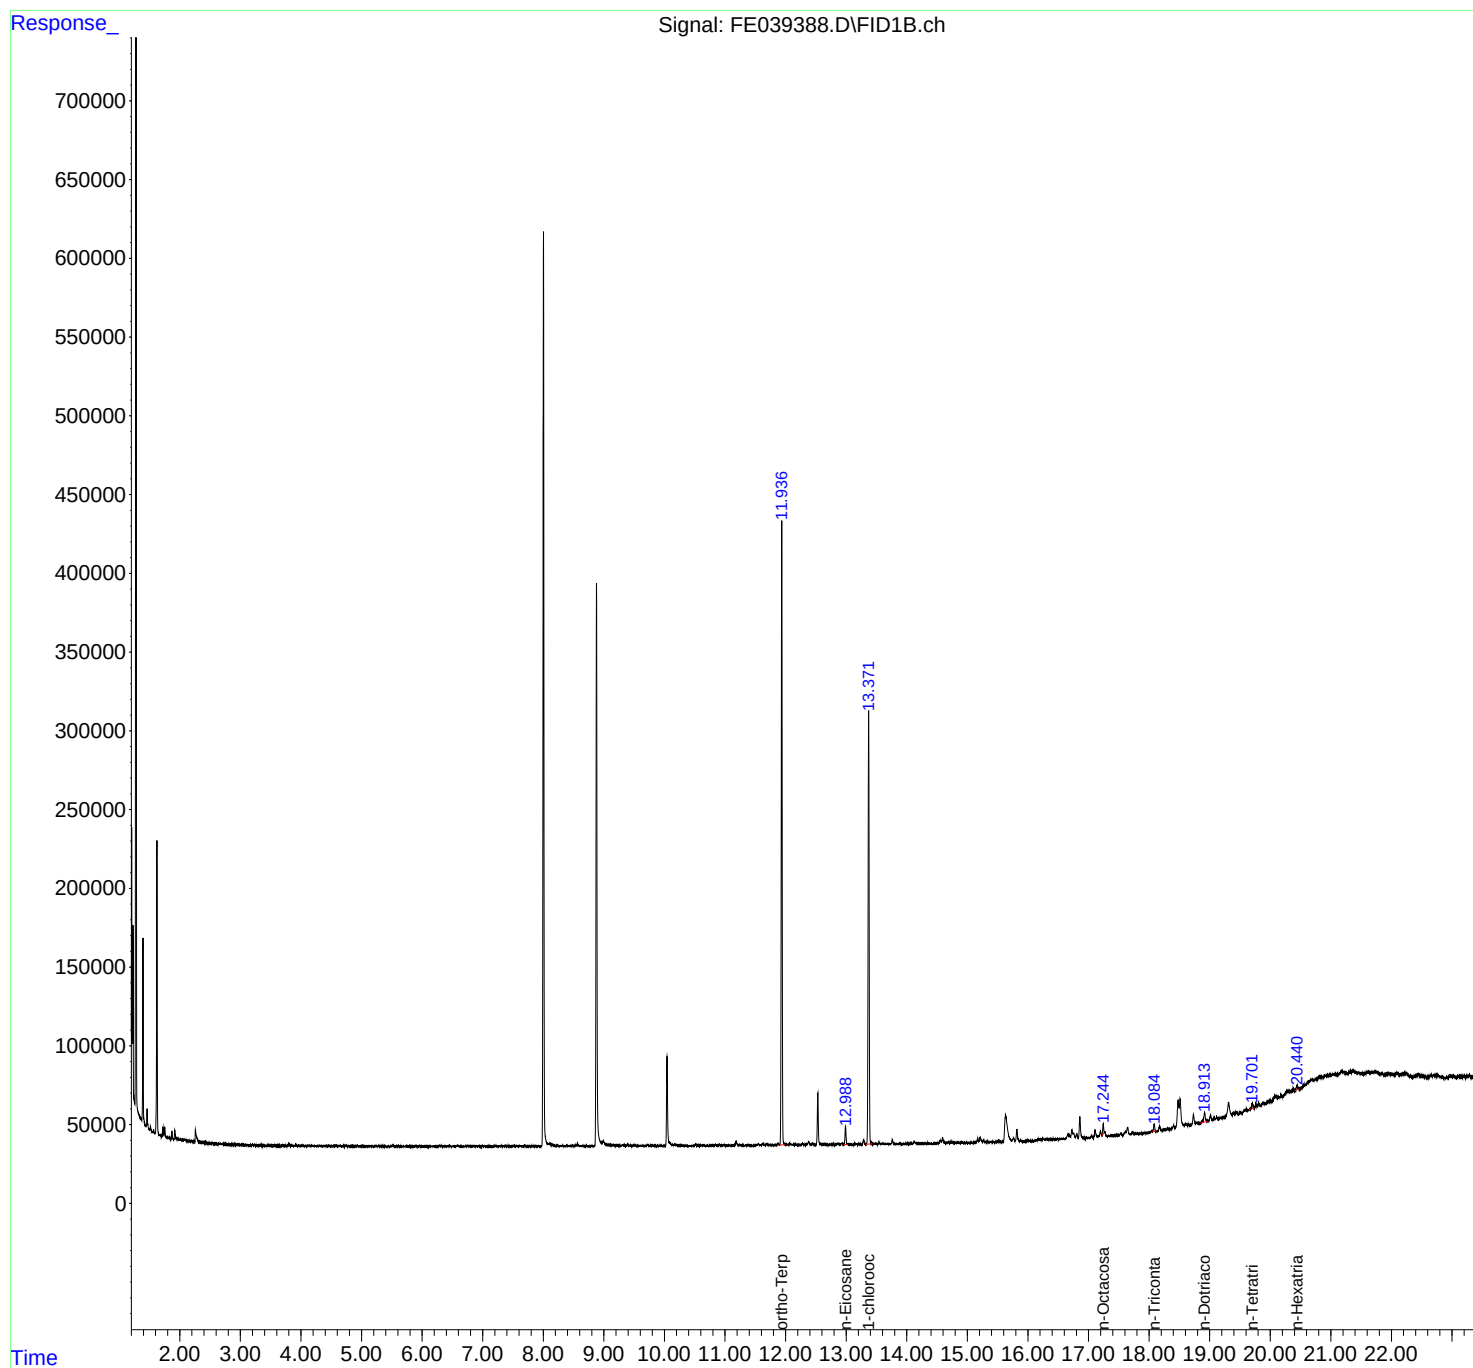


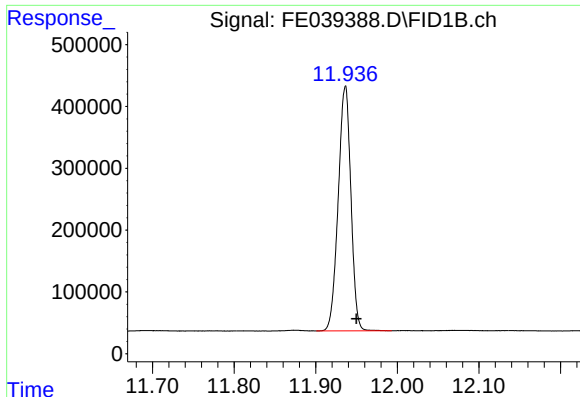

#9 ortho-Terphenyl (SURR)


R.T.: 11.936 min
Delta R.T.: -0.013 min
Response: 4277110
Conc: 28.66 ug/ml

Instrument :
FID_E
ClientSampleId :

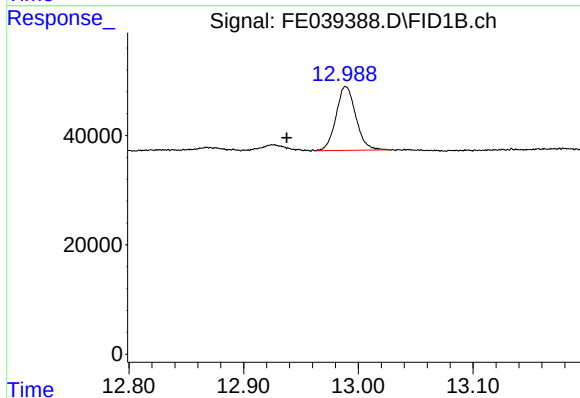


#10 n-Eicosane (C20)

R.T.: 12.989 min
Delta R.T.: 0.051 min
Response: 139652
Conc: 1.02 ug/ml

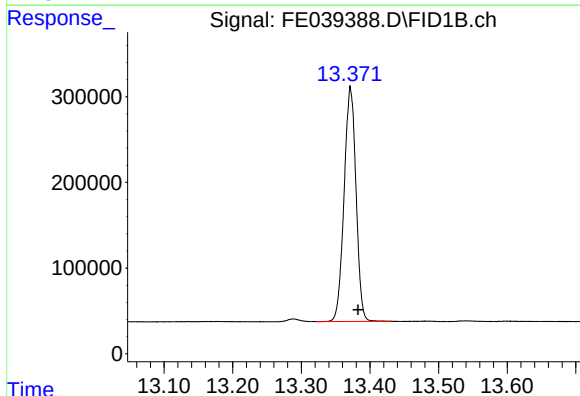


#12 1-chlorooctadecane (SURR)

R.T.: 13.372 min
Delta R.T.: -0.011 min
Response: 3308380
Conc: 28.74 ug/ml

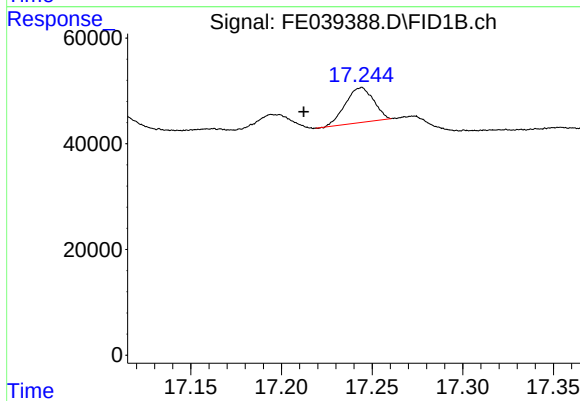

#16 n-Octacosane (C28)


R.T.: 17.244 min
Delta R.T.: 0.032 min
Response: 71543
Conc: 0.56 ug/ml

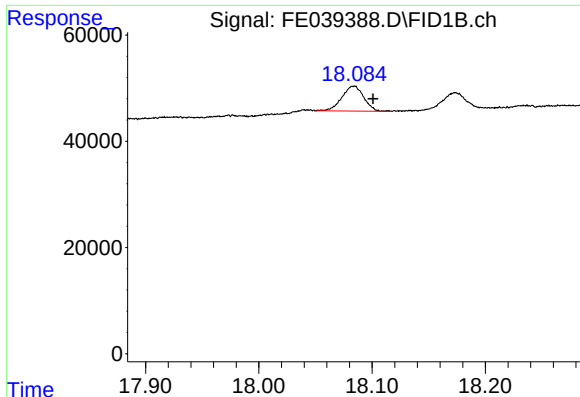

#17 n-Tricontane (C30)


R.T.: 18.084 min
Delta R.T.: -0.017 min
Response: 63158
Conc: 0.49 ug/ml

Instrument :
FID_E
ClientSampleId :

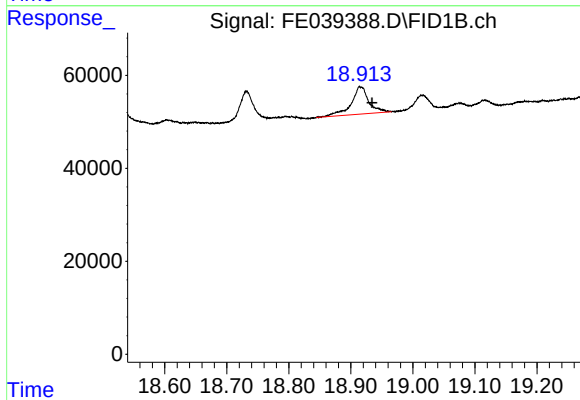


#18 n-Dotriacontane (C32)

R.T.: 18.915 min
Delta R.T.: -0.019 min
Response: 116067
Conc: 0.90 ug/ml

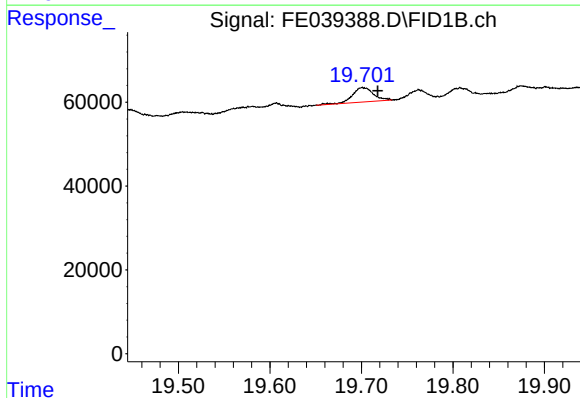

#19 n-Tetratriacontane (C34)

R.T.: 19.701 min
Delta R.T.: -0.017 min
Response: 55740
Conc: 0.44 ug/ml

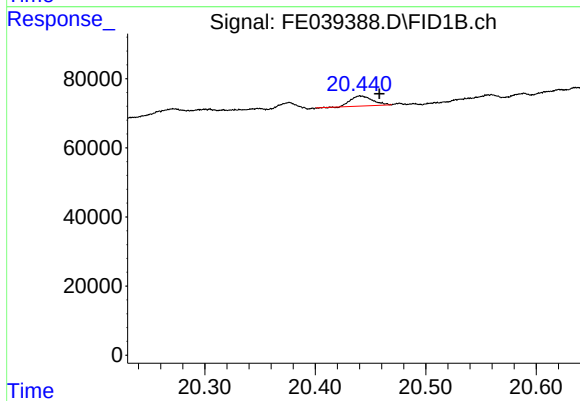

#20 n-Hexatriacontane (C36)

R.T.: 20.441 min
Delta R.T.: -0.017 min
Response: 40527
Conc: 0.34 ug/ml