

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE121922AL\  
 Data File : FE039377.D  
 Signal(s) : FID1B.ch  
 Acq On : 19 Dec 2022 11:37  
 Operator : YP\AJ  
 Sample : N6071-05DL 10X  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 FVSUB-TP7-COMP-07DL

Integration File: autoint1.e  
 Quant Time: Dec 19 14:15:24 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 121722.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Dec 17 15:09:52 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units  |
|--------------------------------|--------|------------|-------------|
| -----                          |        |            |             |
| System Monitoring Compounds    |        |            |             |
| 9) S ortho-Terphenyl (SURR)    | 11.936 | 365167     | 2.447 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 4.89%       |
| 12) S 1-chlorooctadecane (S... | 13.372 | 291117     | 2.529 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 5.06%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE121922AL\  
Data File : FE039377.D  
Signal(s) : FID1B.ch  
Acq On : 19 Dec 2022 11:37  
Operator : YP\AJ  
Sample : N6071-05DL 10X  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
FVSUB-TP7-COMP-07DL

Integration File: autoint1.e  
Quant Time: Dec 19 14:15:24 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 121722.M  
Quant Title : GC Extractables  
QLast Update : Sat Dec 17 15:09:52 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

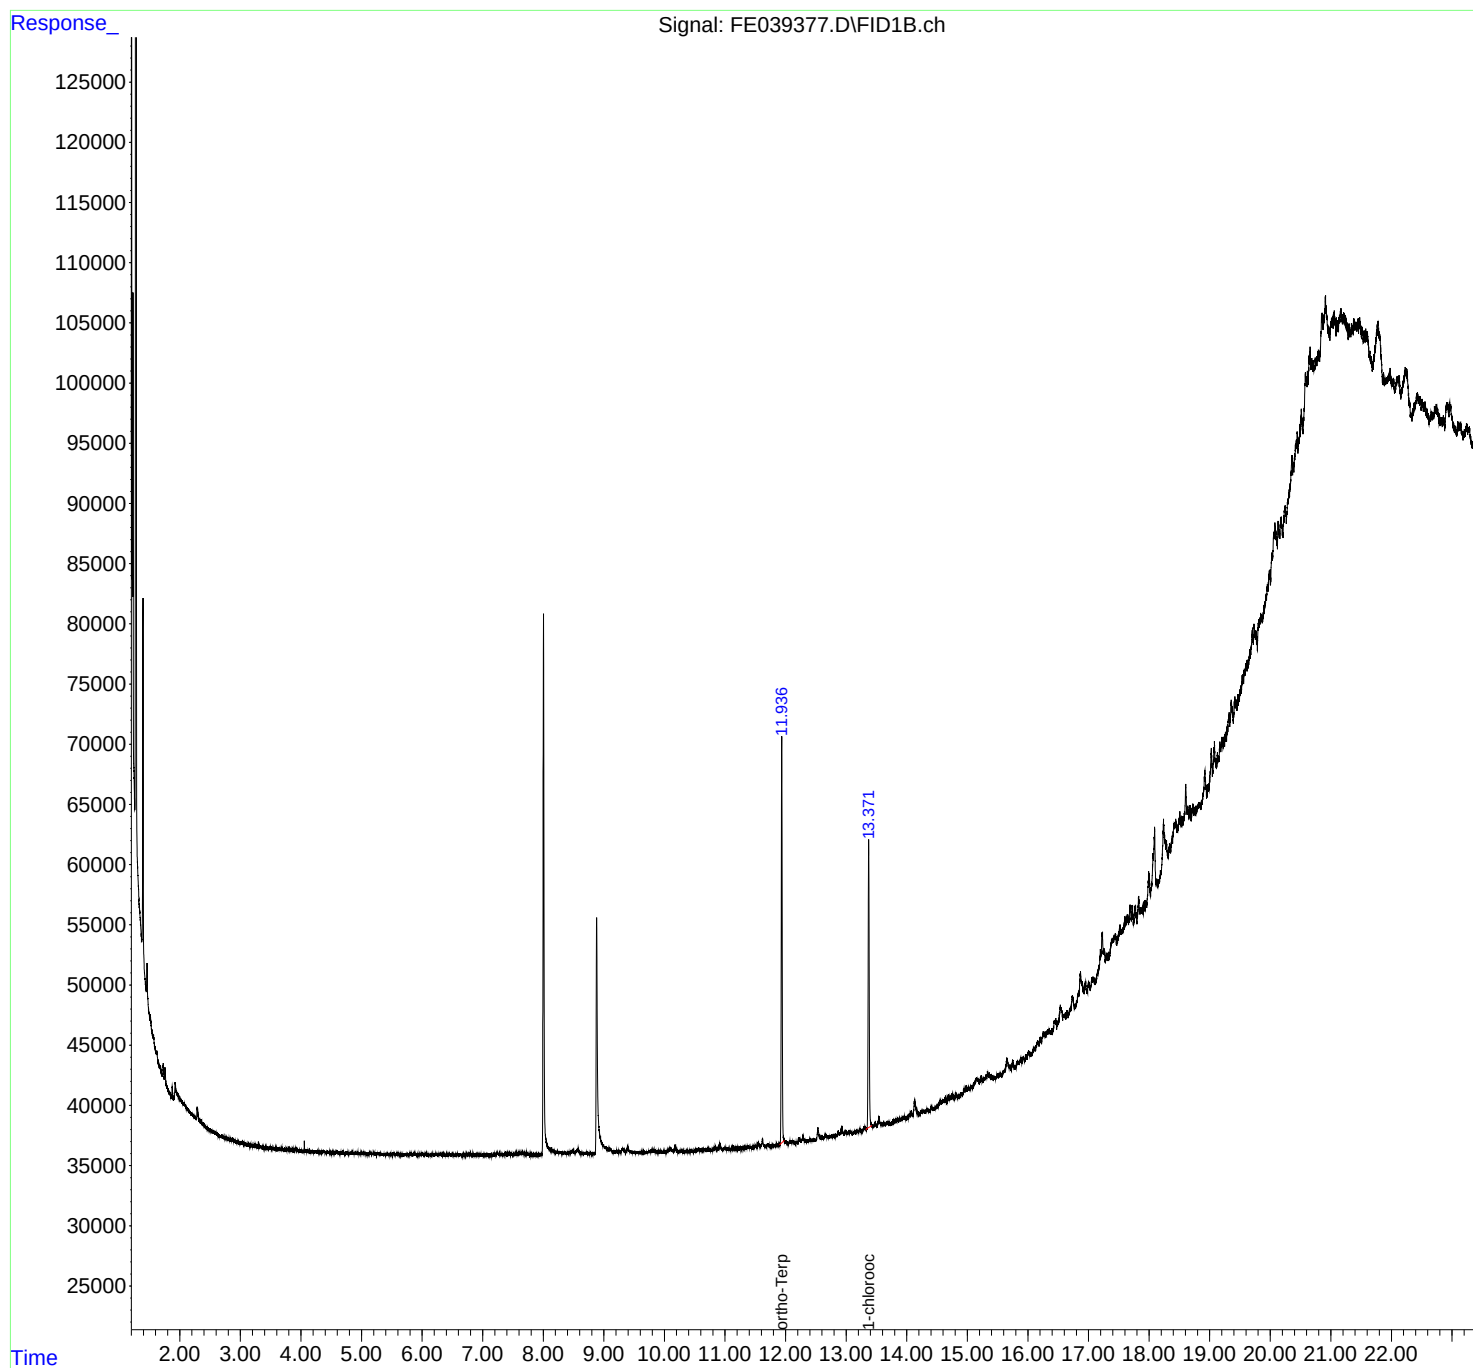


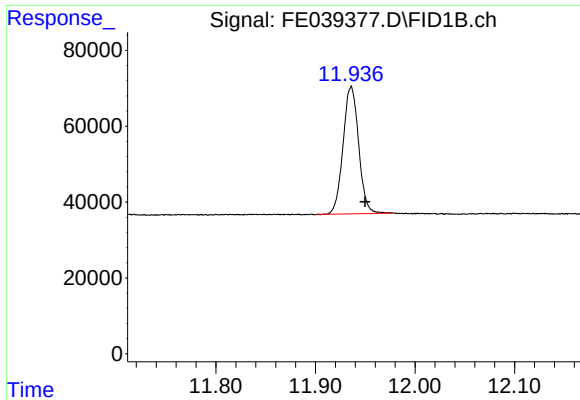

#9 ortho-Terphenyl (SURR)

R.T.: 11.936 min  
Delta R.T.: -0.014 min  
Response: 365167  
Conc: 2.45 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
FVSUB-TP7-COMP-07DL

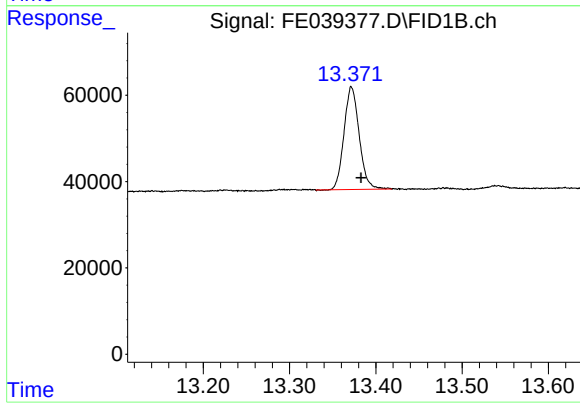

#12 1-chlorooctadecane (SURR)

R.T.: 13.372 min  
Delta R.T.: -0.011 min  
Response: 291117  
Conc: 2.53 ug/ml