

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122019\
 Data File : FE031011.D
 Signal(s) : FID1B.CH
 Acq On : 20 Dec 2019 10:41
 Operator : DD\AJ
 Sample : K6297-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 20 21:02:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE112619.M
 Quant Title :
 QLast Update : Tue Nov 26 14:51:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.635	5902850	19.677 ug/ml
Target Compounds			
4) N-TETRADECANE	8.234	318376	0.870 ug/ml
8) N-DOCOSANE	13.731	247804	0.706 ug/ml
10) N-TETRACOSANE	14.836	679114	1.942 ug/ml
11) N-HEXACOSANE	15.858	1174635	3.429 ug/ml
12) N-OCTACOSANE	16.809	1317545	3.879 ug/ml
13) N-TRIACONTANE	17.696	1092210	3.257 ug/ml
14) N-DOTRIACONTANE	18.529	553778	1.712 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122019\
Data File : FE031011.D
Signal(s) : FID1B.CH
Acq On : 20 Dec 2019 10:41
Operator : DD\AJ
Sample : K6297-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 20 21:02:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE112619.M
Quant Title :
QLast Update : Tue Nov 26 14:51:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

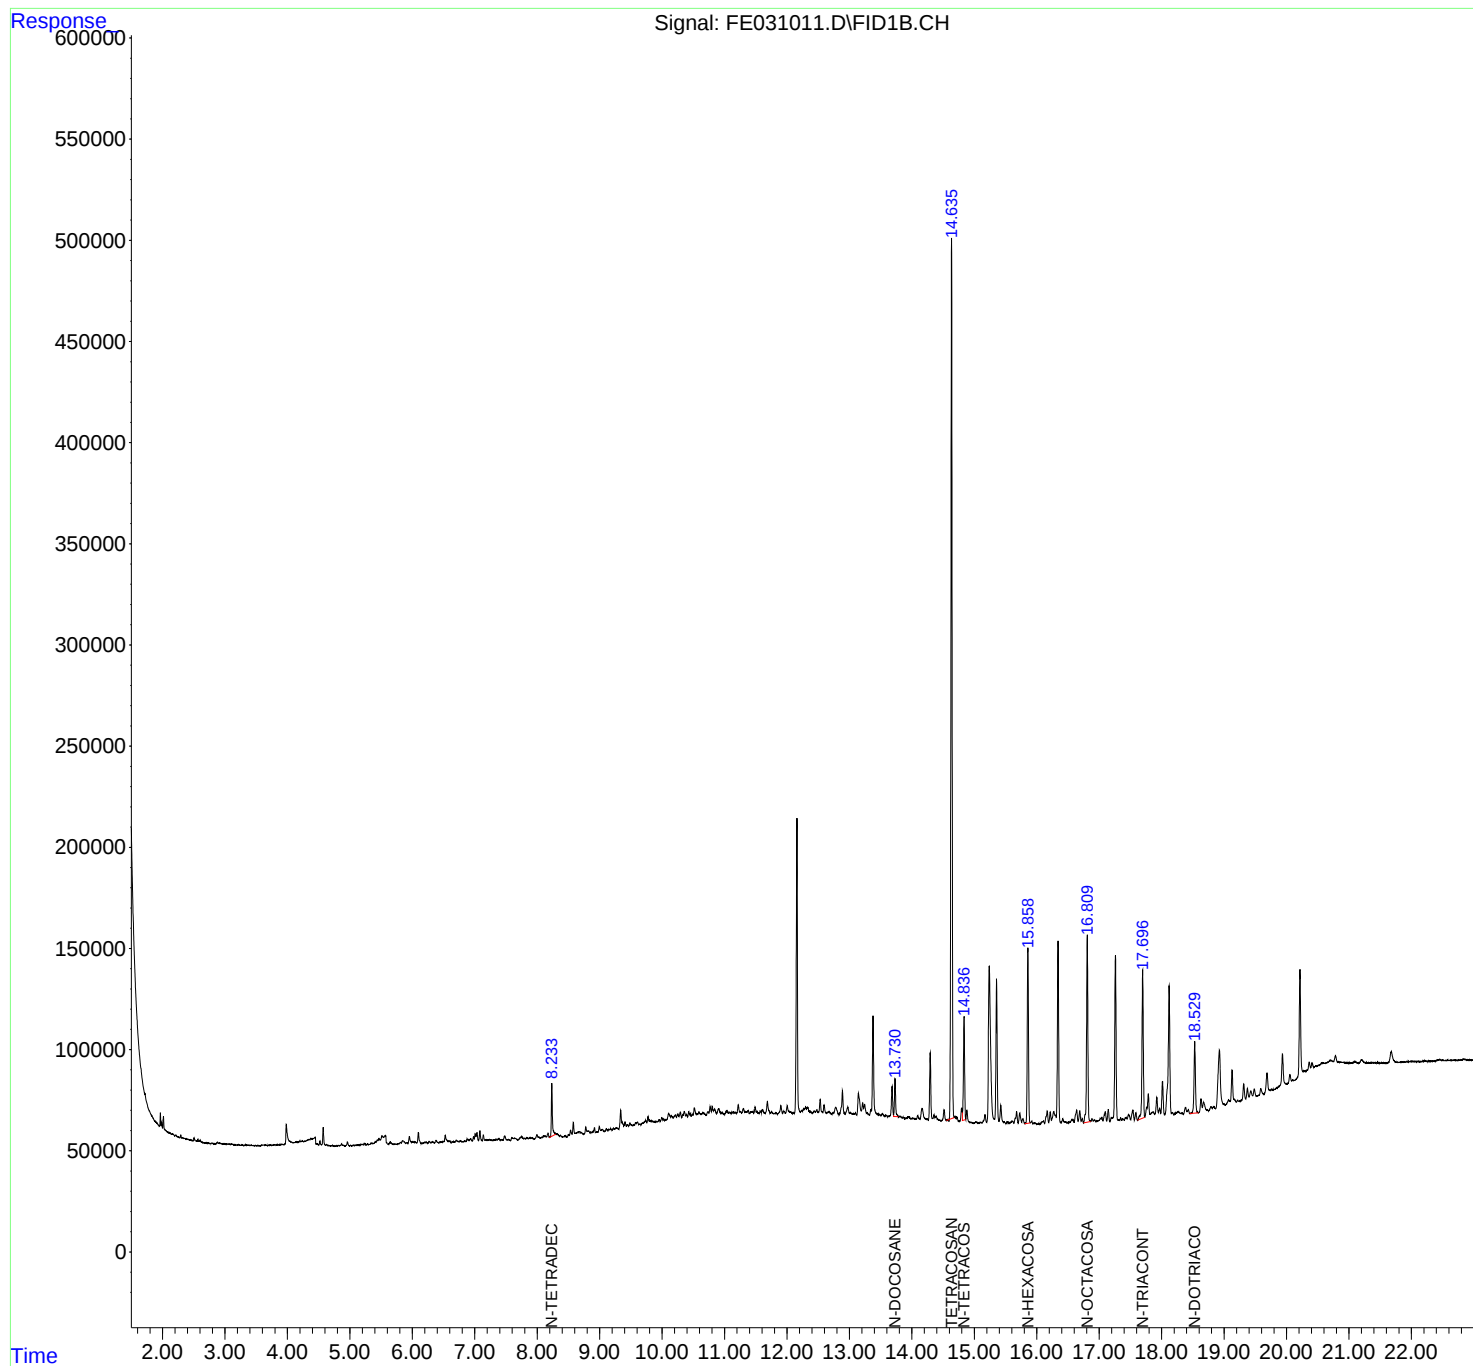


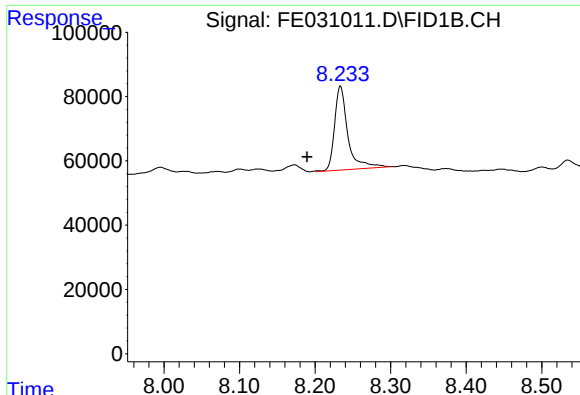

#4 N-TETRADECANE


R.T.: 8.234 min
Delta R.T.: 0.044 min
Response: 318376
Conc: 0.87 ug/ml

Instrument :
FID_E
ClientSampleId :

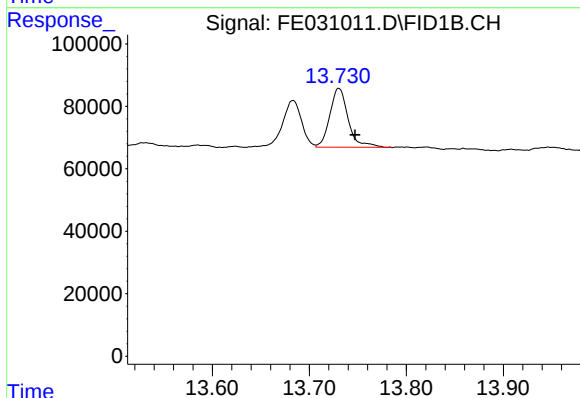


#8 N-DOCOSANE

R.T.: 13.731 min
Delta R.T.: -0.017 min
Response: 247804
Conc: 0.71 ug/ml

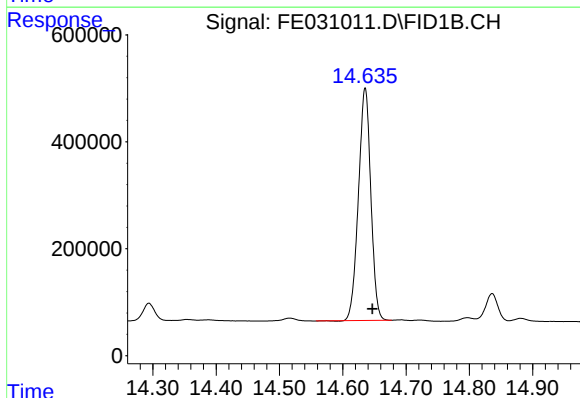


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.635 min
Delta R.T.: -0.012 min
Response: 5902850
Conc: 19.68 ug/ml

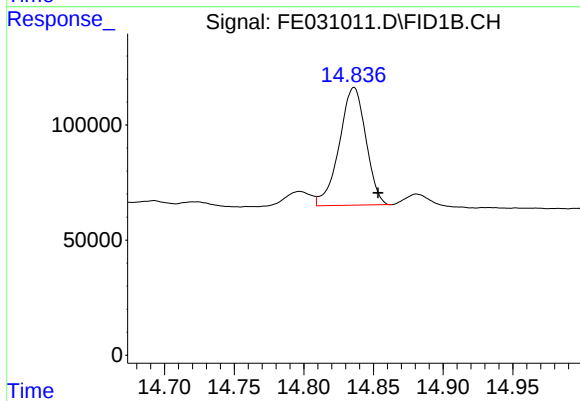

#10 N-TETRACOSANE


R.T.: 14.836 min
Delta R.T.: -0.018 min
Response: 679114
Conc: 1.94 ug/ml

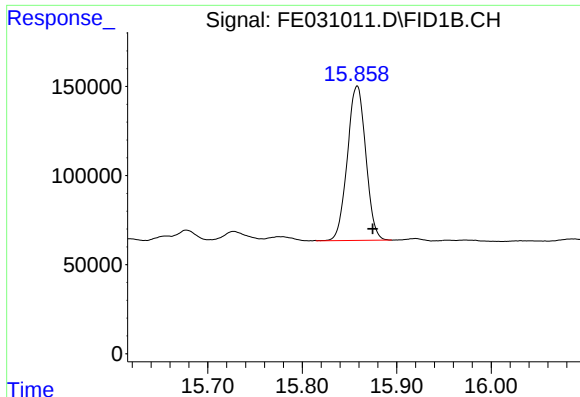

#11 N-HEXACOSANE


R.T.: 15.858 min
Delta R.T.: -0.017 min
Response: 1174635
Conc: 3.43 ug/ml

Instrument :
FID_E
ClientSampleId :

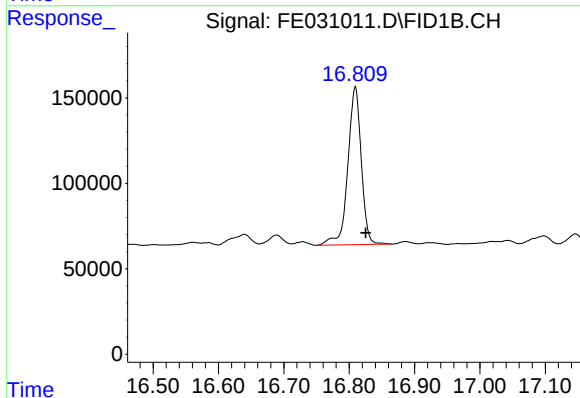


#12 N-OCTACOSANE

R.T.: 16.809 min
Delta R.T.: -0.016 min
Response: 1317545
Conc: 3.88 ug/ml

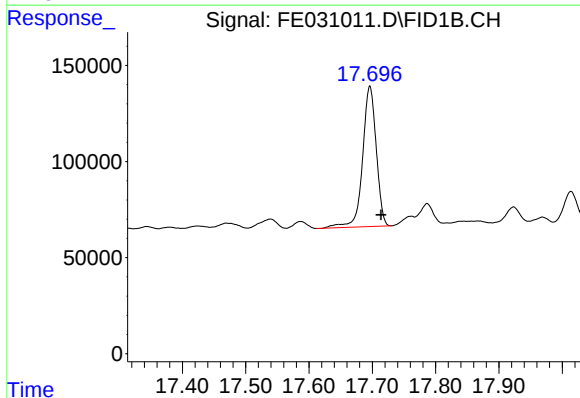

#13 N-TRIACONTANE

R.T.: 17.696 min
Delta R.T.: -0.017 min
Response: 1092210
Conc: 3.26 ug/ml

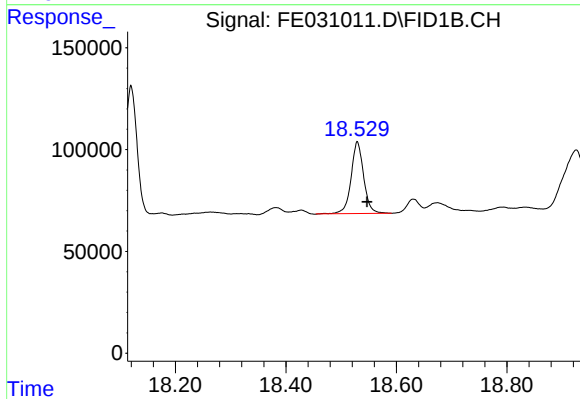

#14 N-DOTRIACONTANE

R.T.: 18.529 min
Delta R.T.: -0.018 min
Response: 553778
Conc: 1.71 ug/ml