

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122019\
 Data File : FE031020.D
 Signal(s) : FID1B.CH
 Acq On : 20 Dec 2019 15:37
 Operator : DD\AJ
 Sample : K6297-06 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 20 21:03:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE112619.M
 Quant Title :
 QLast Update : Tue Nov 26 14:51:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	1258553	4.195 ug/ml
Target Compounds			
3) N-DODECANE	6.375	285376	0.777 ug/ml
6) N-OCTADECANE	11.192	214731	0.599 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122019\
Data File : FE031020.D
Signal(s) : FID1B.CH
Acq On : 20 Dec 2019 15:37
Operator : DD\AJ
Sample : K6297-06 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 20 21:03:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE112619.M
Quant Title :
QLast Update : Tue Nov 26 14:51:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

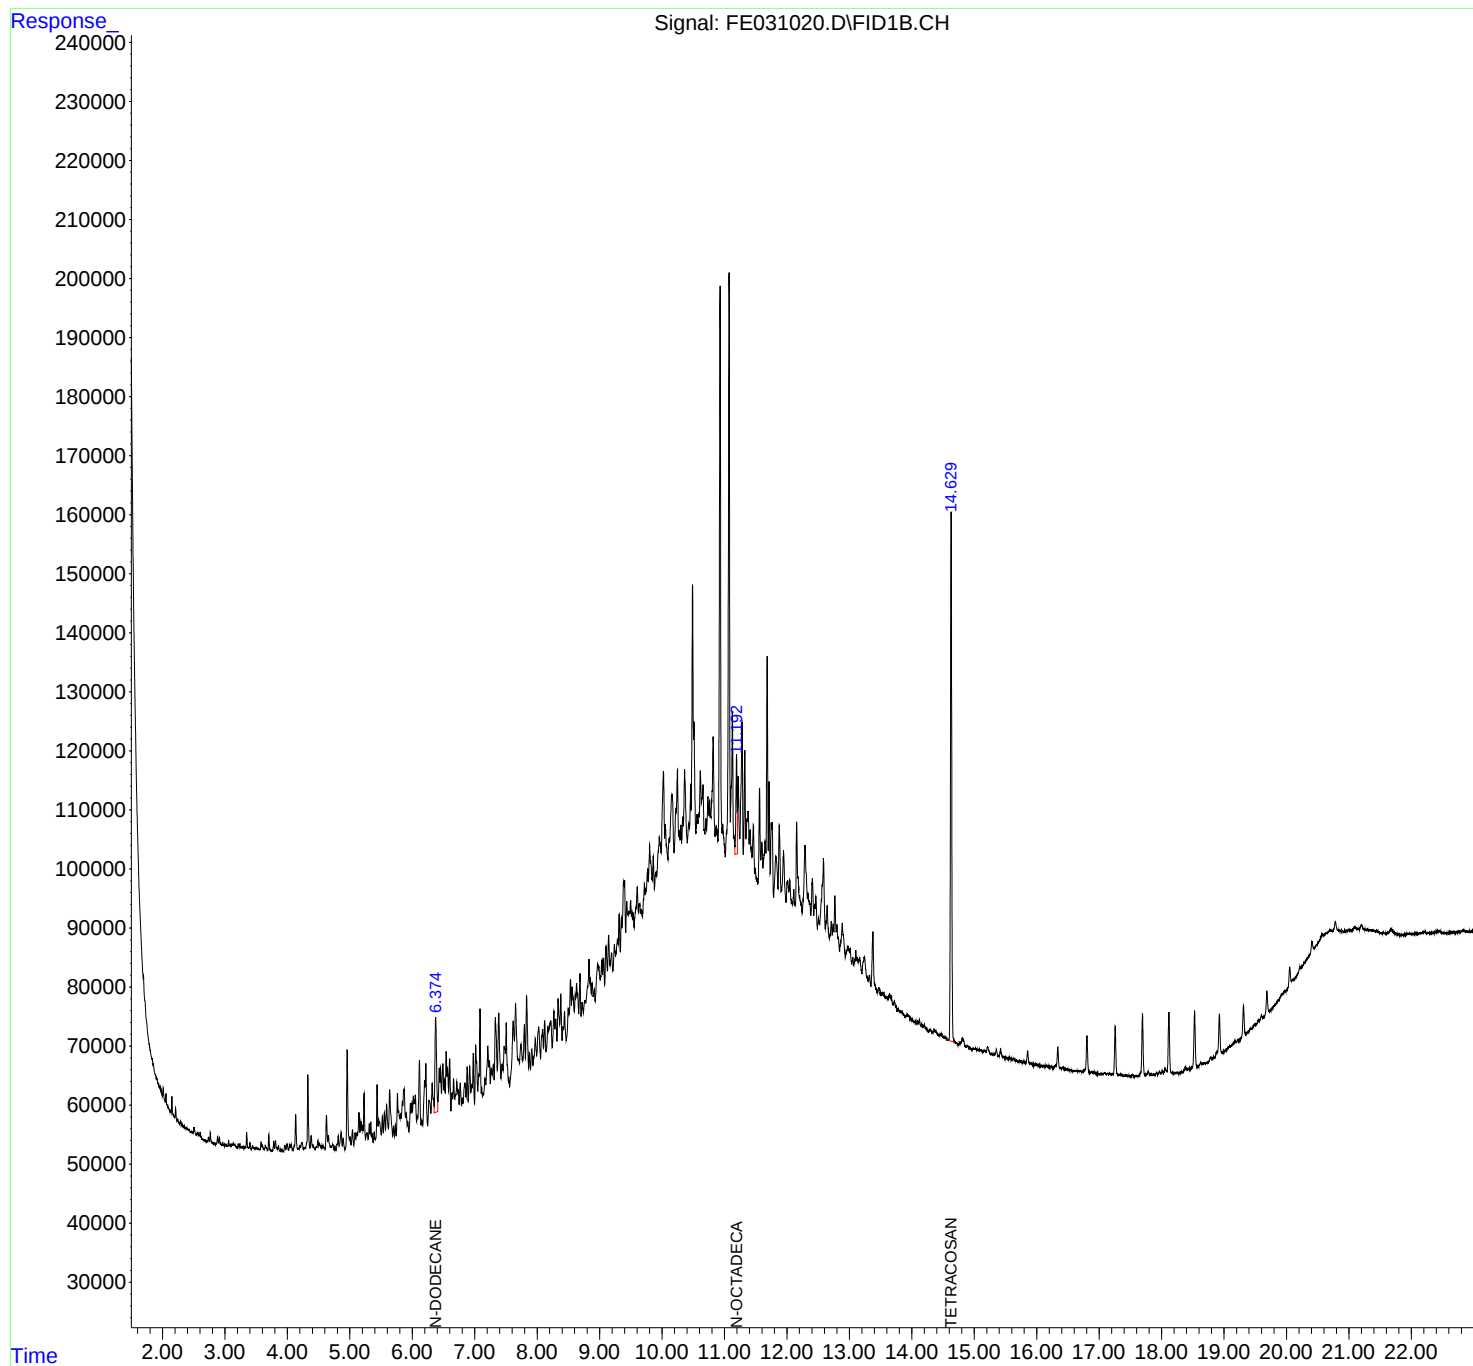


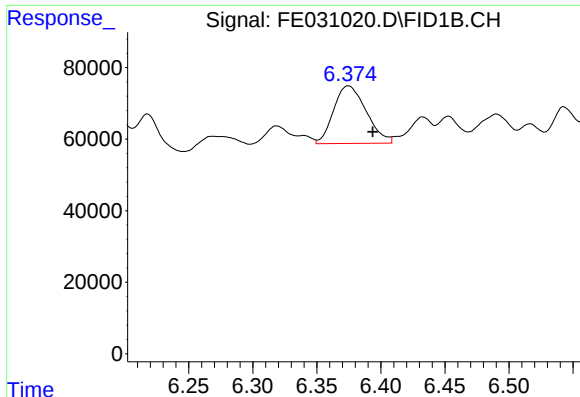

#3 N-DODECANE


R.T.: 6.375 min
Delta R.T.: -0.019 min
Response: 285376
Conc: 0.78 ug/ml

Instrument :
FID_E
ClientSampleId :

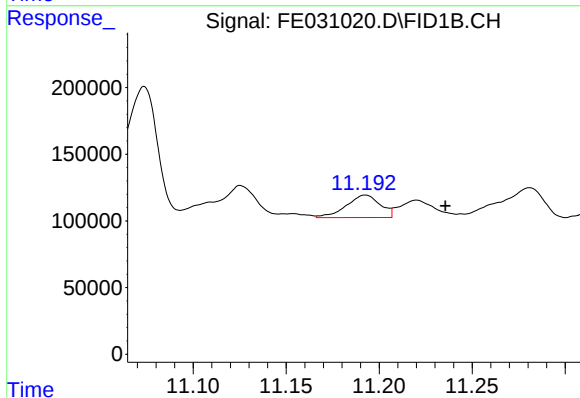

#6 N-OCTADECANE

R.T.: 11.192 min
Delta R.T.: -0.043 min
Response: 214731
Conc: 0.60 ug/ml

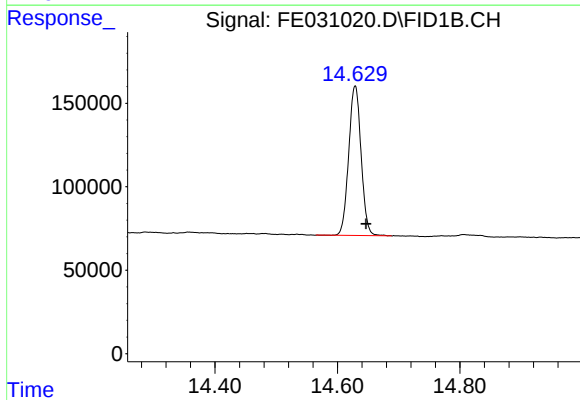

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.629 min
Delta R.T.: -0.018 min
Response: 1258553
Conc: 4.20 ug/ml