

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE122024AL\  
 Data File : FE051729.D  
 Signal(s) : FID1B.ch  
 Acq On : 20 Dec 2024 08:00  
 Operator : YP\AJ  
 Sample : P5342-01DL 2X  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 CHRT26634DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 12/23/2024  
 Supervised By :Ankita Jodhani 12/27/2024

Integration File: autoint1.e  
 Quant Time: Dec 20 22:43:03 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 121724.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Dec 17 15:04:25 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 9) S ortho-Terphenyl (SURR)    | 12.046 | 5222301    | 32.529 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 65.06%        |
| 12) S 1-chlorooctadecane (S... | 13.401 | 2468869    | 19.571 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 39.14%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE122024AL\  
Data File : FE051729.D  
Signal(s) : FID1B.ch  
Acq On : 20 Dec 2024 08:00  
Operator : YP\AJ  
Sample : P5342-01DL 2X  
Misc :  
ALS Vial : 11 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
CHRT26634DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 12/23/2024  
Supervised By :Ankita Jodhani 12/27/2024

Integration File: autoint1.e  
Quant Time: Dec 20 22:43:03 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 121724.M  
Quant Title : GC Extractables  
QLast Update : Tue Dec 17 15:04:25 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

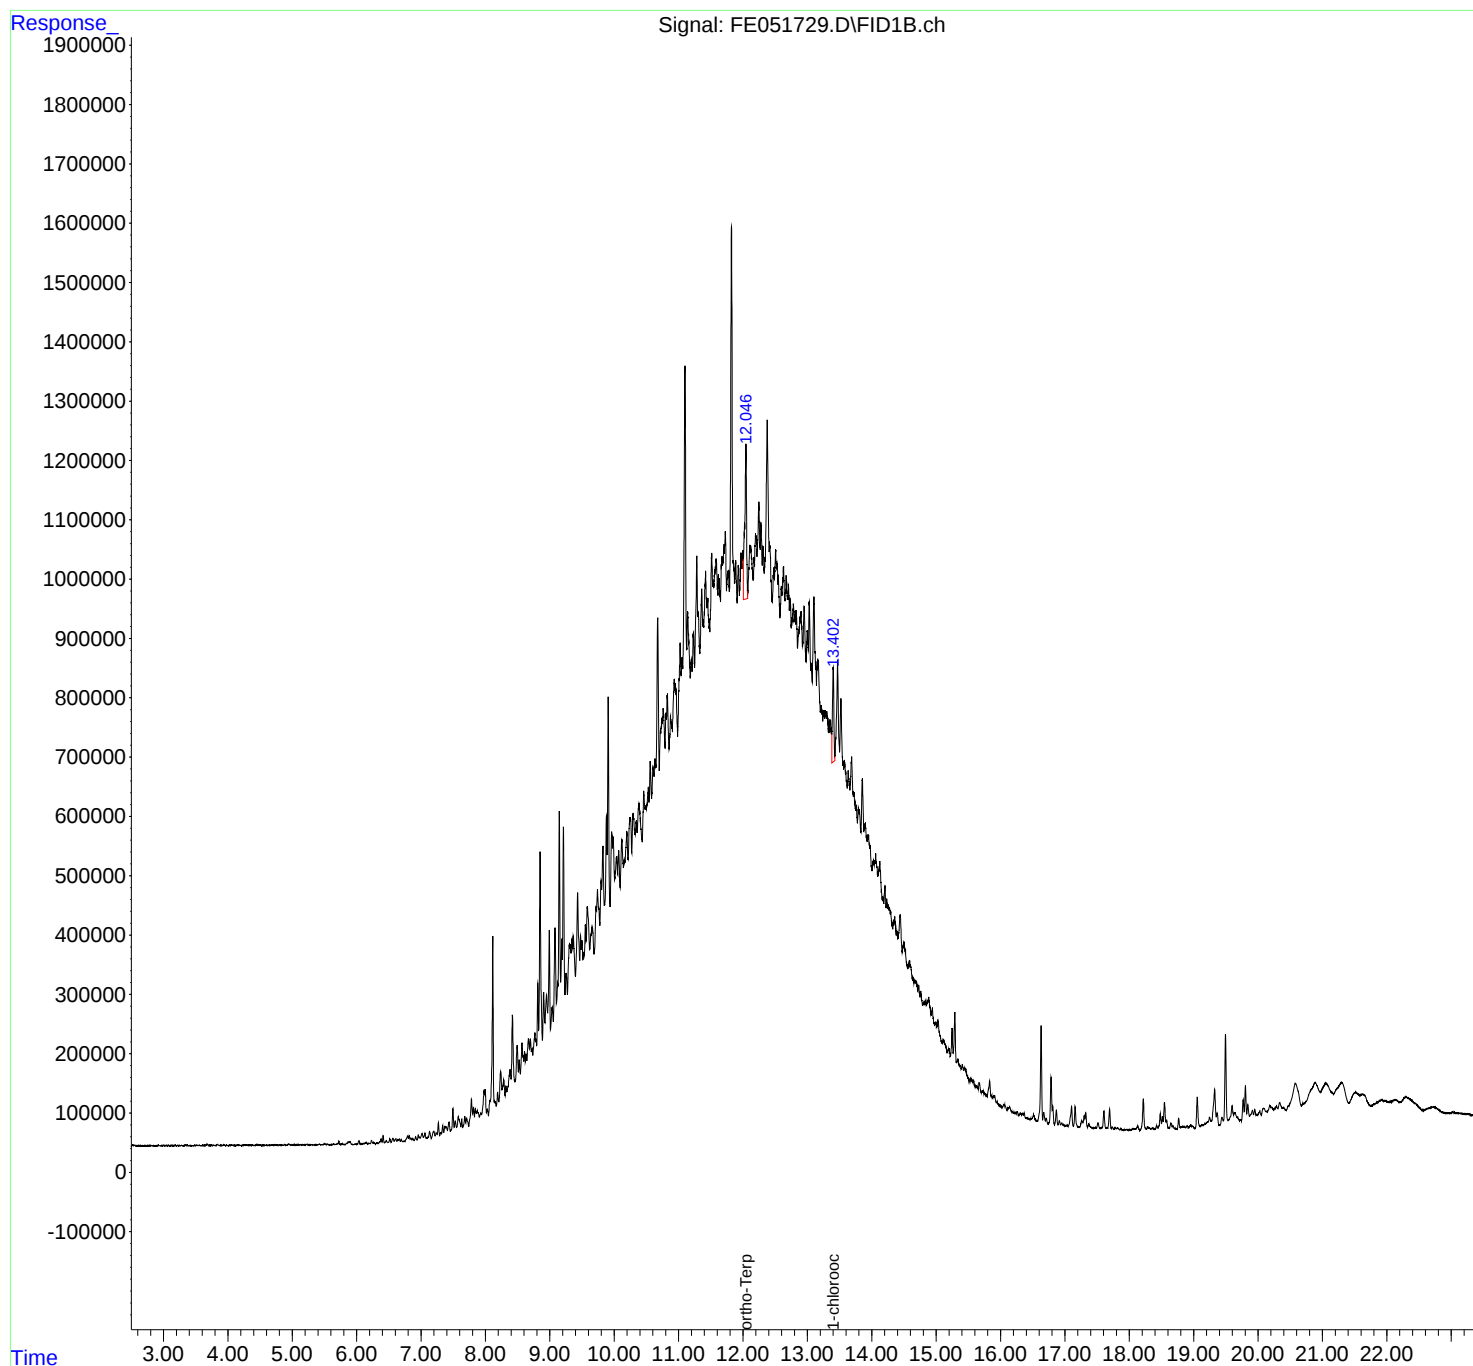

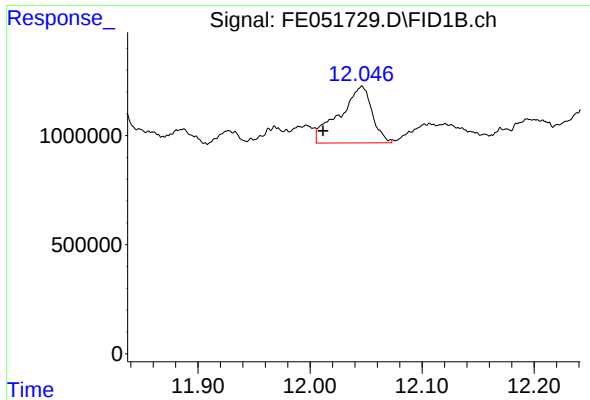


#9 ortho-Terphenyl (SURR)

R.T.: 12.046 min  
Delta R.T.: 0.034 min  
Response: 5222301  
Conc: 32.53 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
CHRT26634DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 12/23/2024  
Supervised By :Ankita Jodhani 12/27/2024

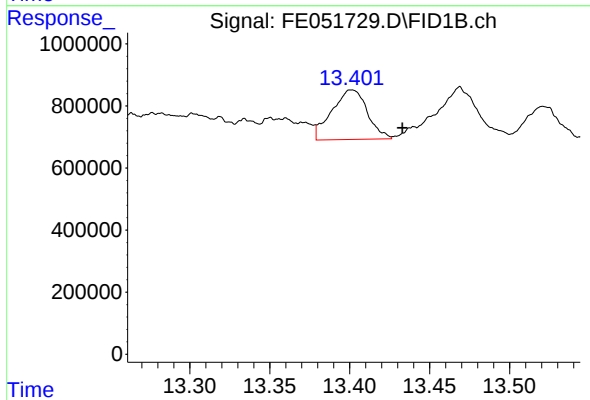

#12 1-chlorooctadecane (SURR)

R.T.: 13.401 min  
Delta R.T.: -0.032 min  
Response: 2468869  
Conc: 19.57 ug/ml m