

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122623AL\
Data File : FE045972.D
Signal(s) : FID1B.ch
Acq On : 26 Dec 2023 19:22
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 26 22:30:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 113023.M
Quant Title : GC Extractables
QLast Update : Thu Nov 30 12:25:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.021	41443	0.237 ug/ml
18) T	n-Dotriacontane (C32)	18.855	302686	1.659 ug/ml
20) T	n-Hexatriacontane (C36)	20.384	12073	0.076 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122623AL\
Data File : FE045972.D
Signal(s) : FID1B.ch
Acq On : 26 Dec 2023 19:22
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 26 22:30:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 113023.M
Quant Title : GC Extractables
QLast Update : Thu Nov 30 12:25:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

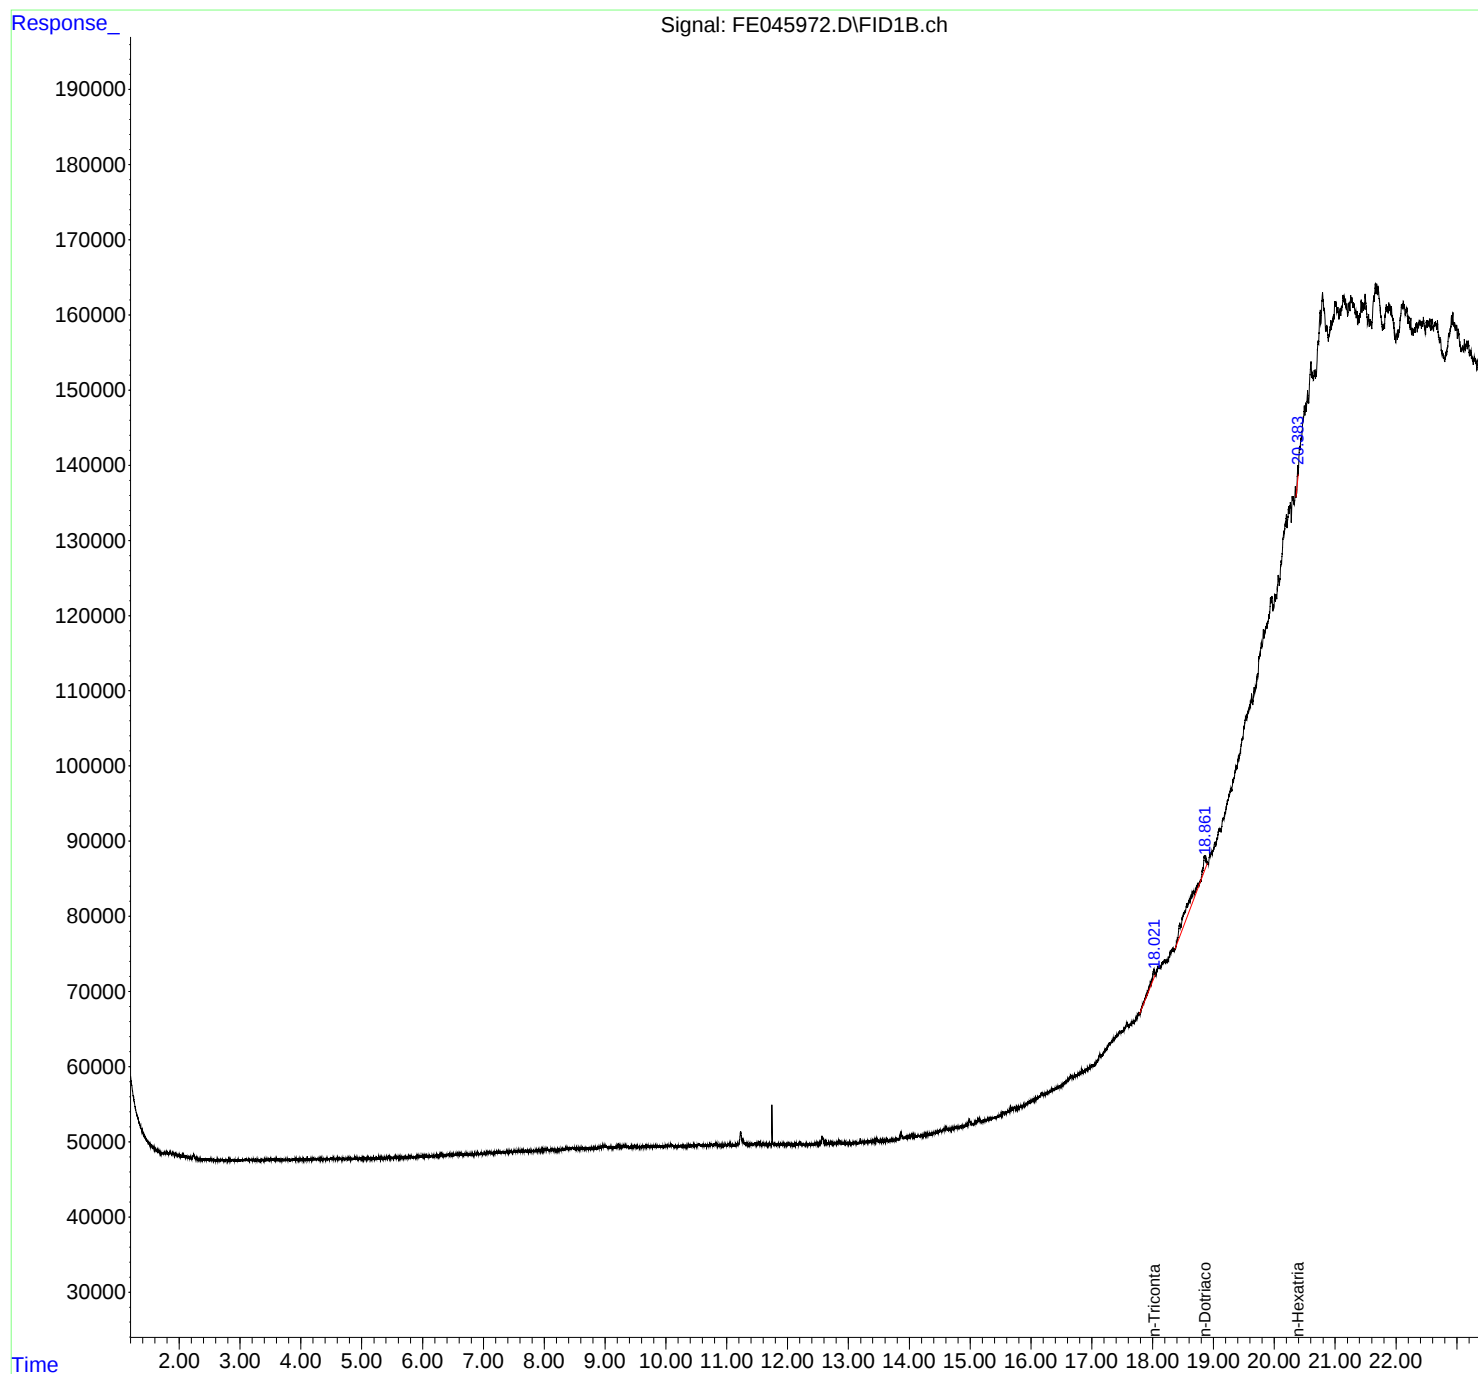


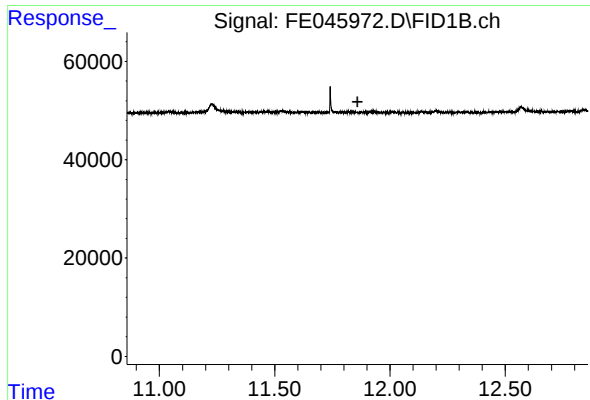

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.859 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

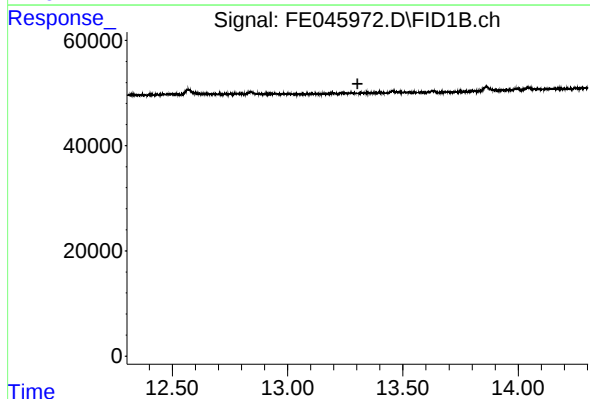


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.303 min
Response: 0
Conc: N.D.

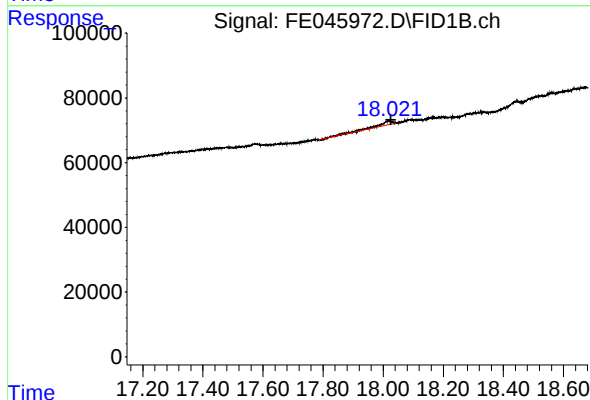


#17 n-Tricontane (C30)

R.T.: 18.021 min
Delta R.T.: -0.005 min
Response: 41443
Conc: 0.24 ug/ml

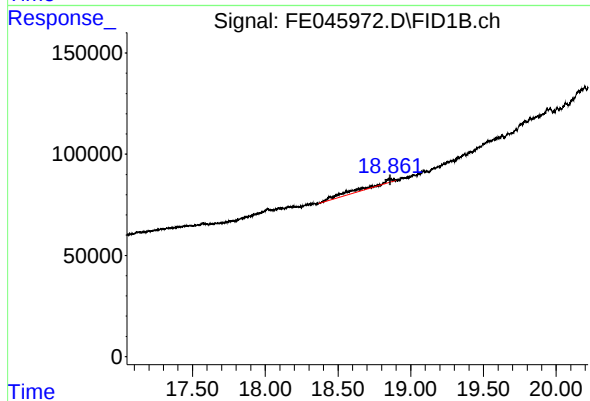

#18 n-Dotriacontane (C32)

R.T.: 18.855 min
Delta R.T.: -0.005 min
Response: 302686
Conc: 1.66 ug/ml

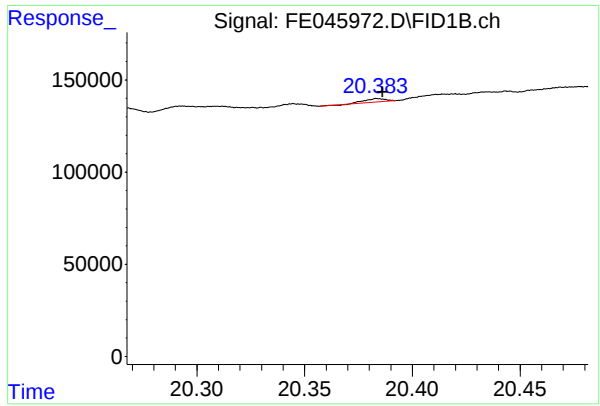

#20 n-Hexatriacontane (C36)

R.T.: 20.384 min
Delta R.T.: -0.002 min
Response: 12073
Conc: 0.08 ug/ml

Instrument :

FID_E

ClientSampleId :