

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122722AL\
 Data File : FE039491.D
 Signal(s) : FID1B.ch
 Acq On : 27 Dec 2022 17:49
 Operator : YP\AJ
 Sample : N6190-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 28 02:18:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 17 15:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.930	5882459	39.418 ug/ml
Spiked Amount 50.000		Recovery =	78.84%
12) S 1-chlorooctadecane (S...	13.363	4440179	38.577 ug/ml
Spiked Amount 50.000		Recovery =	77.15%
Target Compounds			
14) T n-Tetracosane (C24)	15.215	64109	0.478 ug/ml
16) T n-Octacosane (C28)	17.189	78178	0.607 ug/ml
17) T n-Tricontane (C30)	18.073	67830	0.527 ug/ml
18) T n-Dotriacontane (C32)	18.907	87902	0.679 ug/ml
19) T n-Tetratriacontane (C34)	19.687	113551	0.900 ug/ml
20) T n-Hexatriacontane (C36)	20.431	45358	0.375 ug/ml
21) T n-Octatriacontane (C38)	21.167	55804	0.452 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122722AL\
Data File : FE039491.D
Signal(s) : FID1B.ch
Acq On : 27 Dec 2022 17:49
Operator : YP\AJ
Sample : N6190-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 28 02:18:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
Quant Title : GC Extractables
QLast Update : Sat Dec 17 15:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

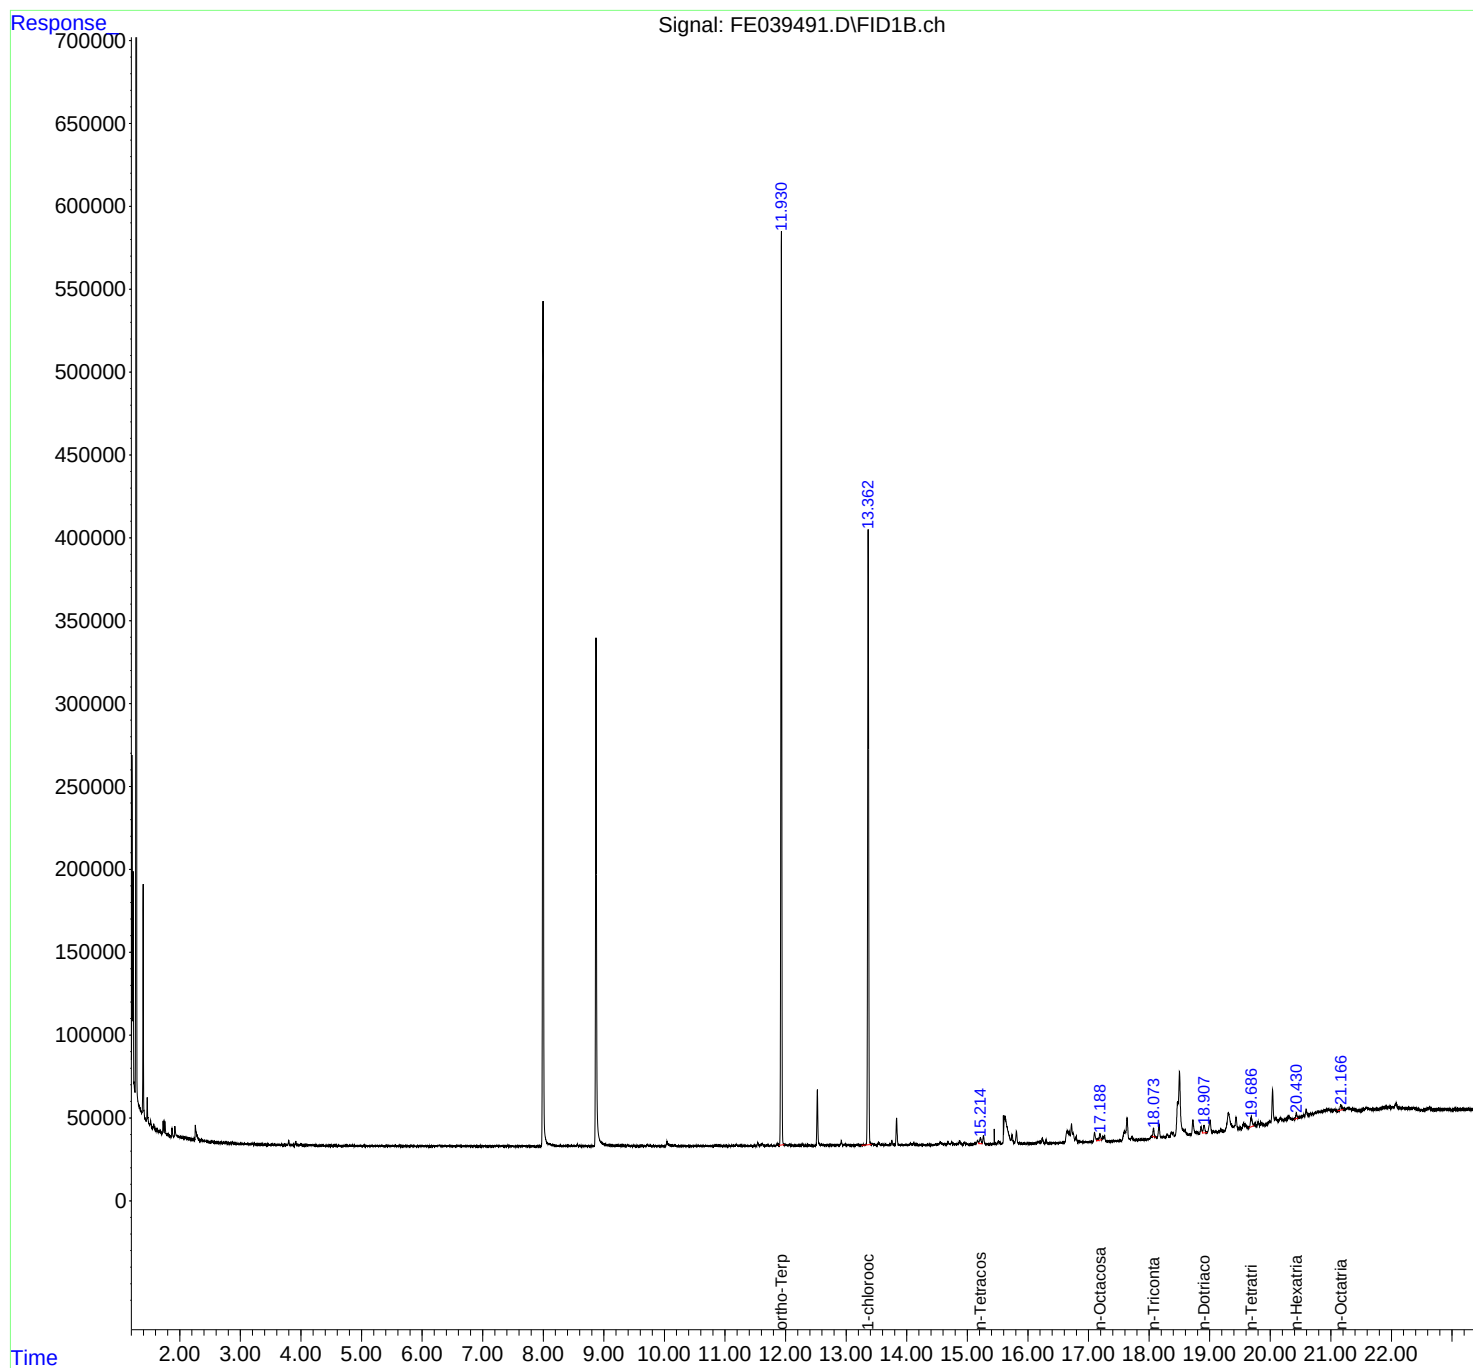


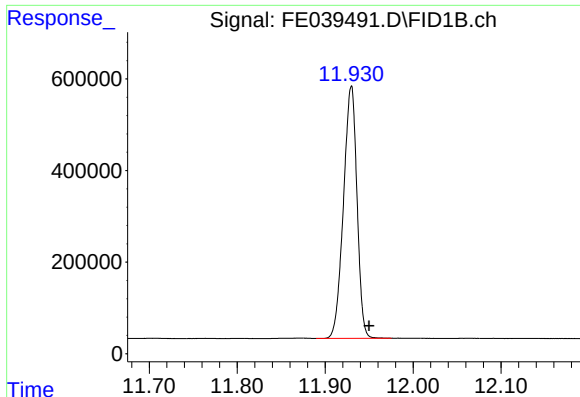

#9 ortho-Terphenyl (SURR)


R.T.: 11.930 min
Delta R.T.: -0.020 min
Response: 5882459
Conc: 39.42 ug/ml

Instrument :
FID_E
ClientSampleId :

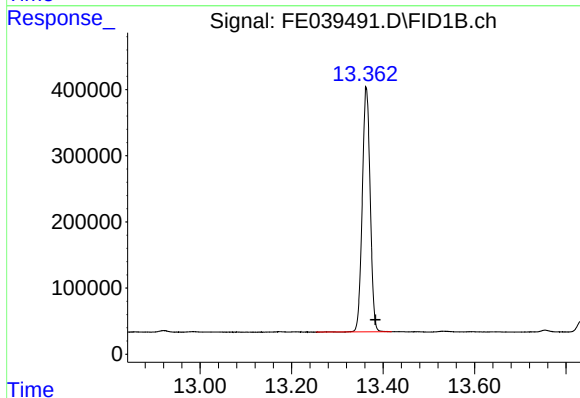


#12 1-chlorooctadecane (SURR)

R.T.: 13.363 min
Delta R.T.: -0.020 min
Response: 4440179
Conc: 38.58 ug/ml

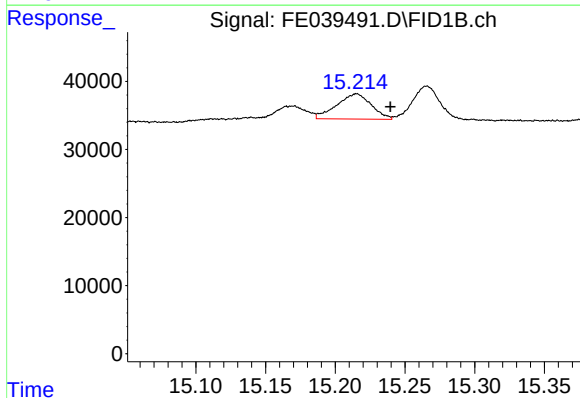


#14 n-Tetracosane (C24)

R.T.: 15.215 min
Delta R.T.: -0.024 min
Response: 64109
Conc: 0.48 ug/ml

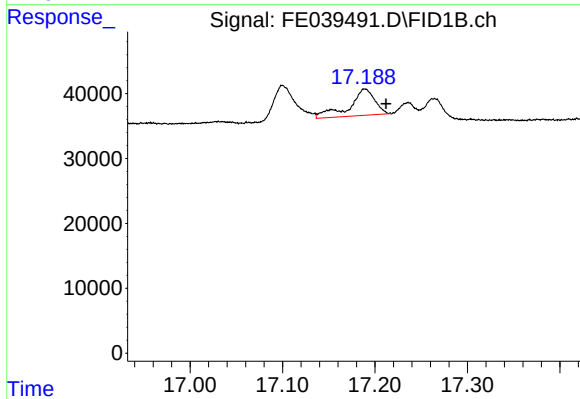

#16 n-Octacosane (C28)


R.T.: 17.189 min
Delta R.T.: -0.023 min
Response: 78178
Conc: 0.61 ug/ml

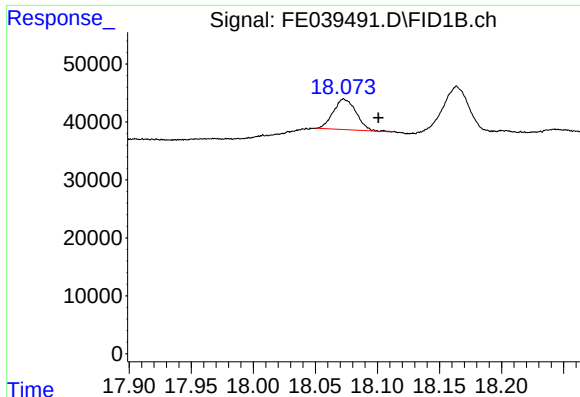

#17 n-Tricontane (C30)


R.T.: 18.073 min
Delta R.T.: -0.028 min
Response: 67830
Conc: 0.53 ug/ml

Instrument :
FID_E
ClientSampleId :

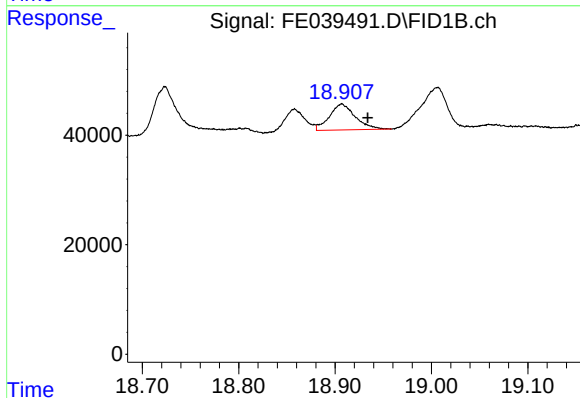


#18 n-Dotriacontane (C32)

R.T.: 18.907 min
Delta R.T.: -0.027 min
Response: 87902
Conc: 0.68 ug/ml

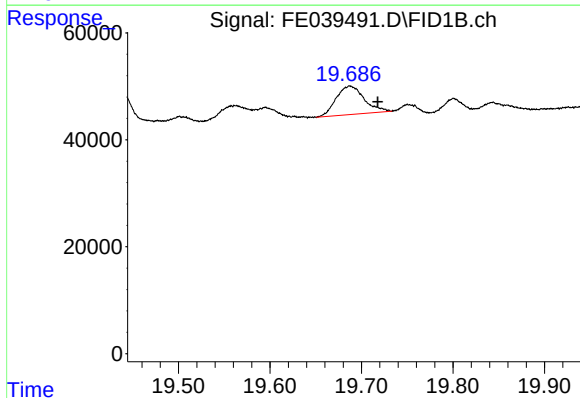


#19 n-Tetratriacontane (C34)

R.T.: 19.687 min
Delta R.T.: -0.030 min
Response: 113551
Conc: 0.90 ug/ml

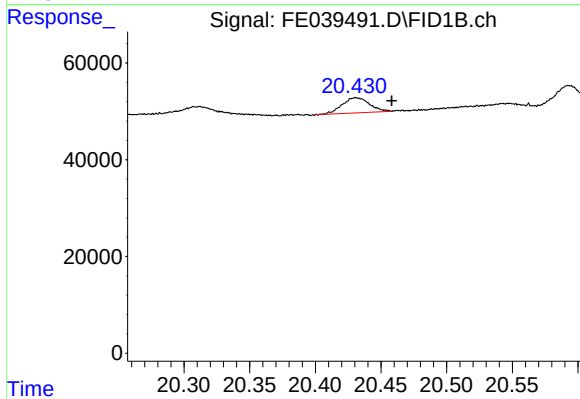

#20 n-Hexatriacontane (C36)

R.T.: 20.431 min
Delta R.T.: -0.027 min
Response: 45358
Conc: 0.38 ug/ml

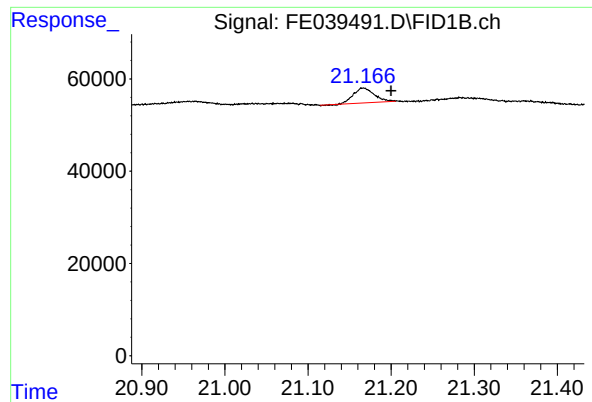

#21 n-Octatriacontane (C38)

R.T.: 21.167 min
Delta R.T.: -0.033 min
Response: 55804
Conc: 0.45 ug/ml

Instrument :

FID_E

ClientSampleId :