

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122822AL\
 Data File : FE039512.D
 Signal(s) : FID1B.ch
 Acq On : 28 Dec 2022 10:14
 Operator : YP\AJ
 Sample : N6205-02DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 28 11:14:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 17 15:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.925	842858	5.648 ug/ml
Spiked Amount 50.000		Recovery =	11.30%
12) S 1-chlorooctadecane (S...	13.361	637550	5.539 ug/ml
Spiked Amount 50.000		Recovery =	11.08%
Target Compounds			
10) T n-Eicosane (C20)	12.981	50762	0.372 ug/ml
15) T n-Hexacosane (C26)	16.236	32484	0.249 ug/ml
16) T n-Octacosane (C28)	17.186	75703	0.588 ug/ml
17) T n-Tricontane (C30)	18.075	56493	0.439 ug/ml
18) T n-Dotriacontane (C32)	18.911	102166	0.789 ug/ml
19) T n-Tetratriacontane (C34)	19.690	19175	0.152 ug/ml
20) T n-Hexatriacontane (C36)	20.502	44395	0.367 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122822AL\
Data File : FE039512.D
Signal(s) : FID1B.ch
Acq On : 28 Dec 2022 10:14
Operator : YP\AJ
Sample : N6205-02DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 28 11:14:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
Quant Title : GC Extractables
QLast Update : Sat Dec 17 15:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

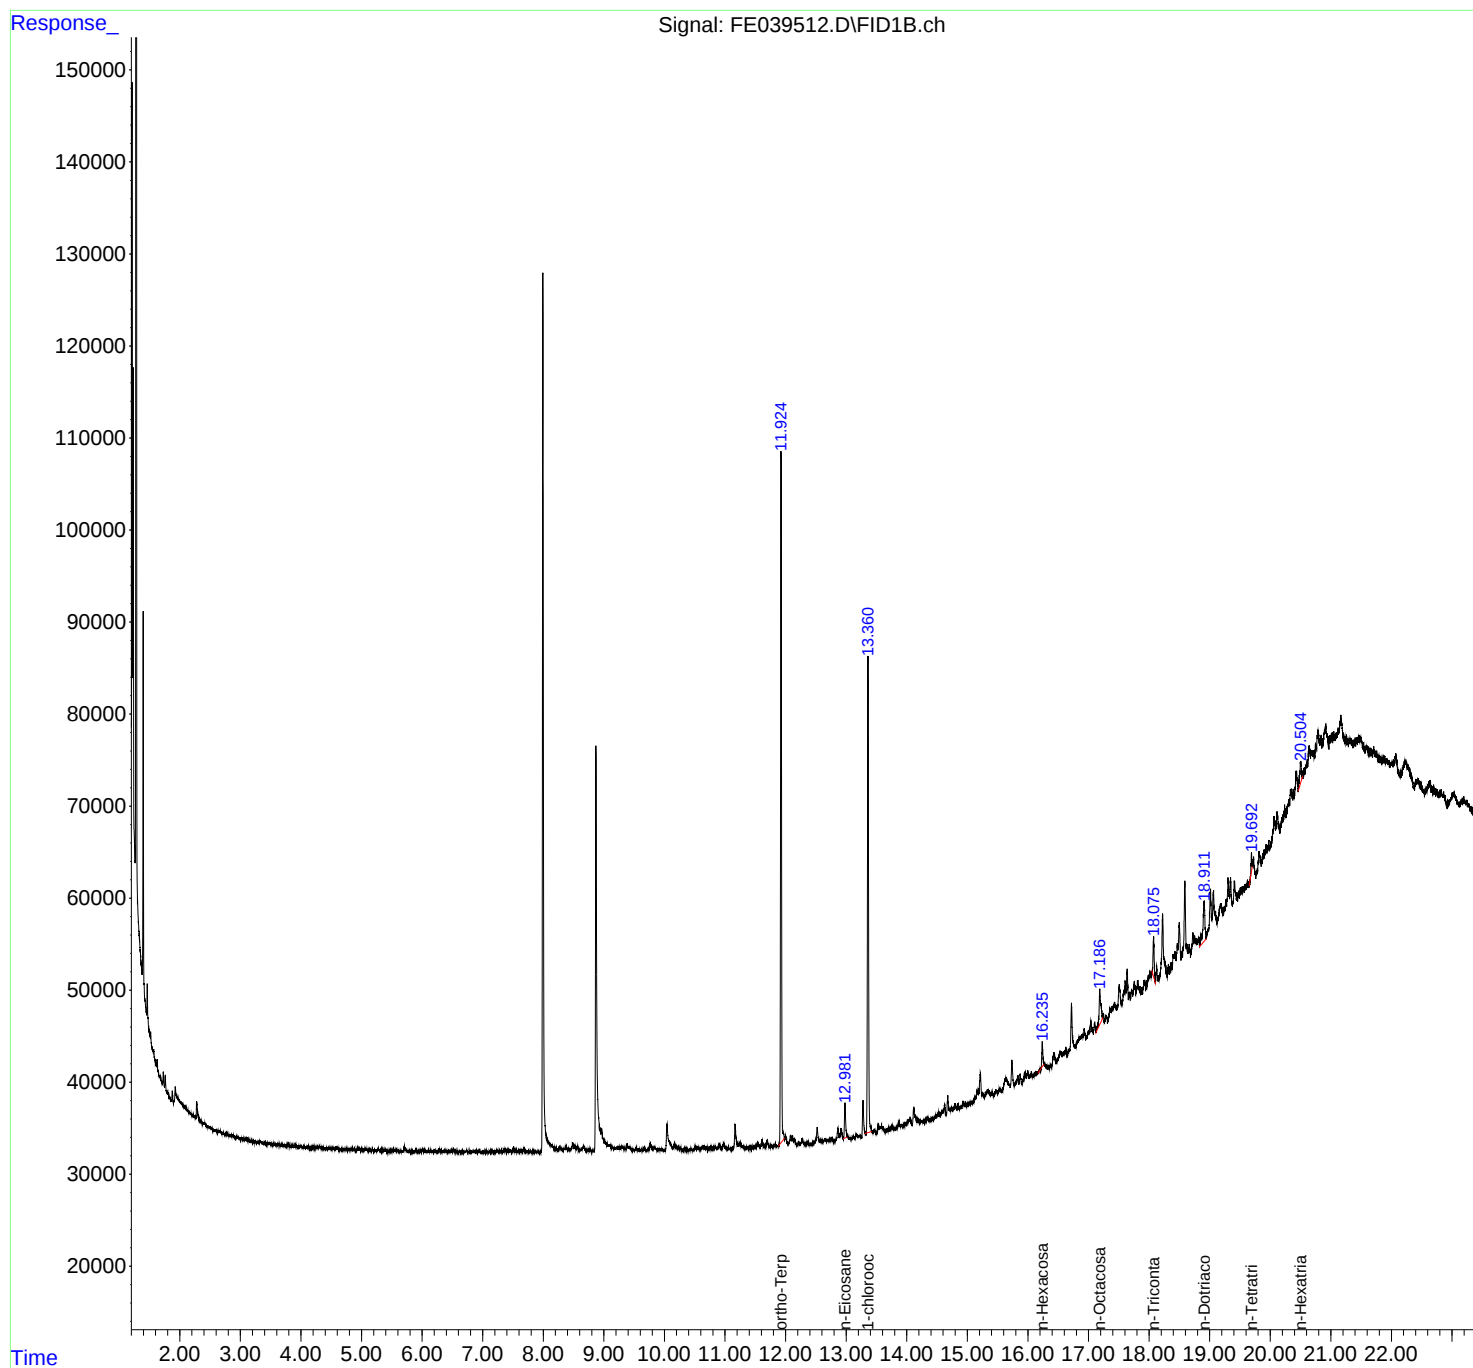


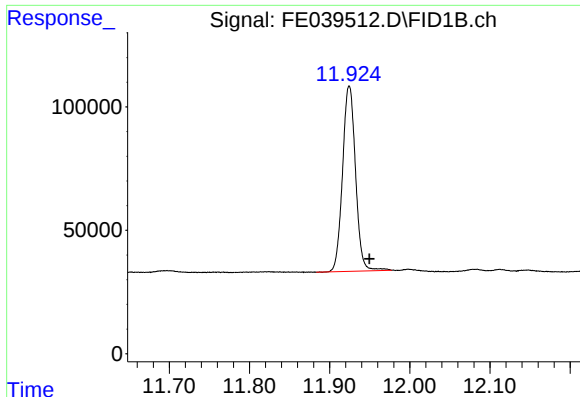

#9 ortho-Terphenyl (SURR)


R.T.: 11.925 min
Delta R.T.: -0.025 min
Response: 842858
Conc: 5.65 ug/ml

Instrument :
FID_E
ClientSampleId :

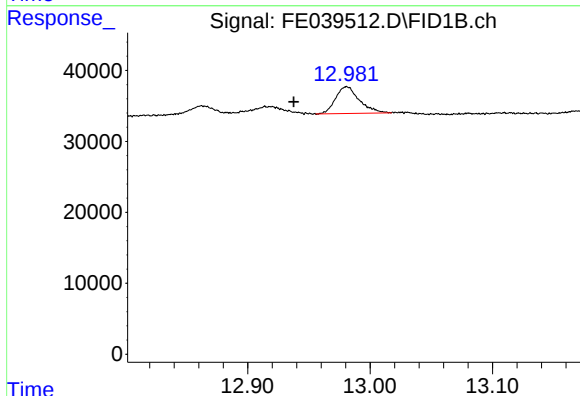


#10 n-Eicosane (C20)

R.T.: 12.981 min
Delta R.T.: 0.043 min
Response: 50762
Conc: 0.37 ug/ml

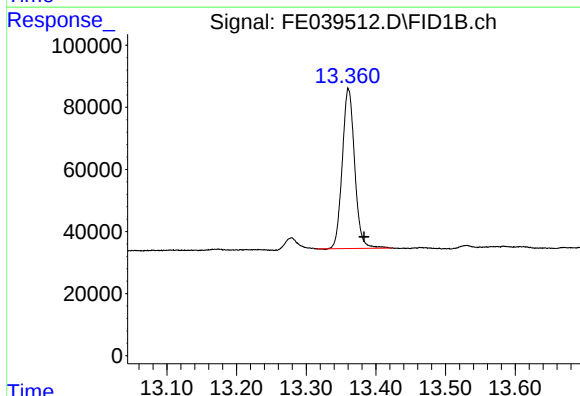


#12 1-chlorooctadecane (SURR)

R.T.: 13.361 min
Delta R.T.: -0.022 min
Response: 637550
Conc: 5.54 ug/ml

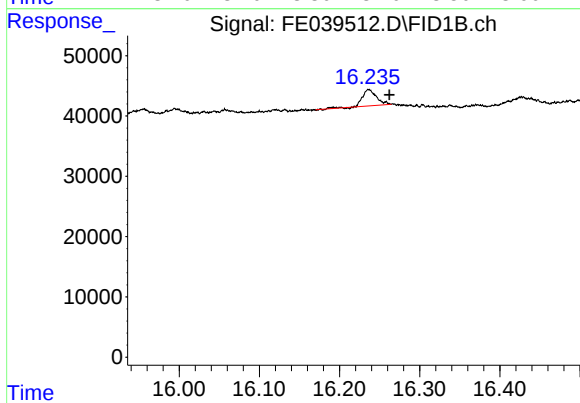

#15 n-Hexacosane (C26)


R.T.: 16.236 min
Delta R.T.: -0.026 min
Response: 32484
Conc: 0.25 ug/ml

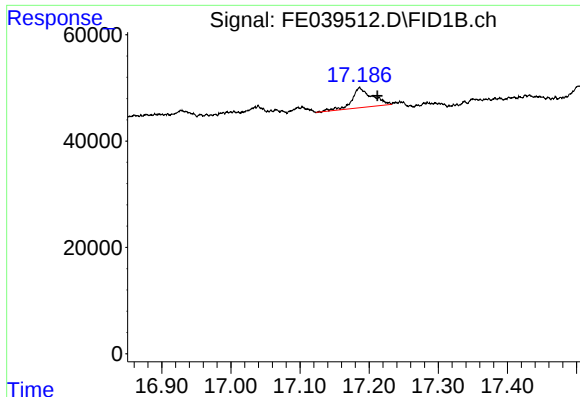

#16 n-Octacosane (C28)


R.T.: 17.186 min
Delta R.T.: -0.026 min
Response: 75703
Conc: 0.59 ug/ml

Instrument :
FID_E
ClientSampleId :

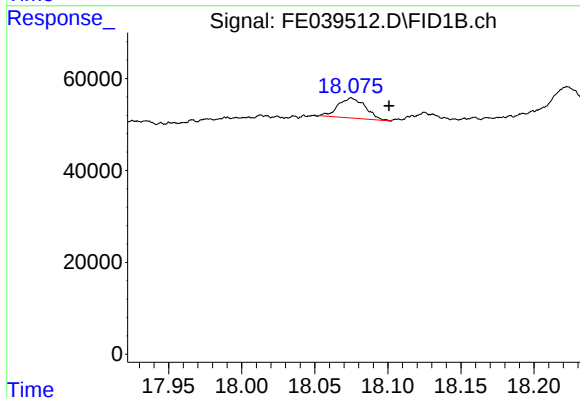


#17 n-Tricontane (C30)

R.T.: 18.075 min
Delta R.T.: -0.026 min
Response: 56493
Conc: 0.44 ug/ml

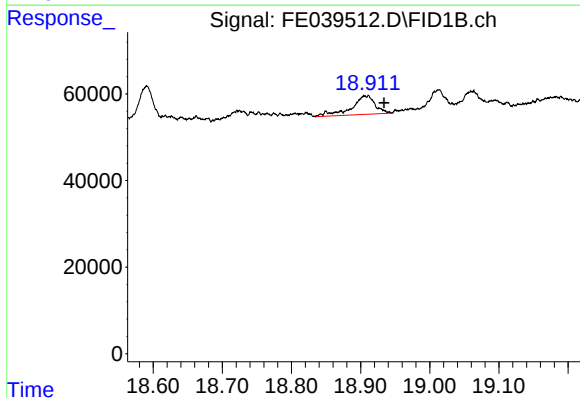


#18 n-Dotriacontane (C32)

R.T.: 18.911 min
Delta R.T.: -0.023 min
Response: 102166
Conc: 0.79 ug/ml

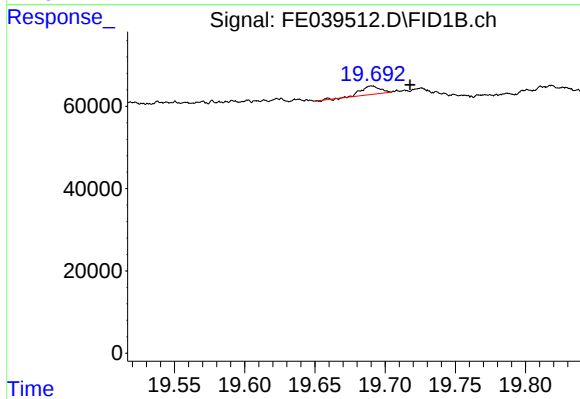

#19 n-Tetratriacontane (C34)

R.T.: 19.690 min
Delta R.T.: -0.027 min
Response: 19175
Conc: 0.15 ug/ml

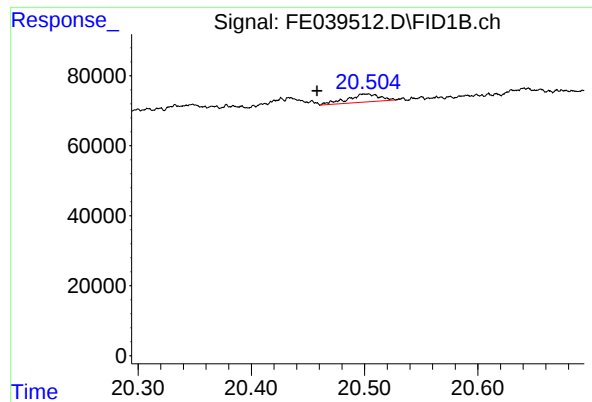

#20 n-Hexatriacontane (C36)

R.T.: 20.502 min
Delta R.T.: 0.044 min
Response: 44395
Conc: 0.37 ug/ml

Instrument :
FID_E
ClientSampleId :