

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE122822AL\  
 Data File : FE039513.D  
 Signal(s) : FID1B.ch  
 Acq On : 28 Dec 2022 10:45  
 Operator : YP\AJ  
 Sample : N6208-01DL 5X  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 HD-01-122322DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 12/29/2022  
 Supervised By :Ankita Jodhani 12/29/2022

Integration File: autoint1.e  
 Quant Time: Dec 28 15:07:32 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 121722.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Dec 17 15:09:52 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units     |
|--------------------------------|--------|------------|----------------|
| -----                          |        |            |                |
| System Monitoring Compounds    |        |            |                |
| 9) S ortho-Terphenyl (SURR)    | 11.925 | 1236600    | 8.286 ug/ml    |
| Spiked Amount 50.000           |        | Recovery = | 16.57%         |
| 12) S 1-chlorooctadecane (S... | 13.353 | 11541284   | 100.273 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 200.55%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE122822AL\  
Data File : FE039513.D  
Signal(s) : FID1B.ch  
Acq On : 28 Dec 2022 10:45  
Operator : YP\AJ  
Sample : N6208-01DL 5X  
Misc :  
ALS Vial : 9 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
HD-01-122322DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 12/29/2022  
Supervised By :Ankita Jodhani 12/29/2022

Integration File: autoint1.e  
Quant Time: Dec 28 15:07:32 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 121722.M  
Quant Title : GC Extractables  
QLast Update : Sat Dec 17 15:09:52 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

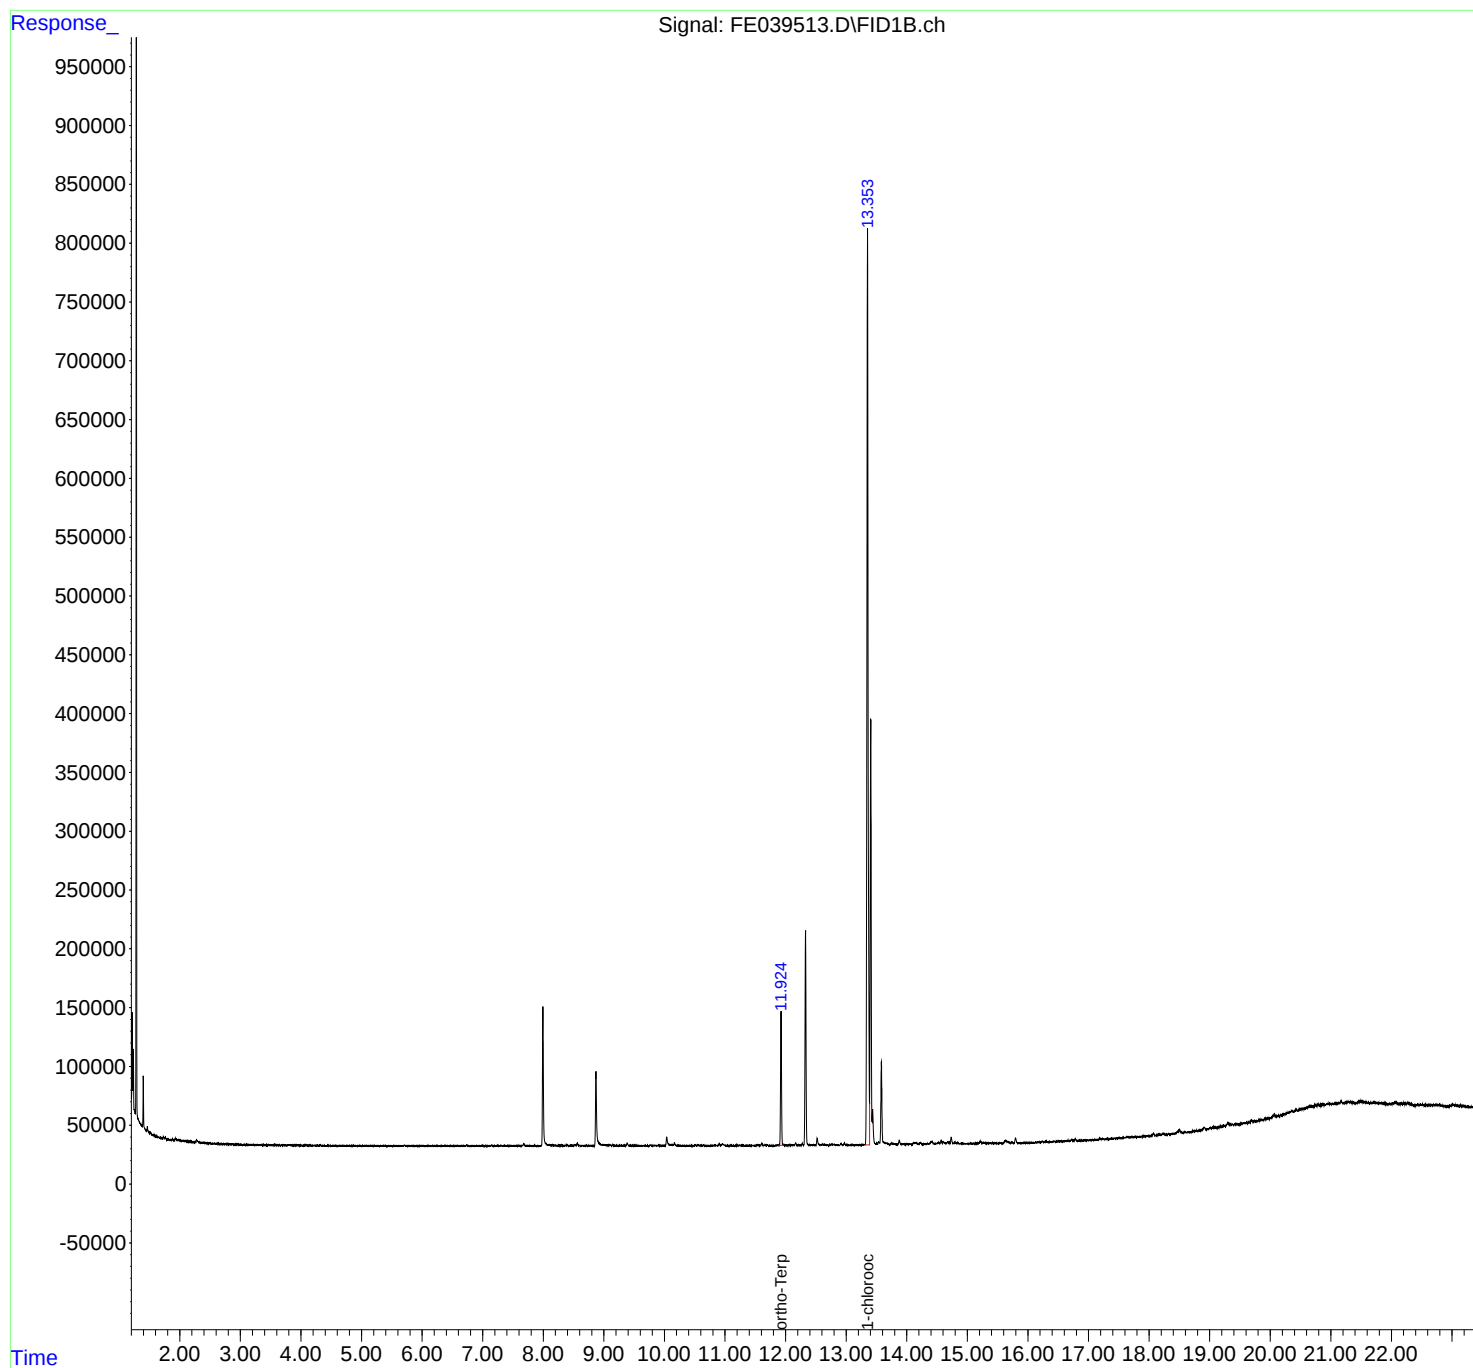

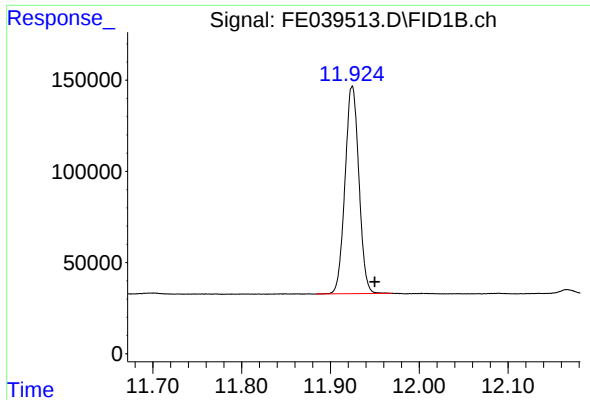


#9 ortho-Terphenyl (SURR)

R.T.: 11.925 min  
Delta R.T.: -0.025 min  
Response: 1236600  
Conc: 8.29 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
HD-01-122322DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 12/29/2022  
Supervised By :Ankita Jodhani 12/29/2022

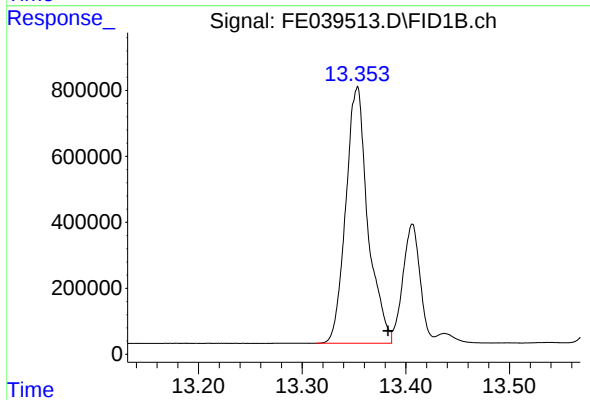

#12 1-chlorooctadecane (SURR)

R.T.: 13.353 min  
Delta R.T.: -0.030 min  
Response: 11541284  
Conc: 100.27 ug/ml m