

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE123022AL\
 Data File : FE039568.D
 Signal(s) : FID1B.ch
 Acq On : 30 Dec 2022 08:05
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 02 05:26:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 17 15:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.903	156720	1.148 ug/ml
11) T n-Heneicosane (C21)	13.522	102194	0.749 ug/ml
13) T n-Docosane (C22)	14.110	139342	1.030 ug/ml
14) T n-Tetracosane (C24)	15.215	175943	1.311 ug/ml
15) T n-Hexacosane (C26)	16.237	86397	0.664 ug/ml
16) T n-Octacosane (C28)	17.190	85093	0.661 ug/ml
17) T n-Tricontane (C30)	18.072	57185	0.444 ug/ml
18) T n-Dotriacontane (C32)	18.904	130579	1.008 ug/ml
19) T n-Tetratriacontane (C34)	19.689	64387	0.510 ug/ml
20) T n-Hexatriacontane (C36)	20.431	48732	0.403 ug/ml
21) T n-Octatriacontane (C38)	21.171	99368	0.805 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE123022AL\
Data File : FE039568.D
Signal(s) : FID1B.ch
Acq On : 30 Dec 2022 08:05
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 02 05:26:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
Quant Title : GC Extractables
QLast Update : Sat Dec 17 15:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

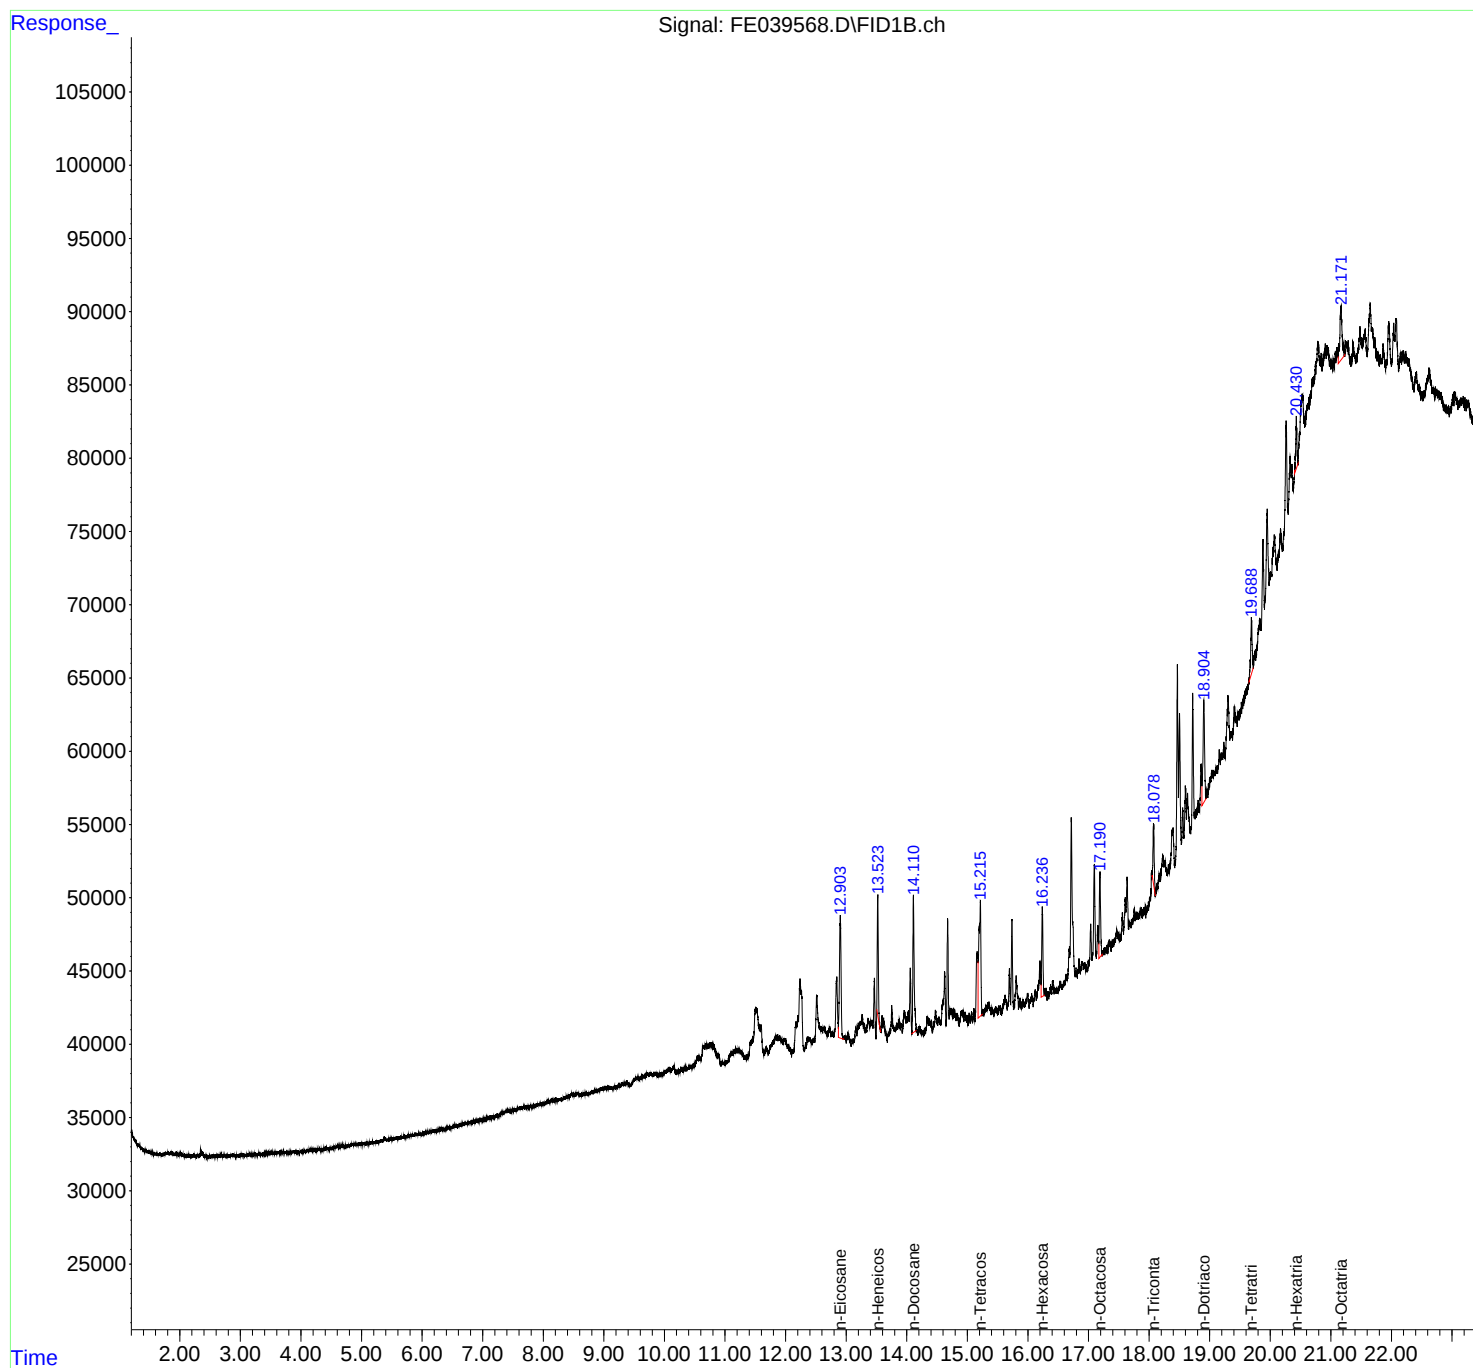


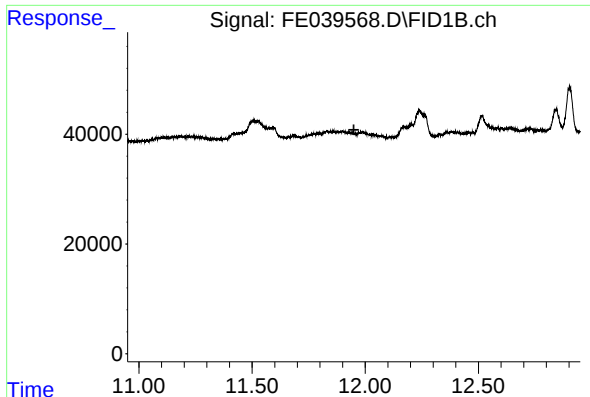

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.950 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

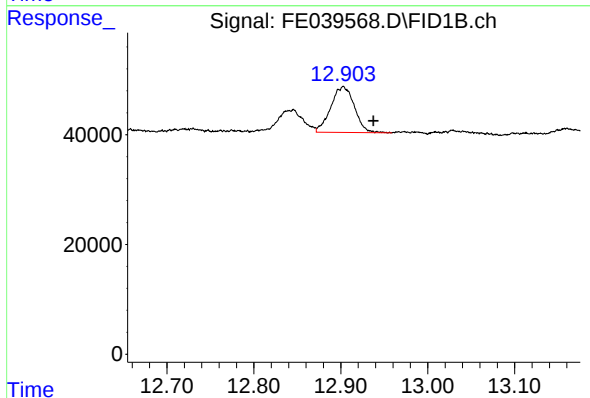


#10 n-Eicosane (C20)

R.T.: 12.903 min
Delta R.T.: -0.035 min
Response: 156720
Conc: 1.15 ug/ml

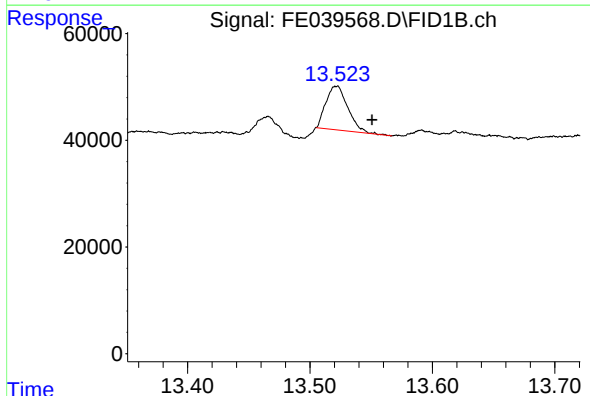


#11 n-Heneicosane (C21)

R.T.: 13.522 min
Delta R.T.: -0.029 min
Response: 102194
Conc: 0.75 ug/ml

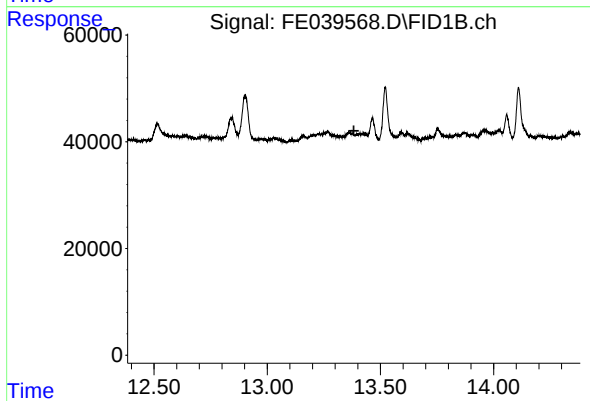

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.383 min
Response: 0
Conc: N.D.

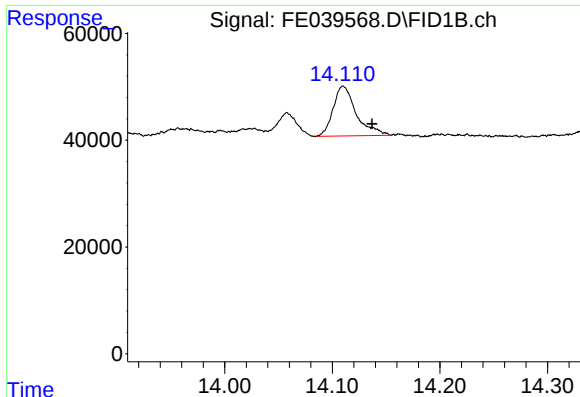

#13 n-Docosane (C22)


R.T.: 14.110 min
Delta R.T.: -0.027 min
Response: 139342
Conc: 1.03 ug/ml

Instrument :
FID_E
ClientSampleId :

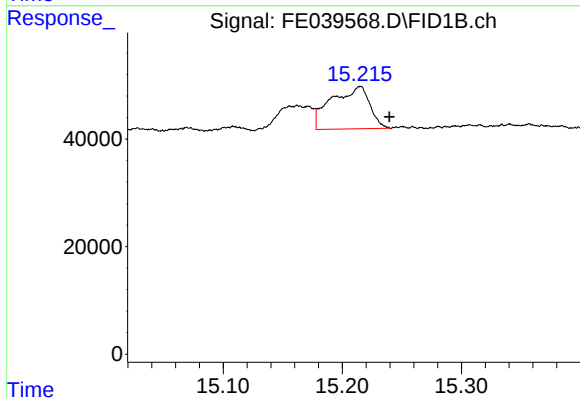


#14 n-Tetracosane (C24)

R.T.: 15.215 min
Delta R.T.: -0.025 min
Response: 175943
Conc: 1.31 ug/ml

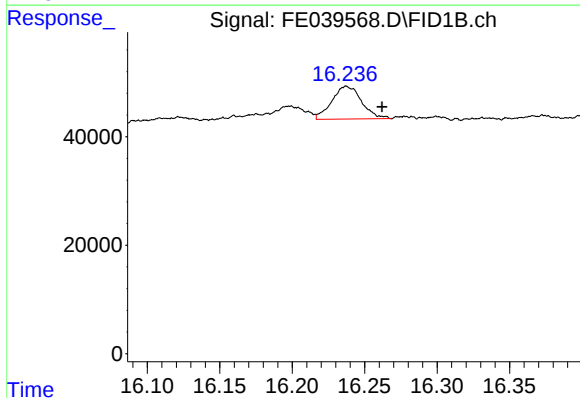


#15 n-Hexacosane (C26)

R.T.: 16.237 min
Delta R.T.: -0.025 min
Response: 86397
Conc: 0.66 ug/ml

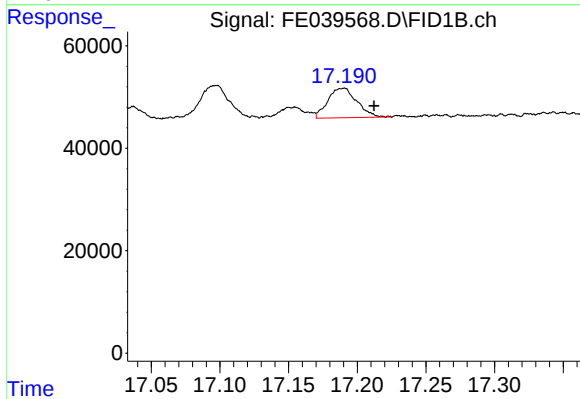

#16 n-Octacosane (C28)


R.T.: 17.190 min
Delta R.T.: -0.022 min
Response: 85093
Conc: 0.66 ug/ml

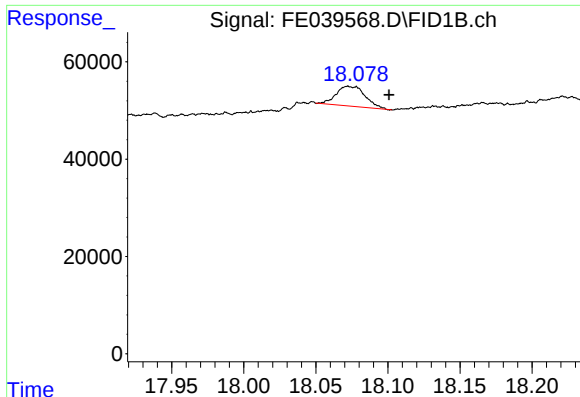

#17 n-Tricontane (C30)


R.T.: 18.072 min
Delta R.T.: -0.029 min
Response: 57185
Conc: 0.44 ug/ml

Instrument :
FID_E
ClientSampleId :

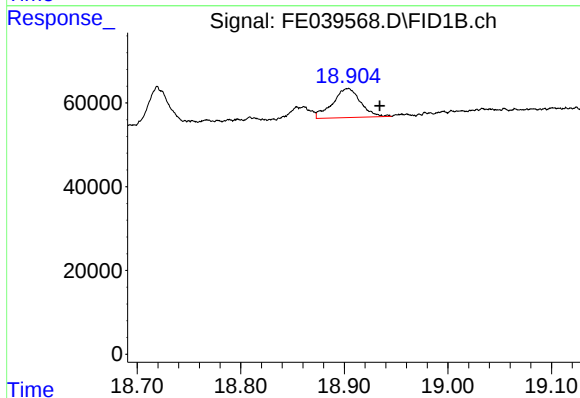


#18 n-Dotriacontane (C32)

R.T.: 18.904 min
Delta R.T.: -0.031 min
Response: 130579
Conc: 1.01 ug/ml

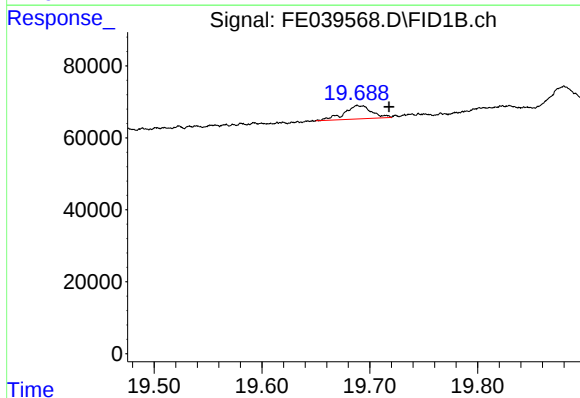


#19 n-Tetratriacontane (C34)

R.T.: 19.689 min
Delta R.T.: -0.029 min
Response: 64387
Conc: 0.51 ug/ml

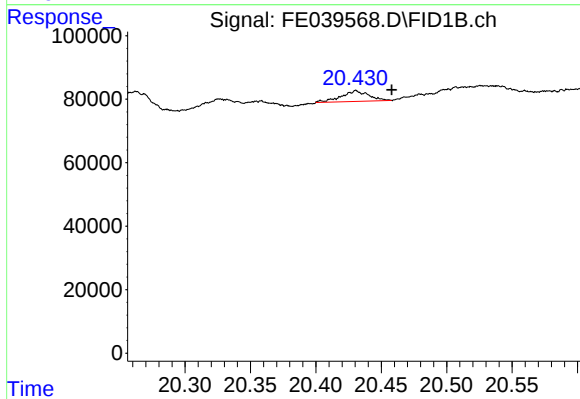

#20 n-Hexatriacontane (C36)

R.T.: 20.431 min
Delta R.T.: -0.027 min
Response: 48732
Conc: 0.40 ug/ml

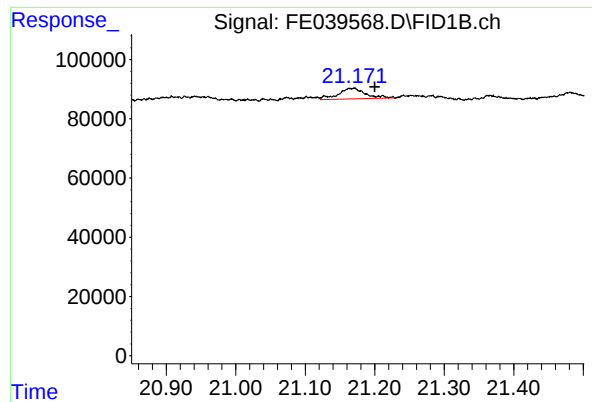

#21 n-Octatriacontane (C38)

R.T.: 21.171 min
Delta R.T.: -0.029 min
Response: 99368
Conc: 0.80 ug/ml

Instrument :

FID_E

ClientSampleId :