

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE123023\  
Data File : FE046042.D  
Signal(s) : FID1B.ch  
Acq On : 29 Dec 2023 14:00  
Operator : YP\AJ  
Sample : 05827-09  
Misc :  
ALS Vial : 34 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
RT-SB-09-10.5-11.5

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 01/02/2024  
Supervised By :Ankita Jodhani 01/02/2024

Integration File: autoint1.e  
Quant Time: Dec 29 23:40:39 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\C44-FE121423.M  
Quant Title :  
QLast Update : Thu Dec 14 11:27:22 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20m x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units    |
|--------------------------------|--------|----------|---------------|
| -----                          |        |          |               |
| System Monitoring Compounds    |        |          |               |
| 13) S TETRACOSANE-d50 (SURR... | 14.948 | 1952290  | 15.635 ug/mlm |
| Target Compounds               |        |          |               |
| -----                          |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE123023\  
Data File : FE046042.D  
Signal(s) : FID1B.ch  
Acq On : 29 Dec 2023 14:00  
Operator : YP\AJ  
Sample : 05827-09  
Misc :  
ALS Vial : 34 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
RT-SB-09-10.5-11.5


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 01/02/2024  
Supervised By :Ankita Jodhani 01/02/2024

Integration File: autoint1.e  
Quant Time: Dec 29 23:40:39 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\C44-FE121423.M  
Quant Title :  
QLast Update : Thu Dec 14 11:27:22 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20m x 0.18mm x 0.18um

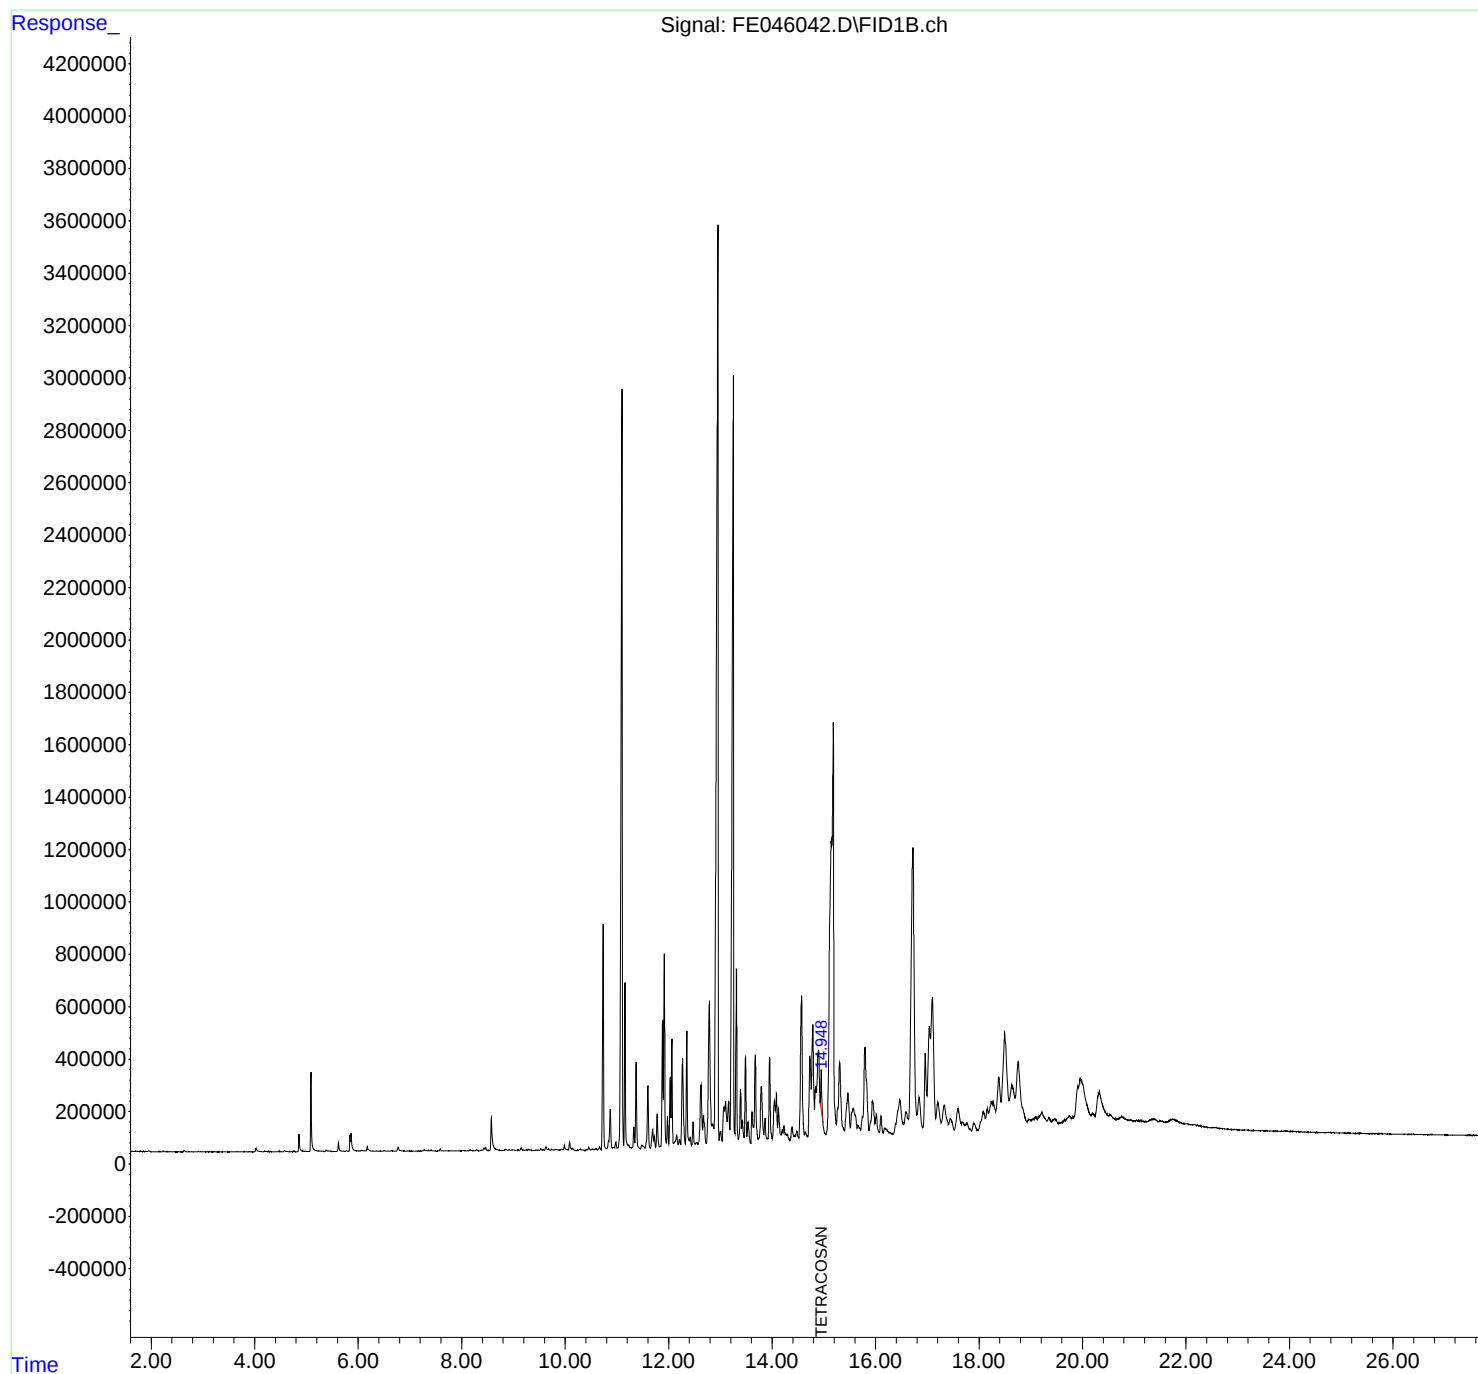

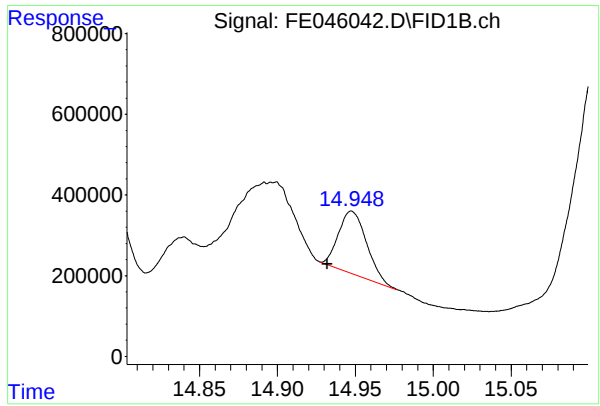

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.948 min  
Delta R.T.: 0.016 min  
Response: 1952290  
Conc: 15.63 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
RT-SB-09-10.5-11.5

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 01/02/2024  
Supervised By :Ankita Jodhani 01/02/2024