

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE123023\
Data File : FE046048.D
Signal(s) : FID1B.ch
Acq On : 29 Dec 2023 17:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Dec 29 23:41:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE121423.M
Quant Title :
QLast Update : Thu Dec 14 11:27:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.933	2230733	17.865 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE123023\
Data File : FE046048.D
Signal(s) : FID1B.ch
Acq On : 29 Dec 2023 17:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Dec 29 23:41:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE121423.M
Quant Title :
QLast Update : Thu Dec 14 11:27:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

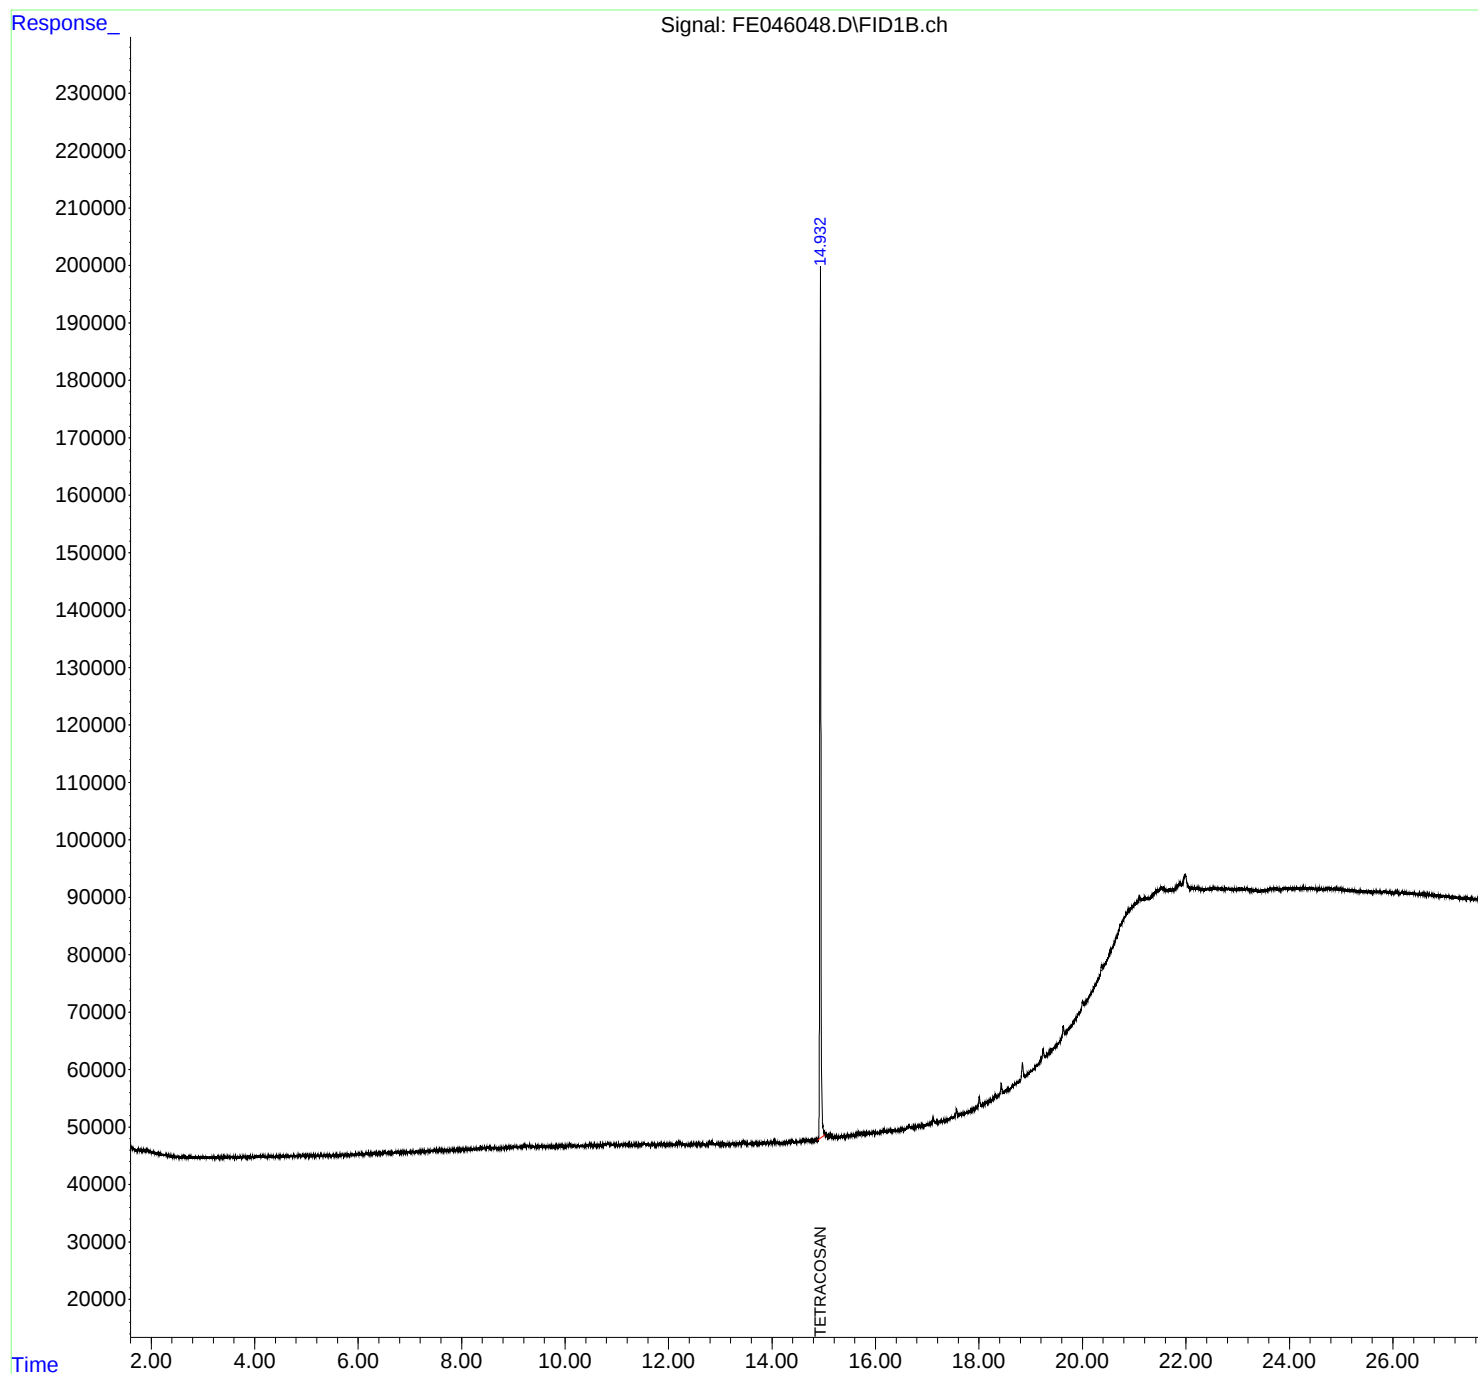

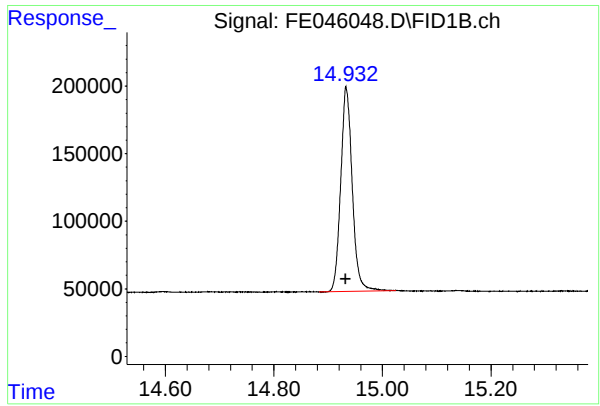

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.933 min
Delta R.T.: 0.001 min
Response: 2230733
Conc: 17.86 ug/ml

Instrument :

FID_E

ClientSampleId :

I.BLK