

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE123124AL\
Data File : FE051820.D
Signal(s) : FID1B.ch
Acq On : 31 Dec 2024 07:58
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 31 10:17:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122724.M
Quant Title : GC Extractables
QLast Update : Tue Dec 31 09:00:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
11) T	n-Heneicosane (C21)	13.696	155917	1.170 ug/ml
19) T	n-Tetratriacontane (C34)	19.847	192136	1.905 ug/ml
20) T	n-Hexatriacontane (C36)	20.588	245605	2.756 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE123124AL\
Data File : FE051820.D
Signal(s) : FID1B.ch
Acq On : 31 Dec 2024 07:58
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 31 10:17:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122724.M
Quant Title : GC Extractables
QLast Update : Tue Dec 31 09:00:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

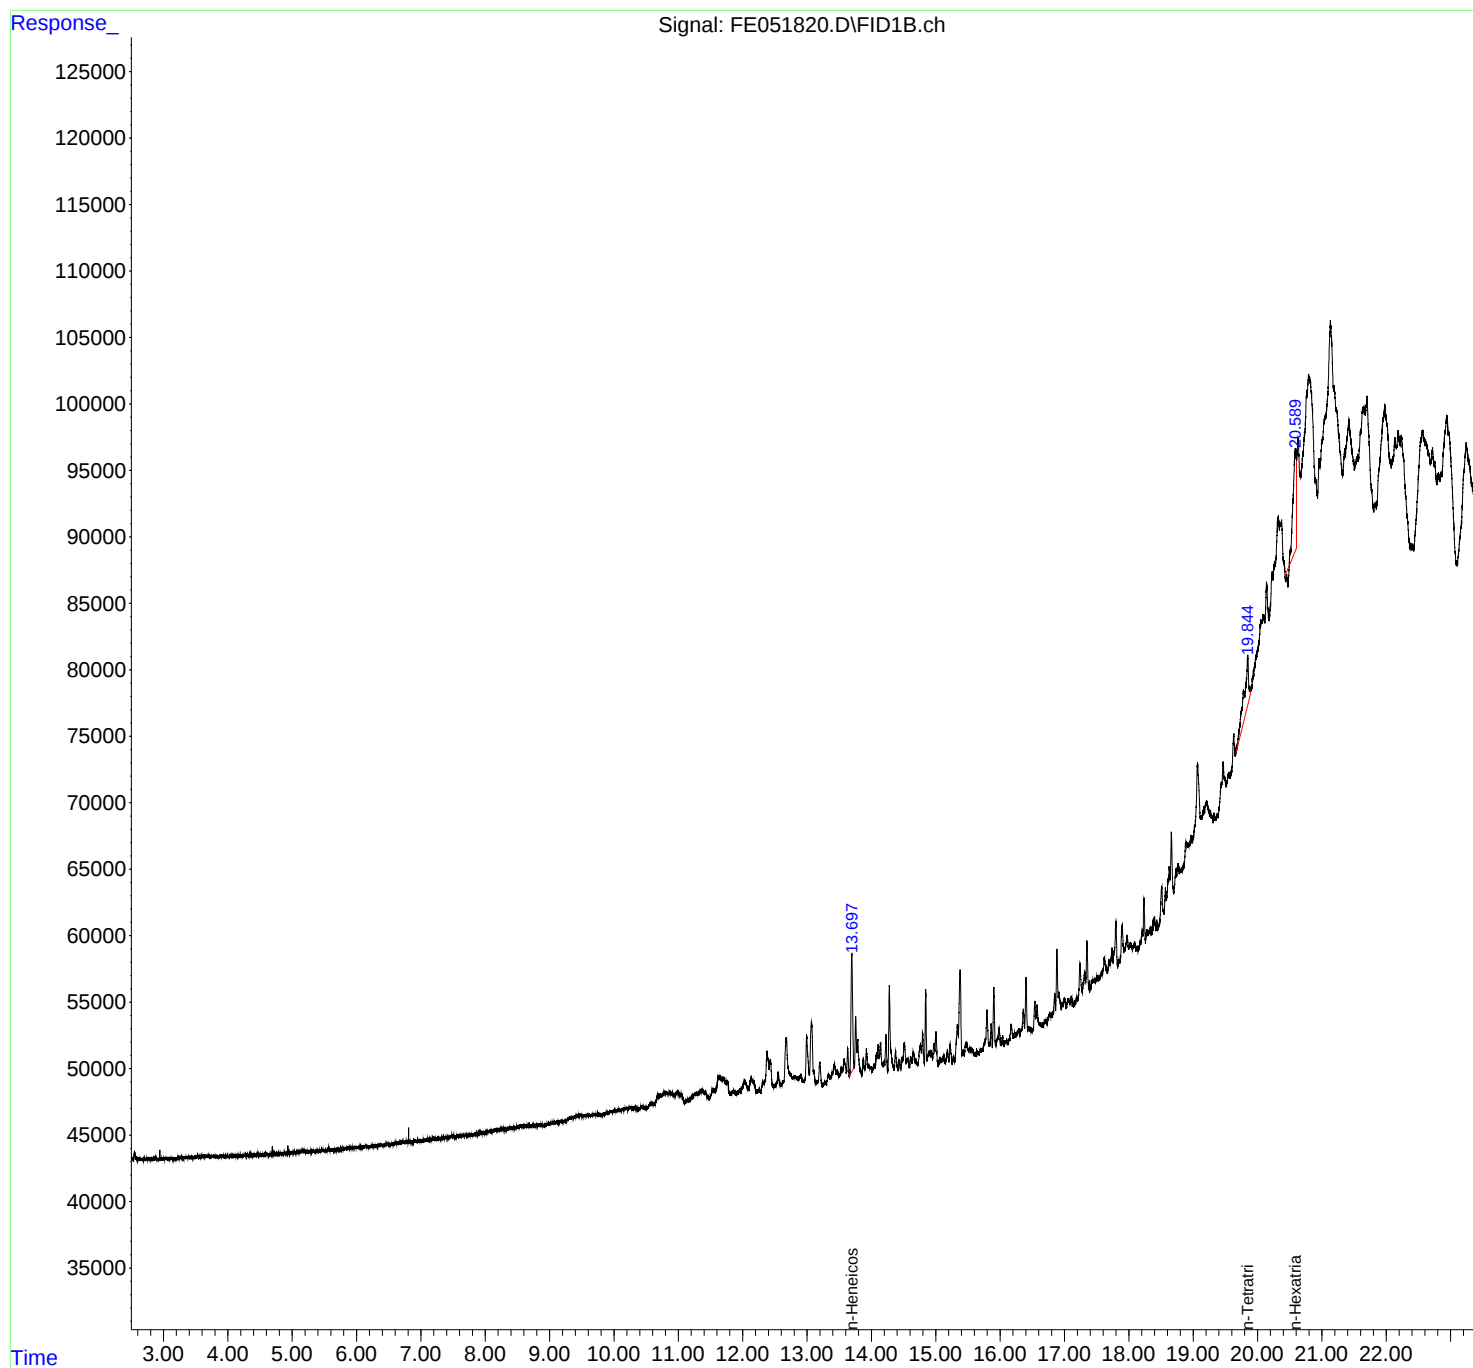


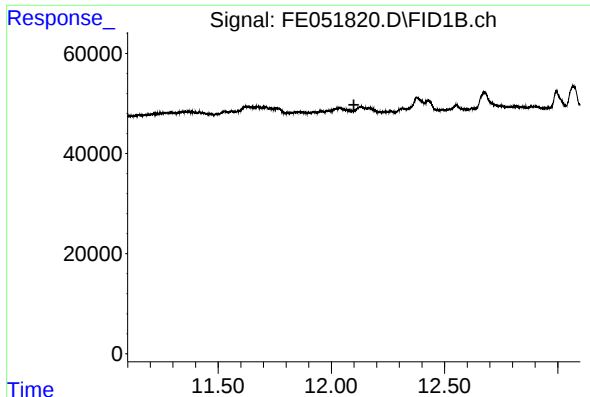

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 12.100 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

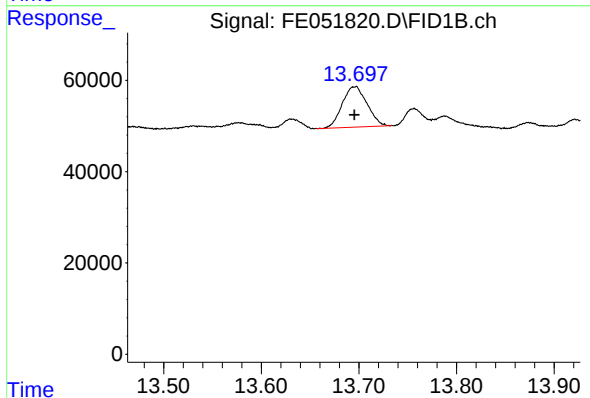


#11 n-Heneicosane (C21)

R.T.: 13.696 min
Delta R.T.: 0.000 min
Response: 155917
Conc: 1.17 ug/ml

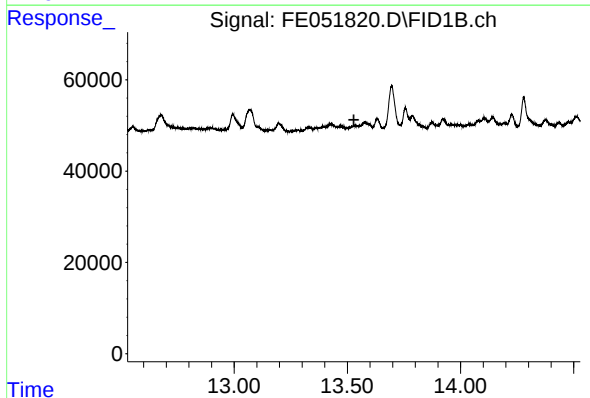


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.529 min
Response: 0
Conc: N.D.

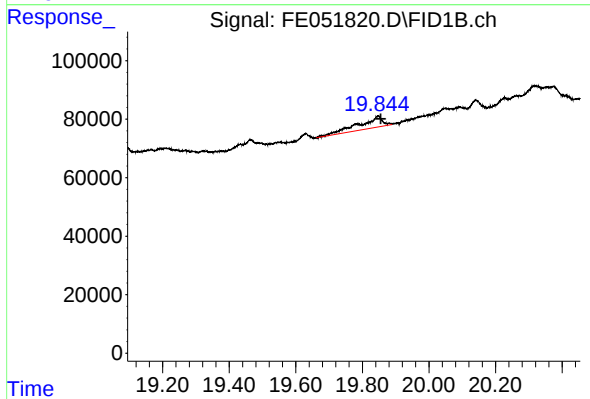

#19 n-Tetratriacontane (C34)

R.T.: 19.847 min
Delta R.T.: -0.007 min
Response: 192136
Conc: 1.90 ug/ml

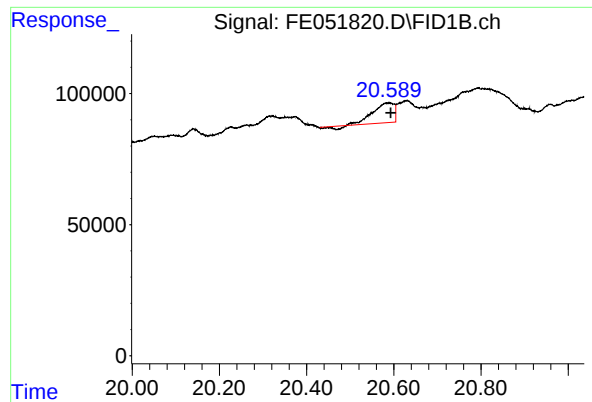

#20 n-Hexatriacontane (C36)

R.T.: 20.588 min
Delta R.T.: -0.005 min
Response: 245605
Conc: 2.76 ug/ml

Instrument :
FID_E
ClientSampleId :