

Data Path : P:\HPCHEM1\FID E\Data\FE030118AL\
Data File : FE026373.D
Signal(s) : FID1B.CH
Acq On : 02 Mar 2018 12:59
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 03 01:12:54 2018
Quant Method : P:\HPCHEM1\FID_E\methods\Alaphatic EPH 022718.M
Quant Title : GC Extractables
QLast Update : Wed Feb 28 13:48:17 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.607	96019	0.587 ug/ml
19) T	n-Tetratriacontane (C34)	19.392	275061	1.761 ug/ml
20) T	n-Hexatriacontane (C36)	20.169	105679	0.694 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID E\Data\FE030118AL\
Data File : FE026373.D
Signal(s) : FID1B.CH
Acq On : 02 Mar 2018 12:59
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 03 01:12:54 2018
Quant Method : P:\HPCHEM1\FID_E\methods\Alaphatic EPH 022718.M
Quant Title : GC Extractables
QLast Update : Wed Feb 28 13:48:17 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

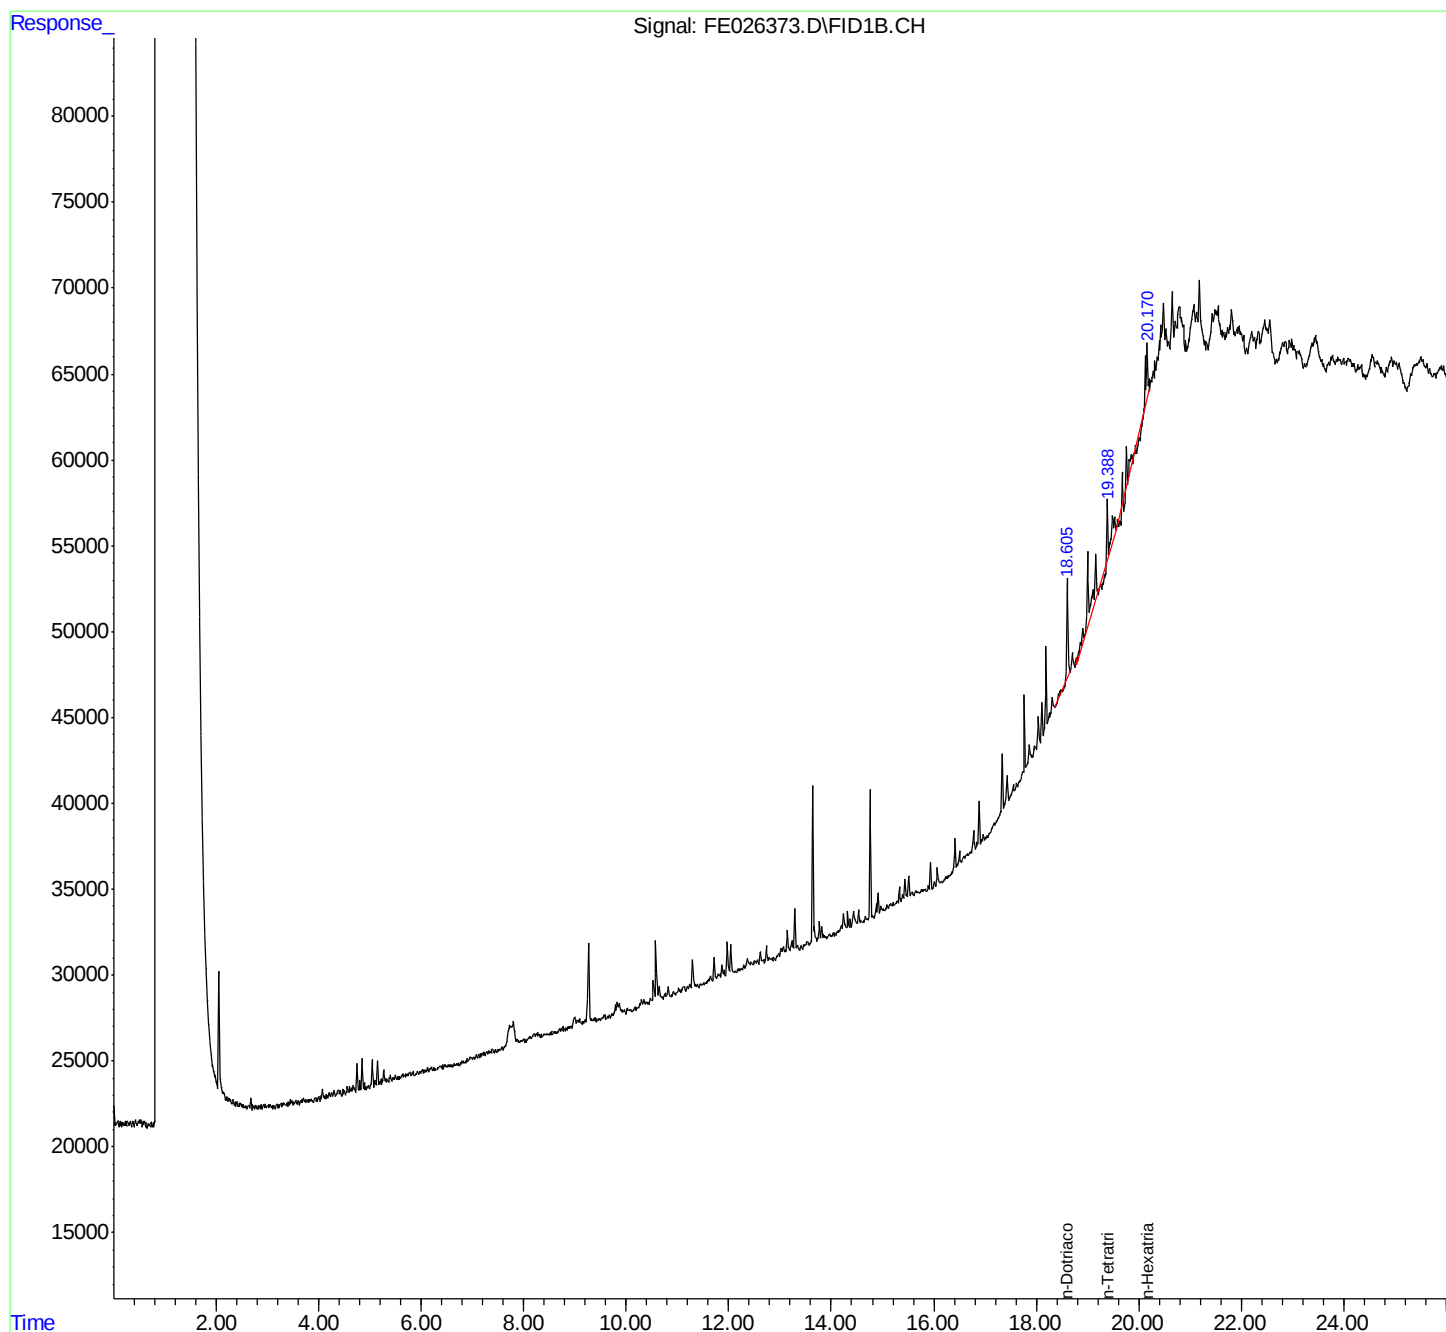

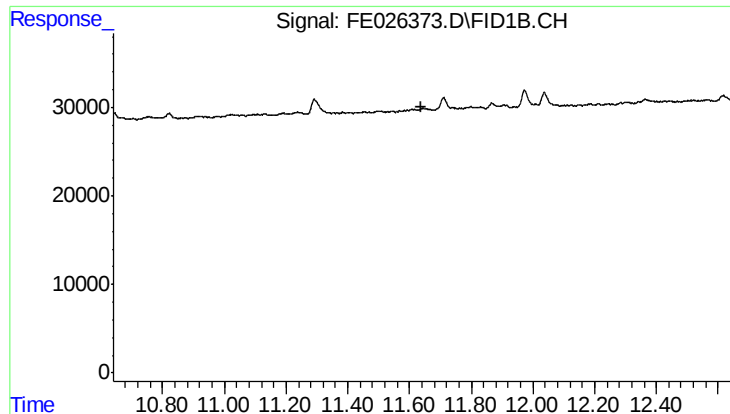


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.640 min
Response: 0
Conc: N.D.

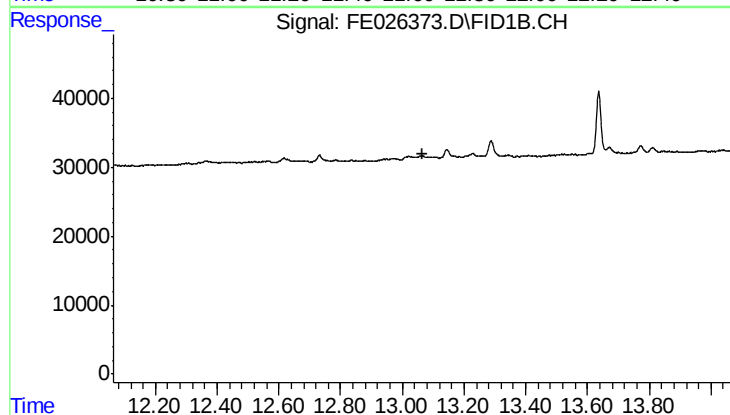


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.064 min
Response: 0
Conc: N.D.

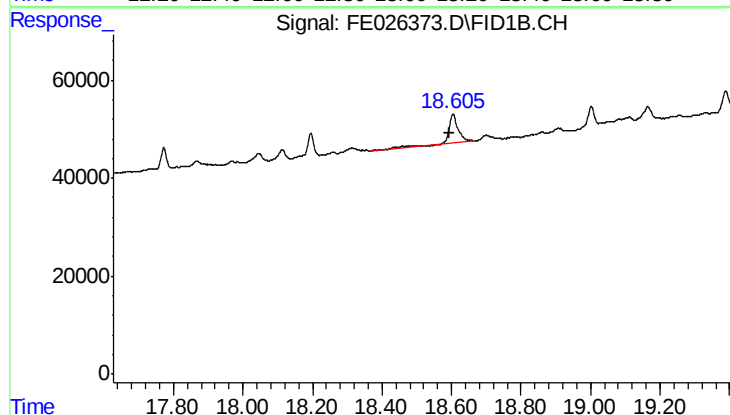


#18 n-Dotriacontane (C32)

R.T.: 18.607 min
Delta R.T.: 0.012 min
Response: 96019
Conc: 0.59 ug/ml

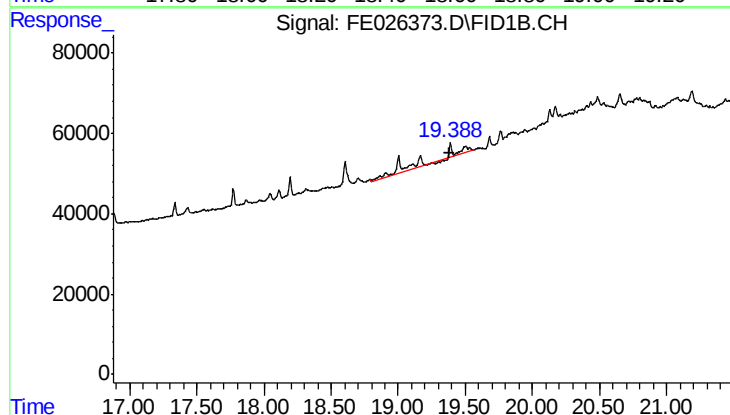

#19 n-Tetratriacontane (C34)

R.T.: 19.392 min
Delta R.T.: 0.015 min
Response: 275061
Conc: 1.76 ug/ml

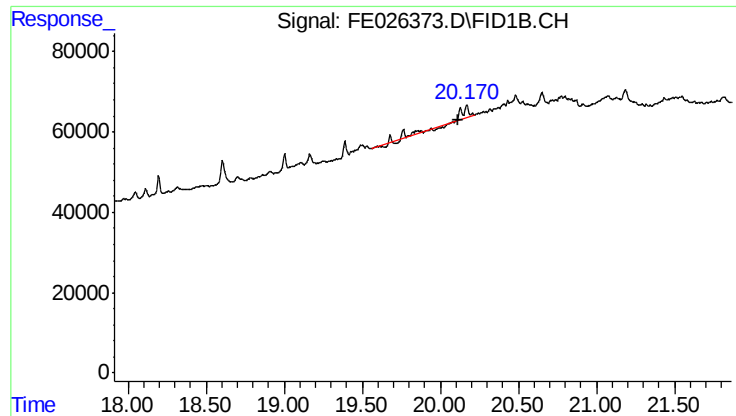

#20 n-Hexatriacontane (C36)

R.T.: 20.169 min
Delta R.T.: 0.054 min
Response: 105679
Conc: 0.69 ug/ml