

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082918\
Data File : FE028598.D
Signal(s) : FID1B.CH
Acq On : 29 Aug 2018 15:43
Operator : AJ\SJ
Sample : J4671-01MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 29 16:13:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
Quant Title :
QLast Update : Tue Aug 21 14:35:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.959	1401057	4.999 ug/mlm
Target Compounds			
1) N-OCTANE	2.536	1189314	9.874 ug/ml
3) N-DECANE	4.655	2544222	12.886 ug/ml
4) N-UNDECANE	5.697	143892	0.996 ug/ml
5) N-DODECANE	6.685	2946756	19.555 ug/ml
6) N-TETRADECANE	8.517	964664	5.781 ug/ml
15) N-TETRACONTANE	22.352	2203292	19.090 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082918\
Data File : FE028598.D
Signal(s) : FID1B.CH
Acq On : 29 Aug 2018 15:43
Operator : AJ\SJ
Sample : J4671-01MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 29 16:13:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
Quant Title :
QLast Update : Tue Aug 21 14:35:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

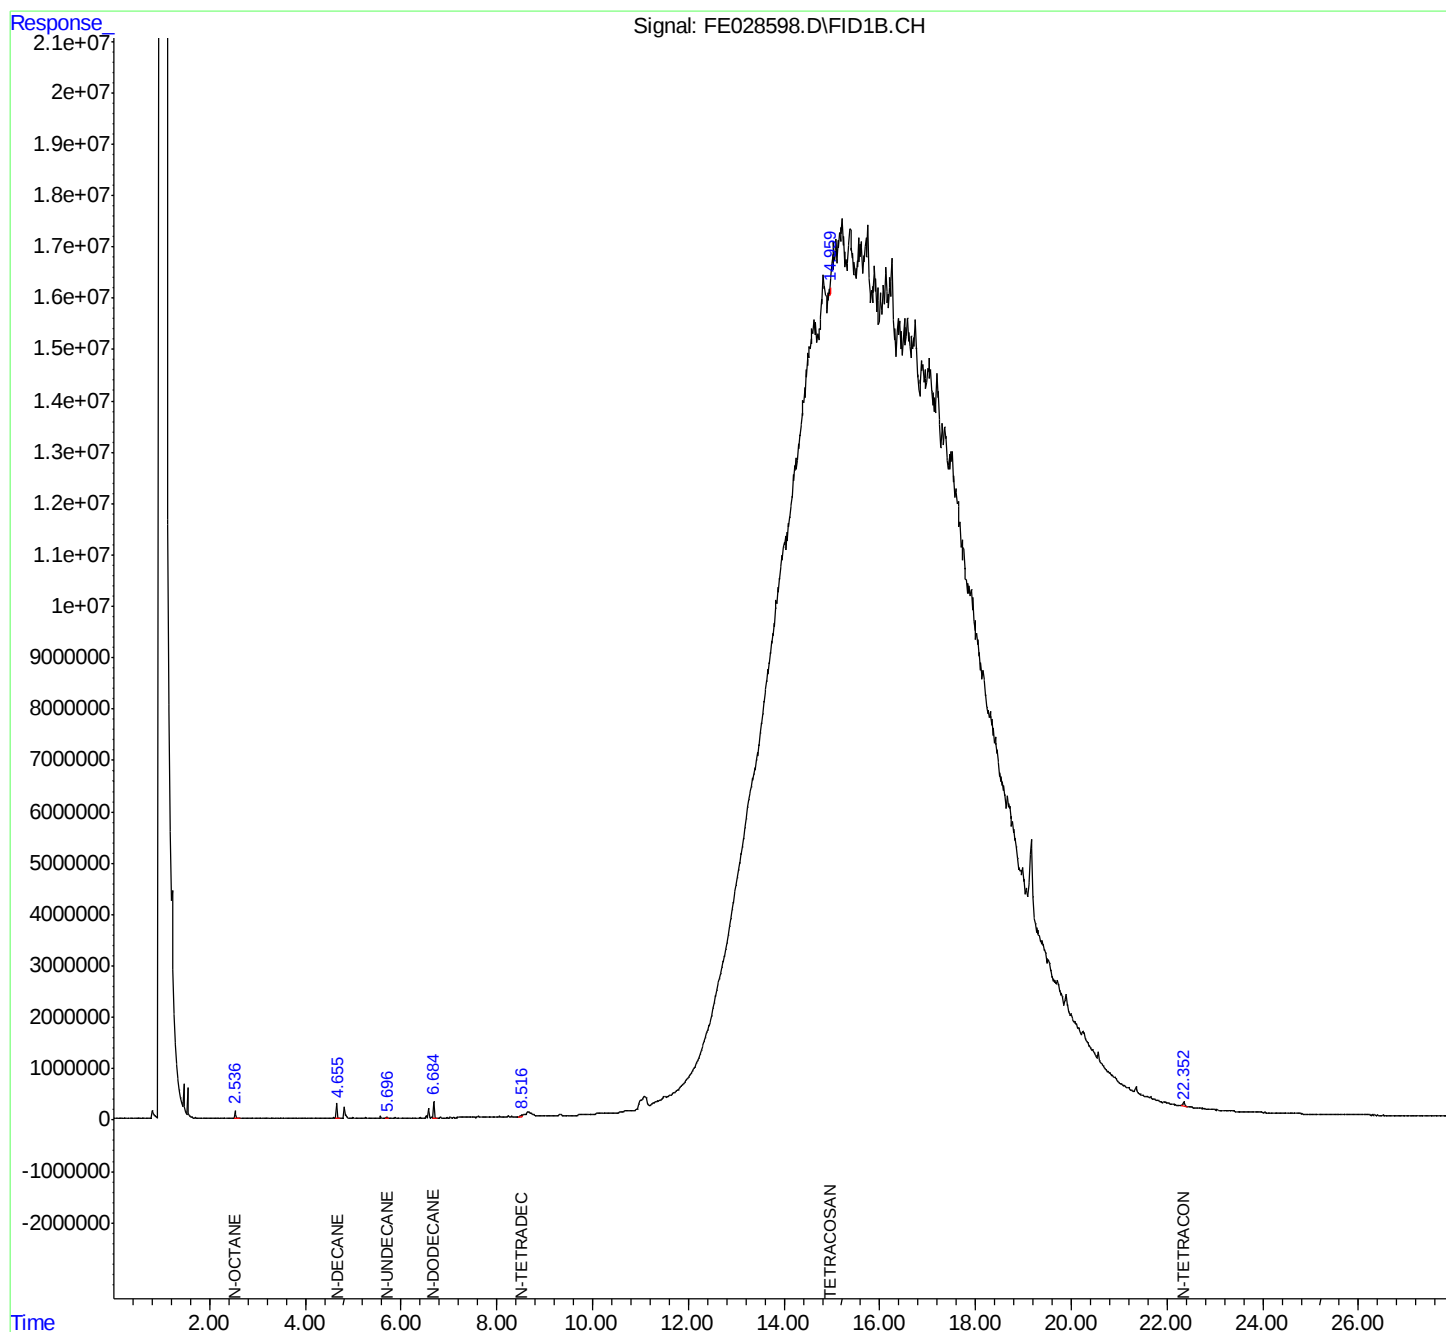

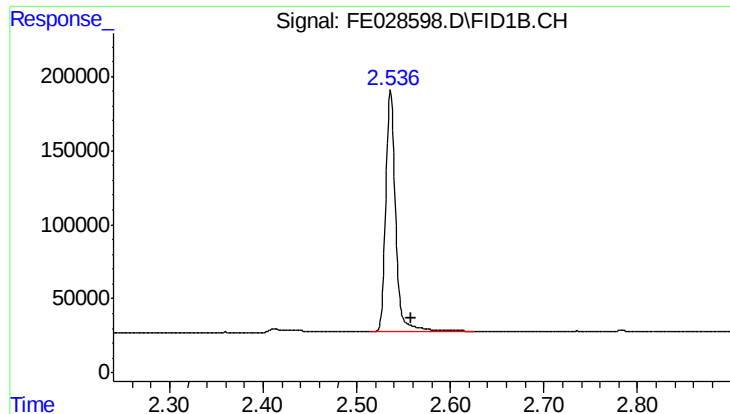


#1 N-OCTANE

R.T.: 2.536 min
Delta R.T.: -0.022 min
Response: 1189314
Conc: 9.87 ug/ml

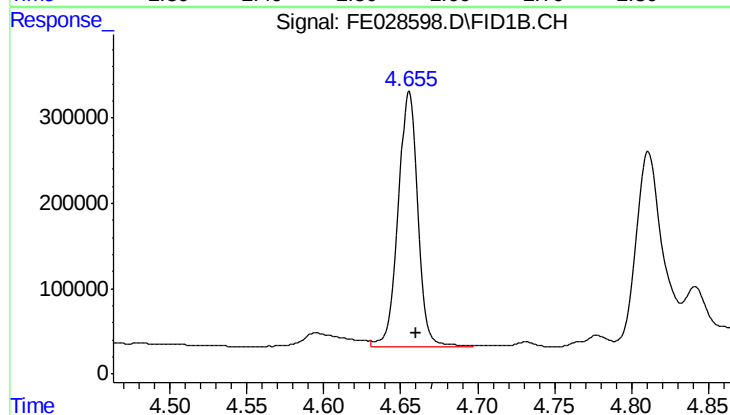


#3 N-DECANE

R.T.: 4.655 min
Delta R.T.: -0.005 min
Response: 2544222
Conc: 12.89 ug/ml

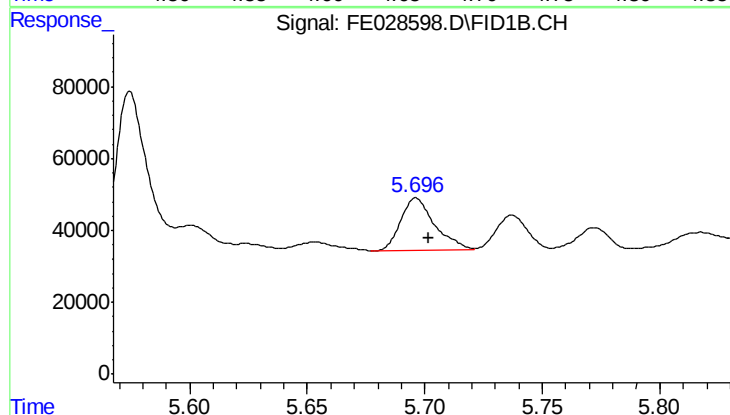


#4 N-UNDECANE

R.T.: 5.697 min
Delta R.T.: -0.005 min
Response: 143892
Conc: 1.00 ug/ml

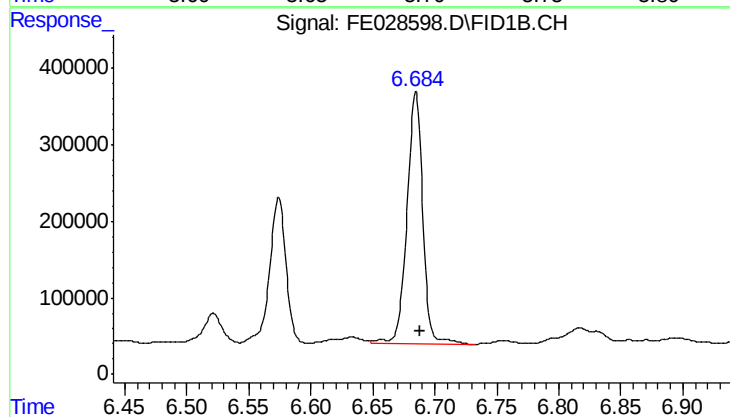


#5 N-DODECANE

R.T.: 6.685 min
Delta R.T.: -0.004 min
Response: 2946756
Conc: 19.55 ug/ml

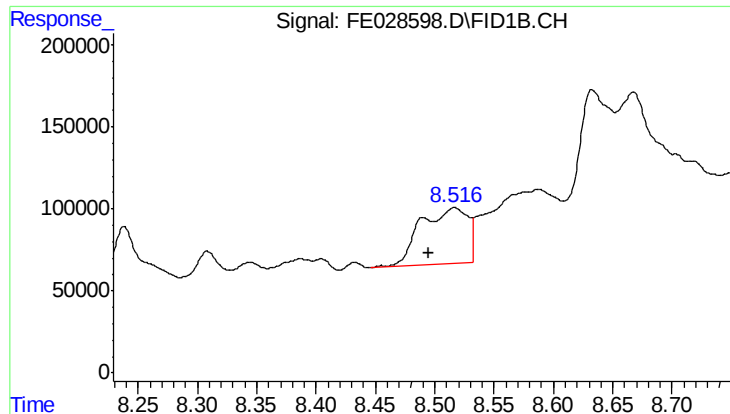


#6 N-TETRADECANE

R.T.: 8.517 min
Delta R.T.: 0.022 min
Response: 964664
Conc: 5.78 ug/ml

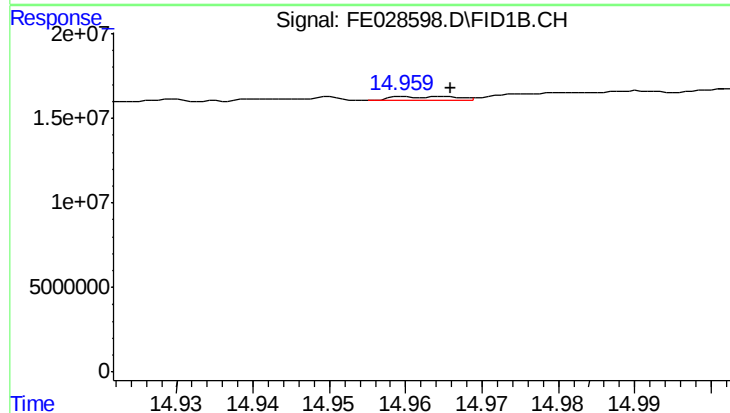

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.959 min
Delta R.T.: -0.006 min
Response: 1401057
Conc: 5.00 ug/ml m

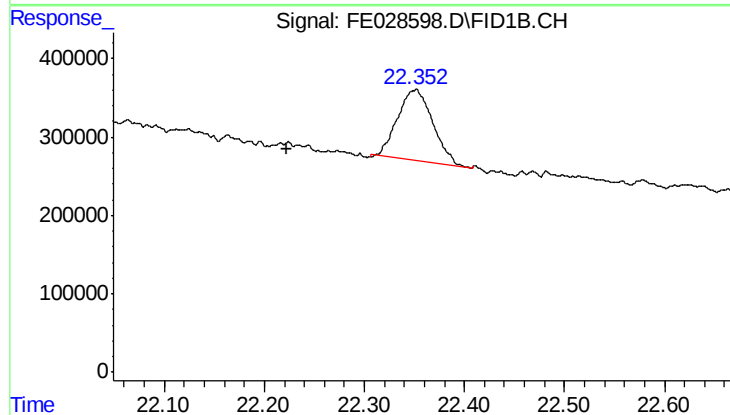

#15 N-TETRACONTANE

R.T.: 22.352 min
Delta R.T.: 0.129 min
Response: 2203292
Conc: 19.09 ug/ml m