

Data Path : P:\HPCHEM1\FID_E\Data\FE011318\
 Data File : FE025562.D
 Signal(s) : FID1B.CH
 Acq On : 13 Jan 2018 20:18
 Operator : UA/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 15 08:39:23 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Fri Jan 12 18:22:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.847	3253439	17.887 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.902	64957	0.411 ug/ml
14)	N-DOTRIACONTANE	18.734	109110	0.673 ug/ml
15)	N-TETRATRIACONTANE	19.514	49209	0.317 ug/ml
16)	N-HEXATRIACONTANE	20.288	39563	0.298 ug/ml
18)	N-TETRACONTANE	21.972	136196	1.063 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE011318\
Data File : FE025562.D
Signal(s) : FID1B.CH
Acq On : 13 Jan 2018 20:18
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 15 08:39:23 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

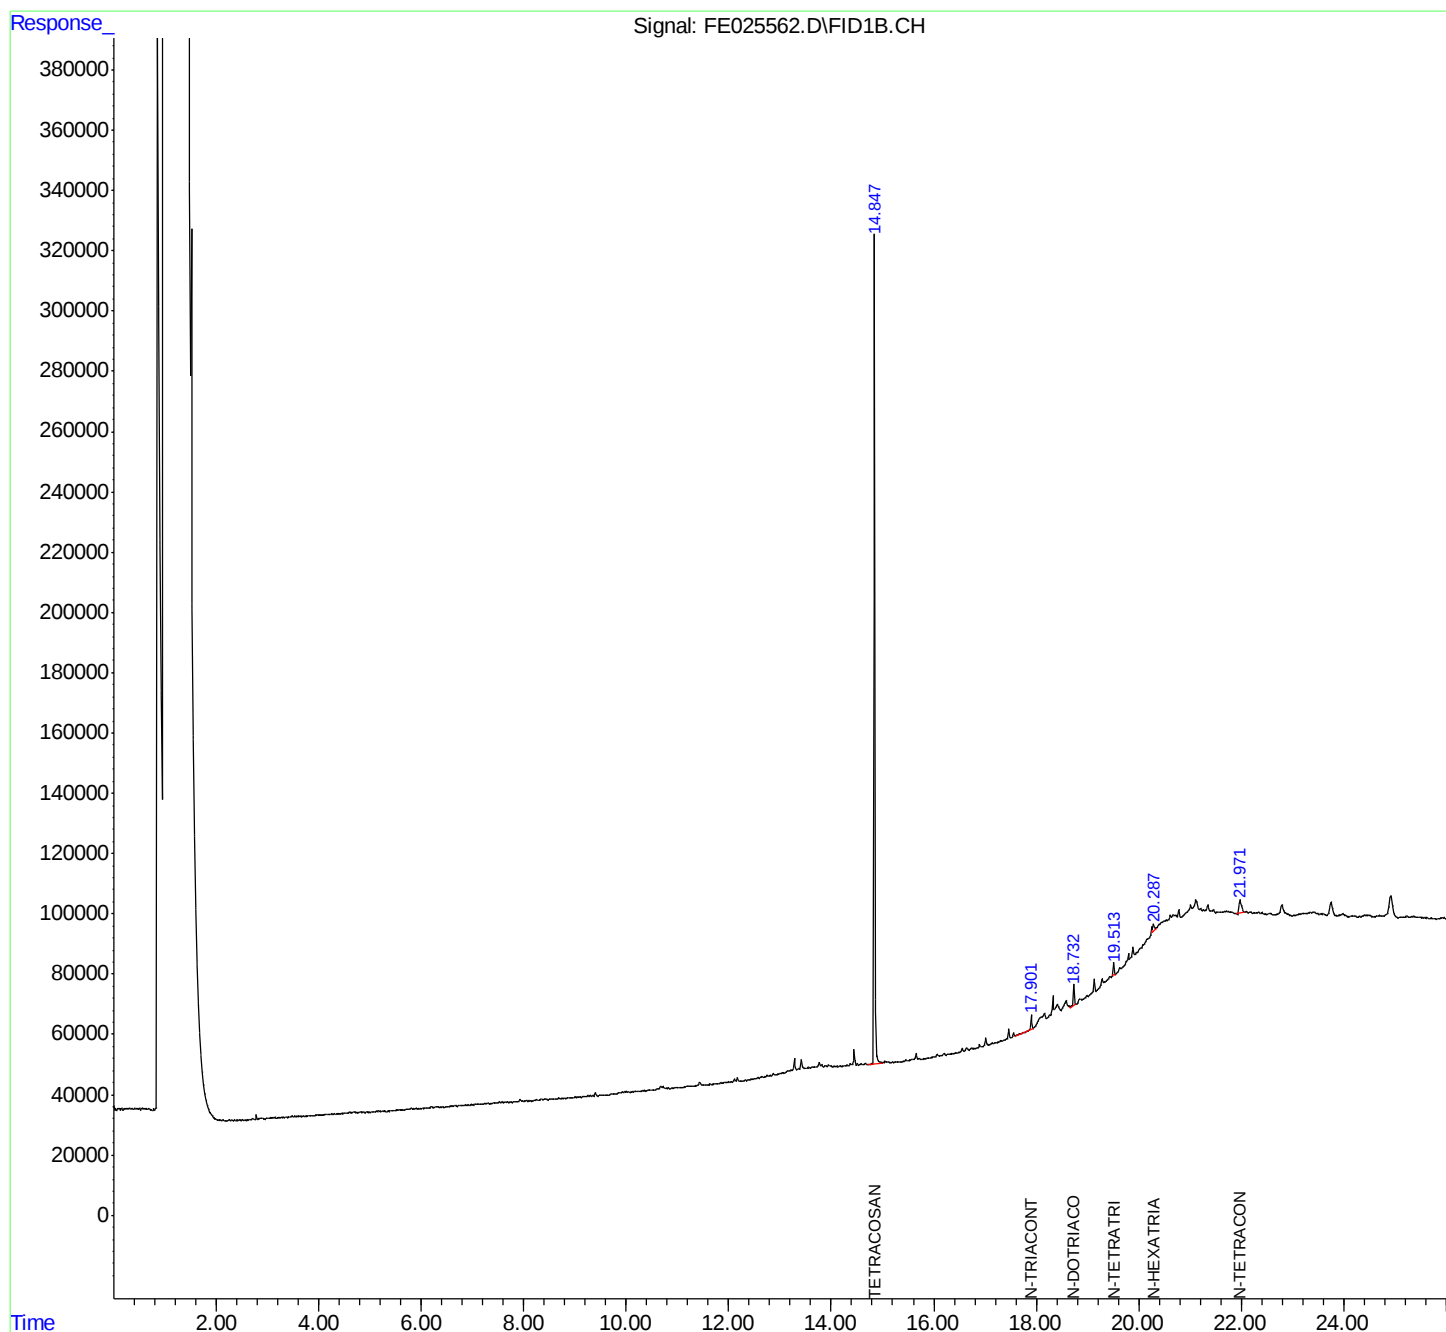


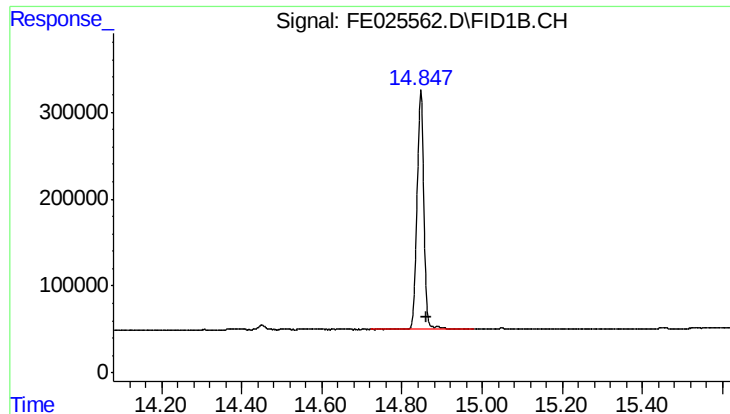

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.847 min
Delta R.T.: -0.014 min
Response: 3253439
Conc: 17.89 ug/ml

Instrument :
FID_E
ClientSampleId :

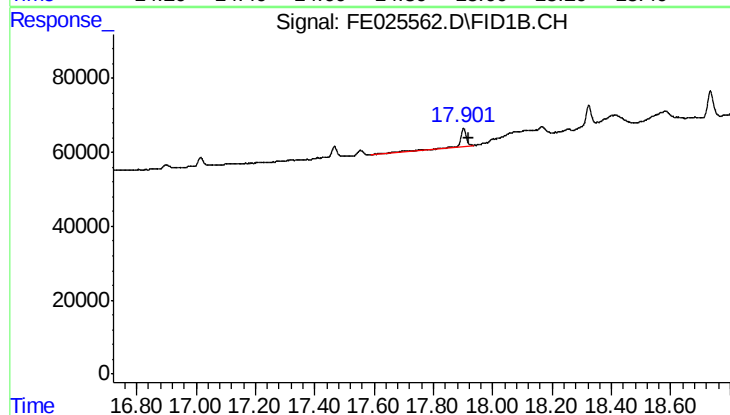


#13 N-TRIACONTANE

R.T.: 17.902 min
Delta R.T.: -0.019 min
Response: 64957
Conc: 0.41 ug/ml

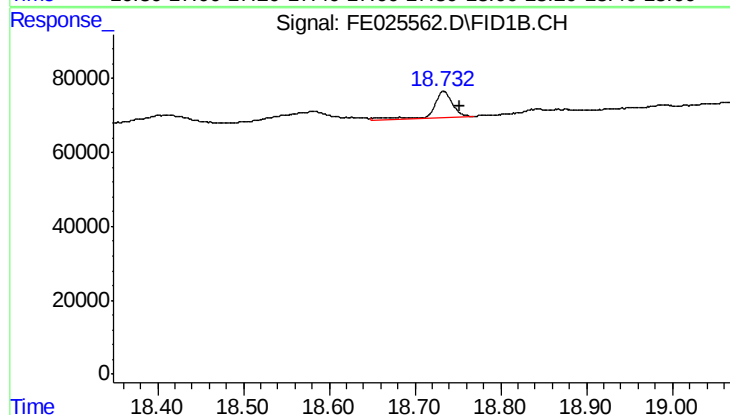


#14 N-DOTRIACONTANE

R.T.: 18.734 min
Delta R.T.: -0.019 min
Response: 109110
Conc: 0.67 ug/ml

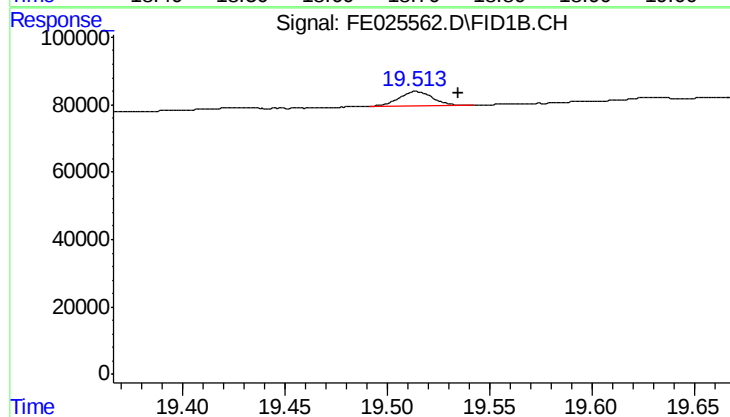

#15 N-TETRATRIACONTANE


R.T.: 19.514 min
Delta R.T.: -0.020 min
Response: 49209
Conc: 0.32 ug/ml

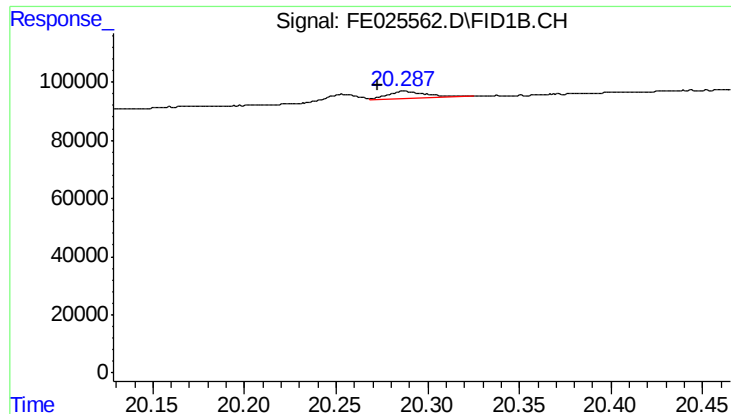

#16 N-HEXATRIACONTANE

R.T.: 20.288 min
Delta R.T.: 0.016 min
Response: 39563
Conc: 0.30 ug/ml

Instrument :
FID_E
ClientSampleId :

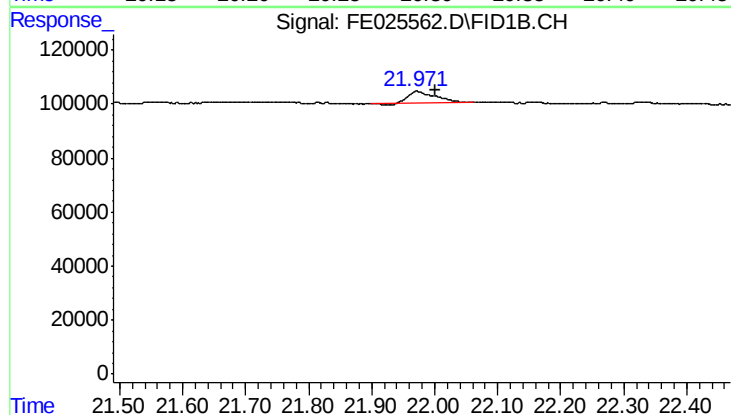

#18 N-TETRACONTANE

R.T.: 21.972 min
Delta R.T.: -0.029 min
Response: 136196
Conc: 1.06 ug/ml