

Data Path : P:\HPCHEM1\FID_E\Data\FE011318\
 Data File : FE025567.D
 Signal(s) : FID1B.CH
 Acq On : 13 Jan 2018 23:11
 Operator : UA/AJ
 Sample : J1078-02
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 15 08:40:36 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Fri Jan 12 18:22:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.842	2102353	11.559 ug/ml
Target Compounds			
4) N-TETRADECANE	8.406	464519	2.549 ug/ml
5) N-HEXADECANE	9.994	313857	1.537 ug/ml
6) N-OCTADECANE	11.434	182316	0.825 ug/ml
8) N-DOCOSANE	13.939	101905	0.464 ug/ml
10) N-TETRACOSANE	15.043	450675	2.113 ug/ml
11) N-HEXACOSANE	16.062	255756	1.327 ug/ml
12) N-OCTACOSANE	17.048	162930	0.969 ug/ml
13) N-TRIACONTANE	17.879	863354	5.468 ug/ml
14) N-DOTRIACONTANE	18.722	553465	3.412 ug/ml
15) N-TETRATRIACONTANE	19.510	44118	0.284 ug/ml
16) N-HEXATRIACONTANE	20.284	77967	0.587 ug/ml
18) N-TETRACONTANE	22.001	204844	1.599 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE011318\
Data File : FE025567.D
Signal(s) : FID1B.CH
Acq On : 13 Jan 2018 23:11
Operator : UA/AJ
Sample : J1078-02
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 15 08:40:36 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

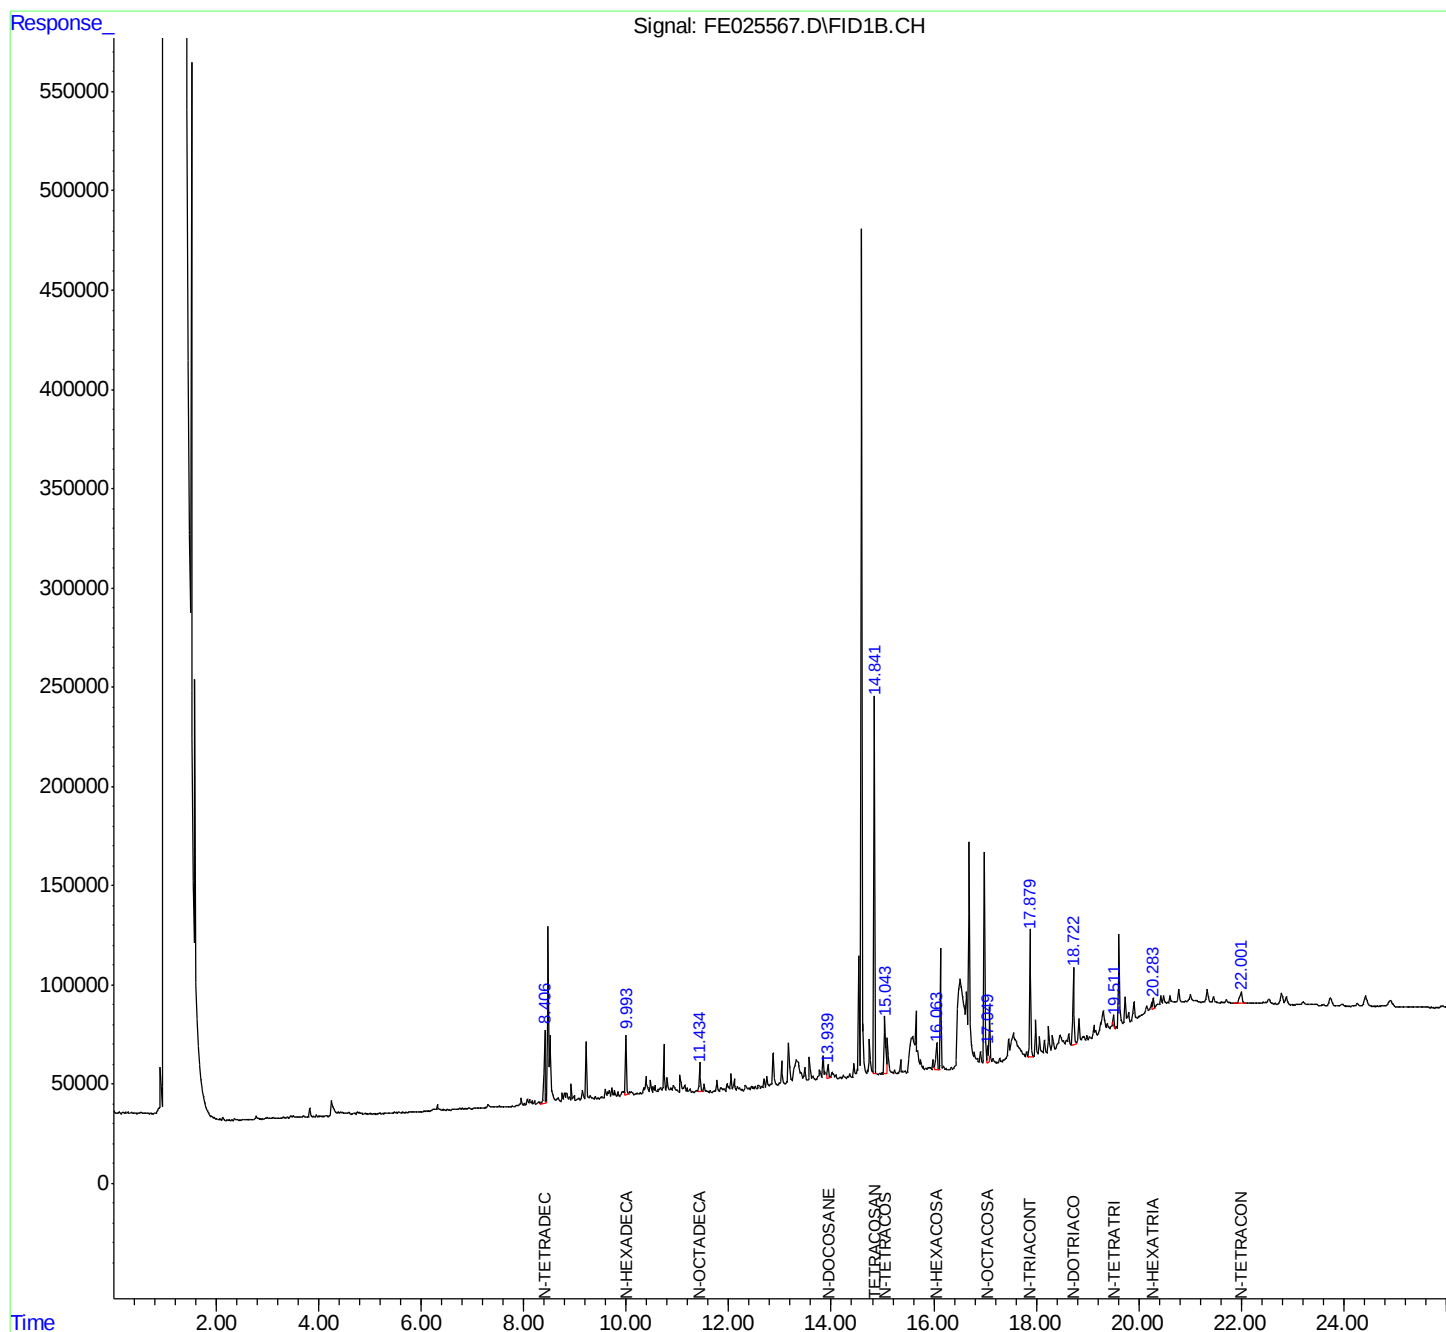


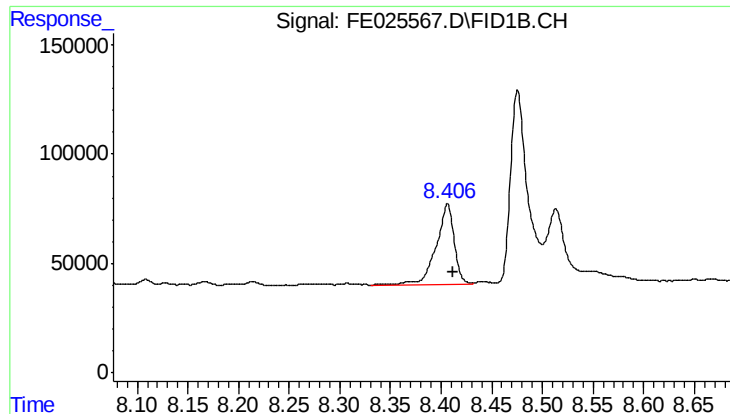

#4 N-TETRADECANE


R.T.: 8.406 min
Delta R.T.: -0.006 min
Response: 464519
Conc: 2.55 ug/ml

Instrument :
FID_E
ClientSampleId :

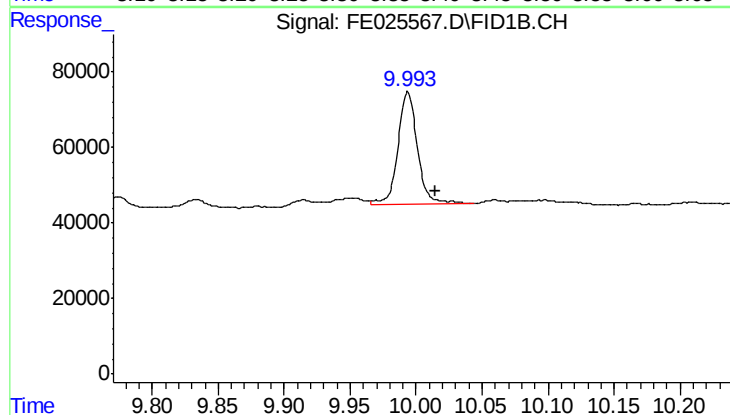


#5 N-HEXADECANE

R.T.: 9.994 min
Delta R.T.: -0.021 min
Response: 313857
Conc: 1.54 ug/ml

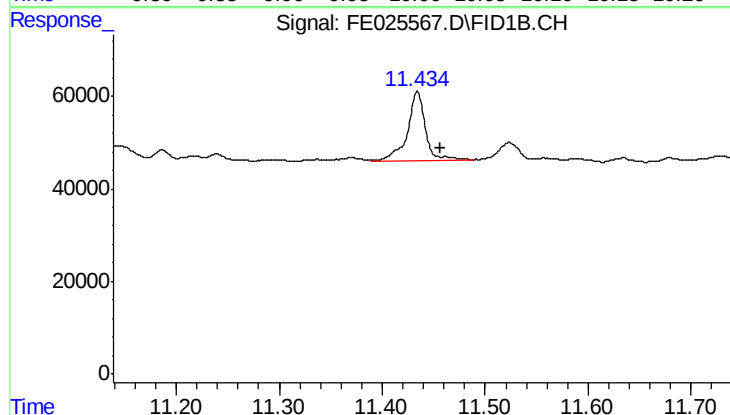


#6 N-OCTADECANE

R.T.: 11.434 min
Delta R.T.: -0.022 min
Response: 182316
Conc: 0.82 ug/ml

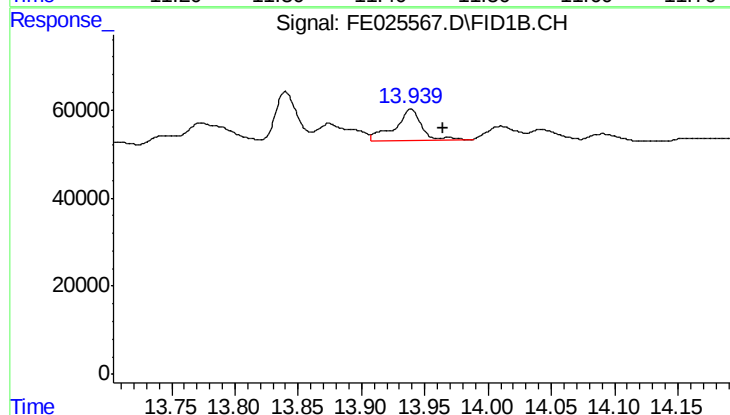

#8 N-DOCOSANE


R.T.: 13.939 min
Delta R.T.: -0.025 min
Response: 101905
Conc: 0.46 ug/ml

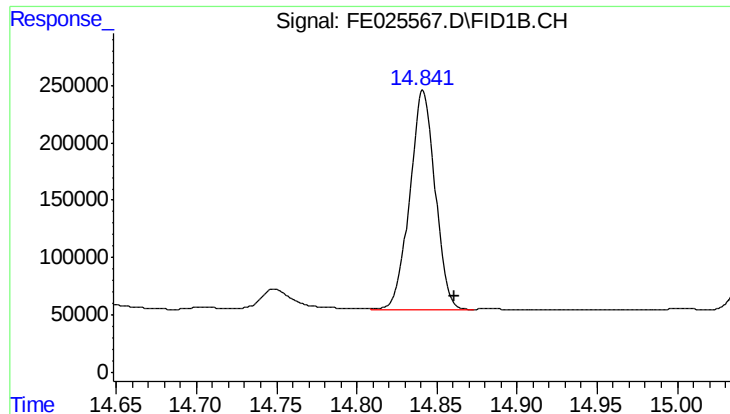

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.842 min
Delta R.T.: -0.020 min
Response: 2102353
Conc: 11.56 ug/ml

Instrument :
FID_E
ClientSampleId :

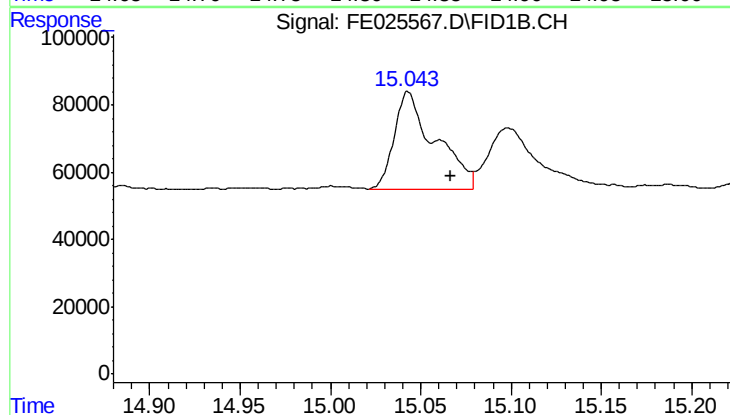


#10 N-TETRACOSANE

R.T.: 15.043 min
Delta R.T.: -0.023 min
Response: 450675
Conc: 2.11 ug/ml

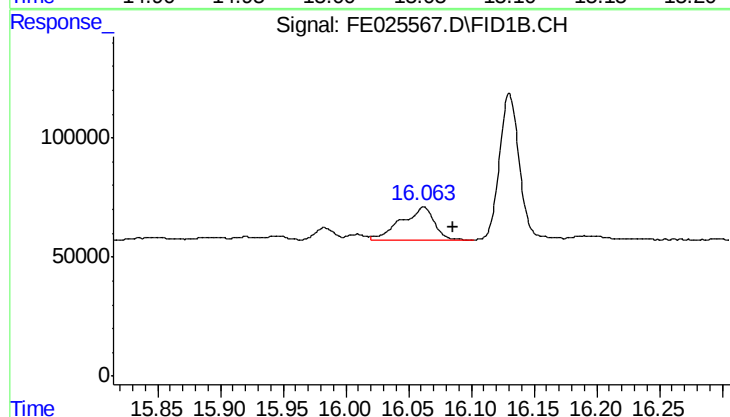


#11 N-HEXACOSANE

R.T.: 16.062 min
Delta R.T.: -0.024 min
Response: 255756
Conc: 1.33 ug/ml

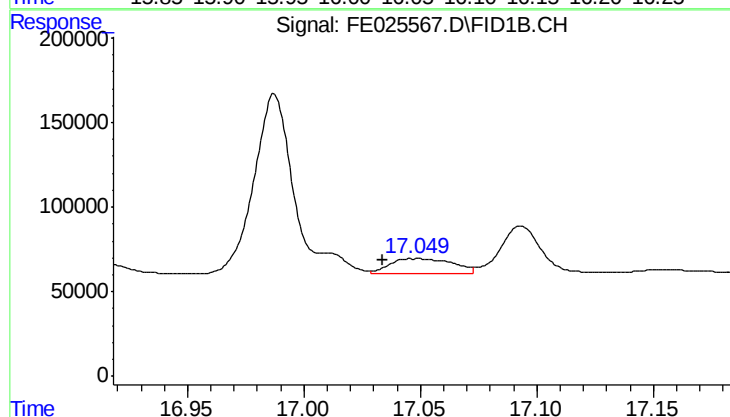

#12 N-OCTACOSANE


R.T.: 17.048 min
Delta R.T.: 0.014 min
Response: 162930
Conc: 0.97 ug/ml

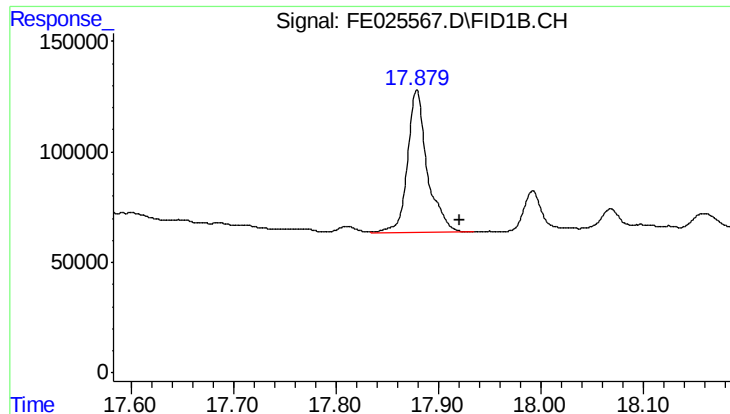

#13 N-TRIACONTANE


R.T.: 17.879 min
Delta R.T.: -0.042 min
Response: 863354
Conc: 5.47 ug/ml

Instrument :
FID_E
ClientSampleId :

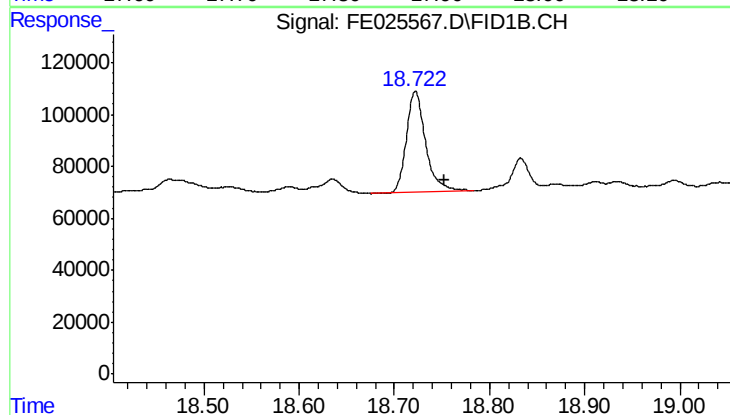


#14 N-DOTRIACONTANE

R.T.: 18.722 min
Delta R.T.: -0.031 min
Response: 553465
Conc: 3.41 ug/ml

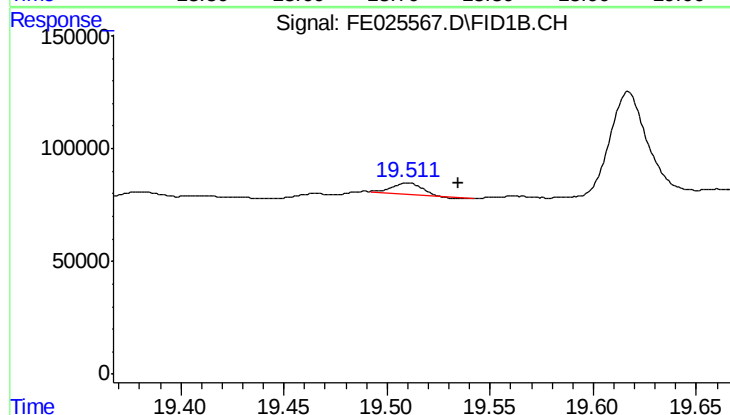


#15 N-TETRATRIACONTANE

R.T.: 19.510 min
Delta R.T.: -0.025 min
Response: 44118
Conc: 0.28 ug/ml

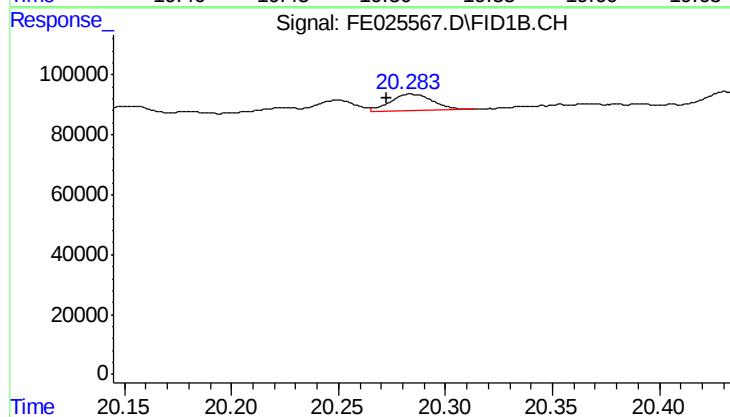

#16 N-HEXATRIACONTANE

R.T.: 20.284 min
Delta R.T.: 0.012 min
Response: 77967
Conc: 0.59 ug/ml

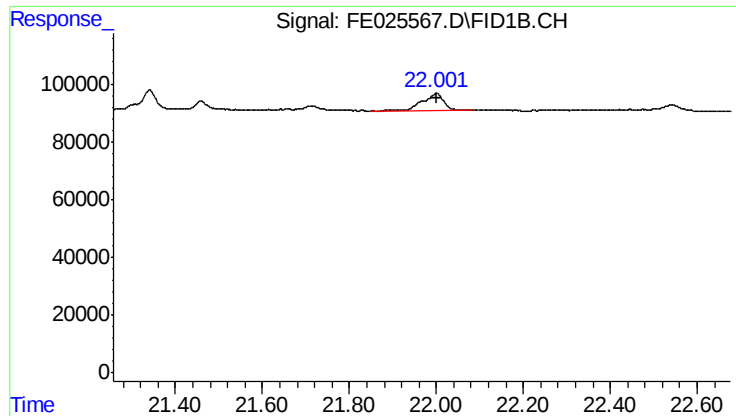

#18 N-TETRACONTANE

R.T.: 22.001 min
Delta R.T.: 0.000 min
Response: 204844
Conc: 1.60 ug/ml

Instrument :
FID_E
ClientSampleId :