

Data Path : P:\HPCHEM1\FID E\Data\FE011818\
 Data File : FE025692.D
 Signal(s) : FID1B.CH
 Acq On : 19 Jan 2018 1:01
 Operator : UA/AJ
 Sample : J1187-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 19 03:23:42 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Thu Jan 18 13:52:52 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.822	3325219	18.282 ug/ml
Target Compounds			
4) N-TETRADECANE	8.454	1307516	7.174 ug/ml
5) N-HEXADECANE	9.973	318919	1.561 ug/ml
8) N-DOCOSANE	13.919	225549	1.028 ug/ml
12) N-OCTACOSANE	16.989	272456	1.621 ug/ml
13) N-TRIACONTANE	17.875	232064	1.470 ug/ml
14) N-DOTRIACONTANE	18.704	173856	1.072 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE011818\
Data File : FE025692.D
Signal(s) : FID1B.CH
Acq On : 19 Jan 2018 1:01
Operator : UA/AJ
Sample : J1187-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 19 03:23:42 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Thu Jan 18 13:52:52 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

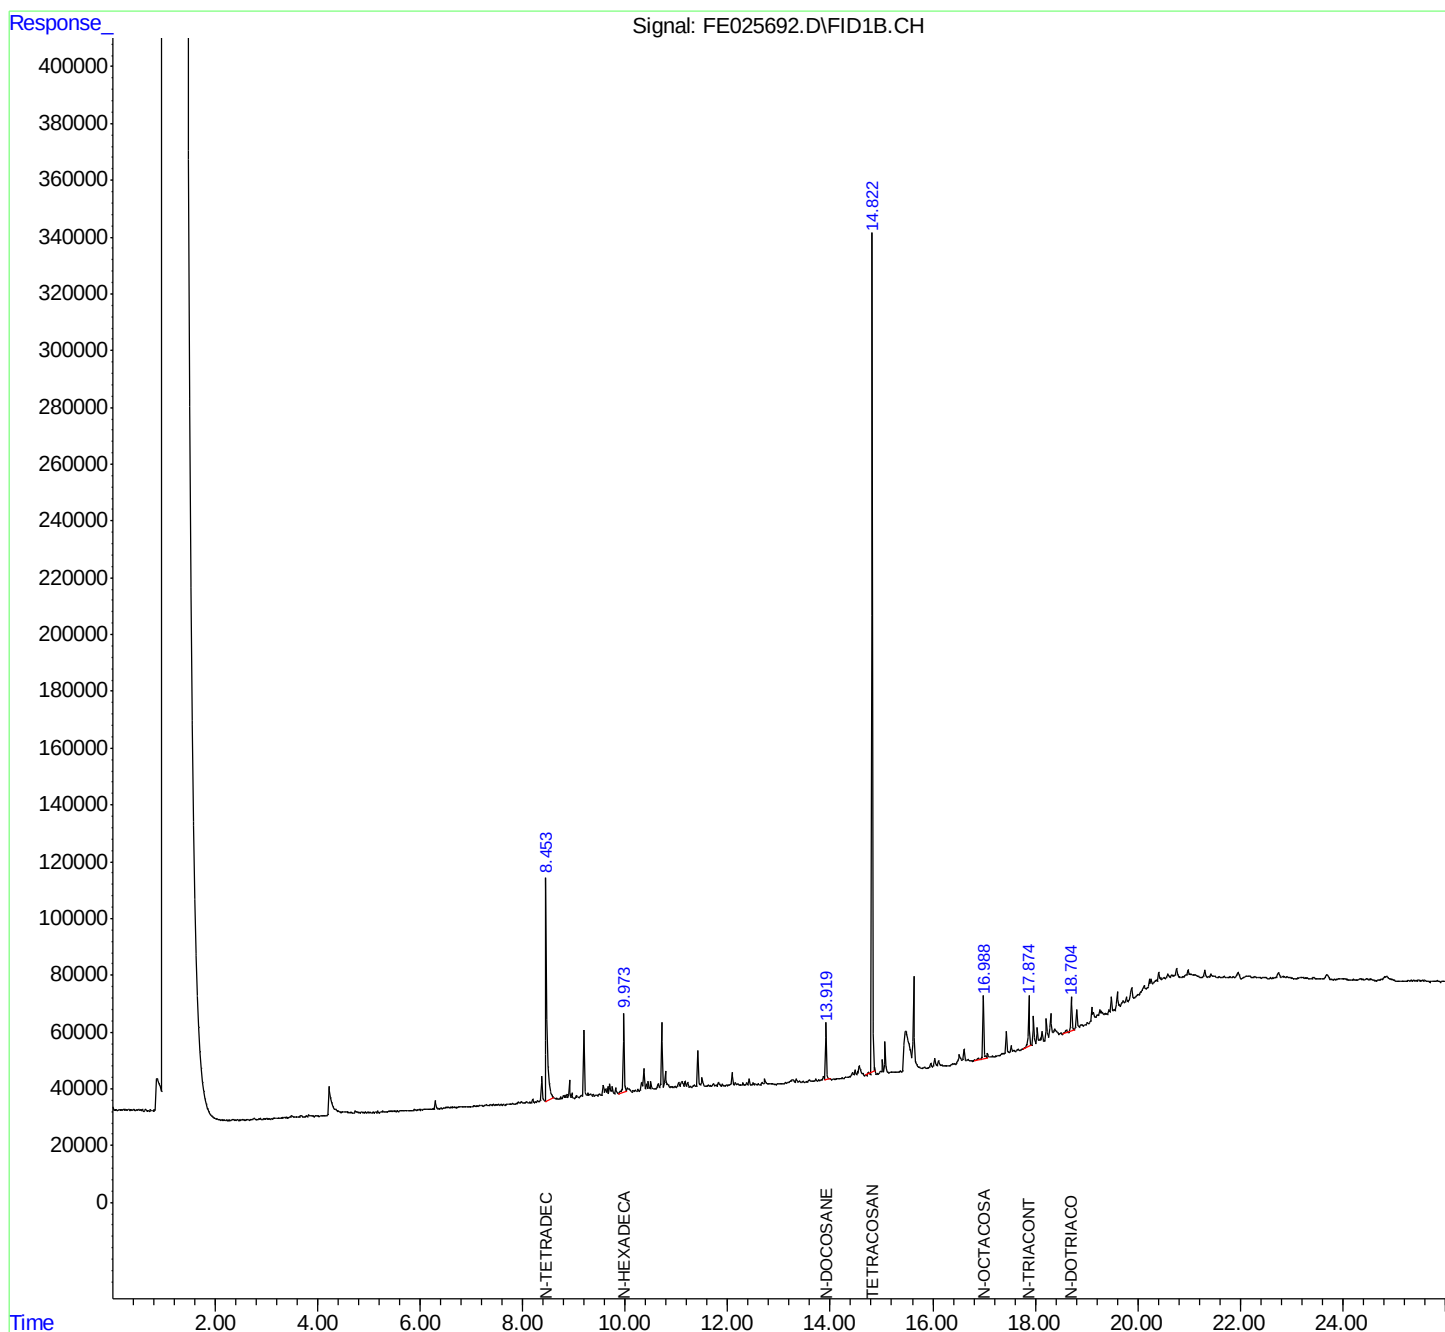


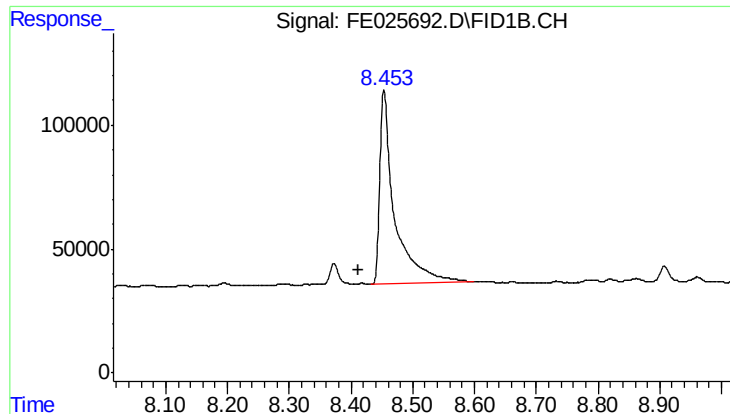

#4 N-TETRADECANE


R.T.: 8.454 min
Delta R.T.: 0.042 min
Response: 1307516
Conc: 7.17 ug/ml

Instrument :
FID_E
ClientSampleId :

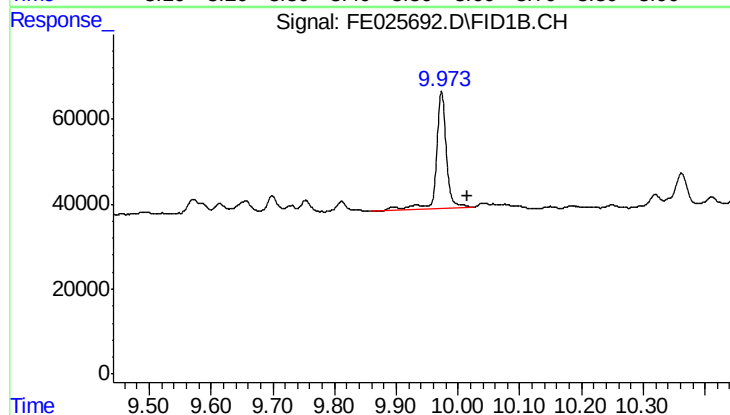


#5 N-HEXADECANE

R.T.: 9.973 min
Delta R.T.: -0.041 min
Response: 318919
Conc: 1.56 ug/ml

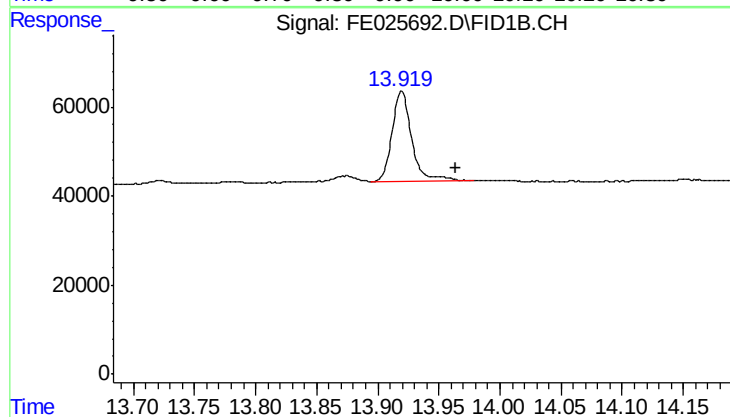


#8 N-DOCOSANE

R.T.: 13.919 min
Delta R.T.: -0.045 min
Response: 225549
Conc: 1.03 ug/ml

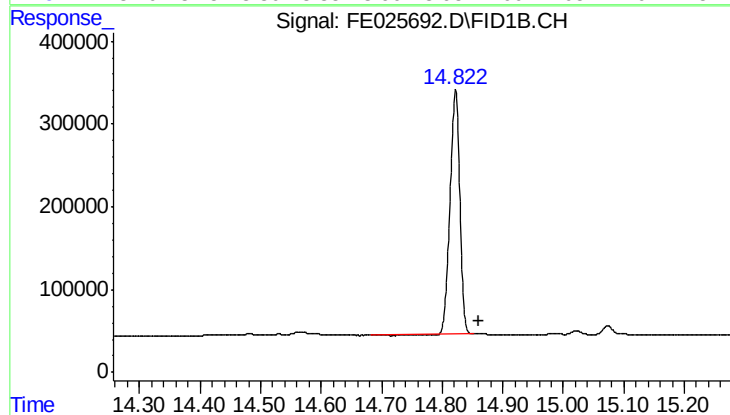

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.822 min
Delta R.T.: -0.039 min
Response: 3325219
Conc: 18.28 ug/ml

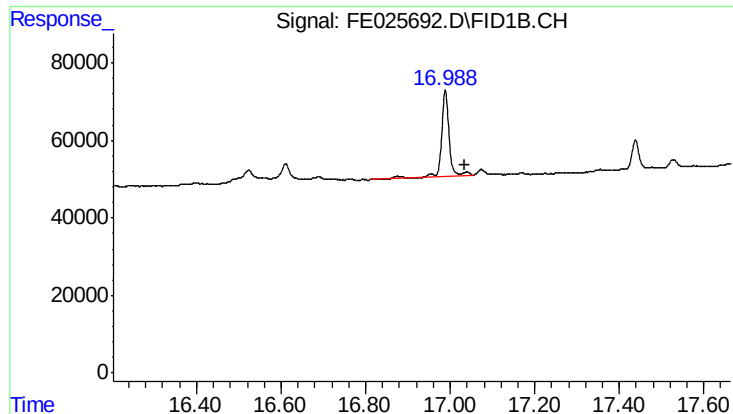

#12 N-OCTACOSANE


R.T.: 16.989 min
Delta R.T.: -0.045 min
Response: 272456
Conc: 1.62 ug/ml

Instrument :
FID_E
ClientSampleId :

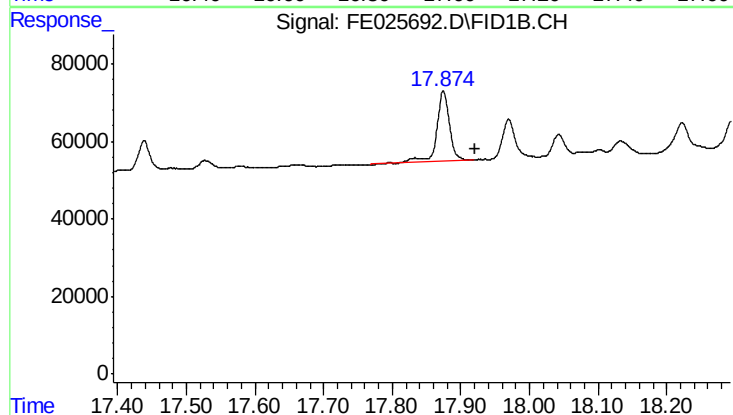

#13 N-TRIACONTANE

R.T.: 17.875 min
Delta R.T.: -0.046 min
Response: 232064
Conc: 1.47 ug/ml

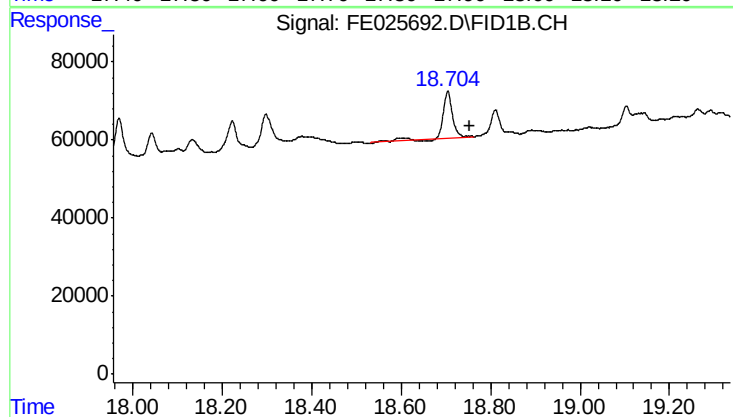

#14 N-DOTRIACONTANE

R.T.: 18.704 min
Delta R.T.: -0.048 min
Response: 173856
Conc: 1.07 ug/ml