

Data Path : P:\HPCHEM1\FID E\Data\FE011818\
 Data File : FE025694.D
 Signal(s) : FID1B.CH
 Acq On : 19 Jan 2018 2:11
 Operator : UA/AJ
 Sample : J1010-06 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 19 03:24:18 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Thu Jan 18 13:52:52 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.818	285567	1.570 ug/ml
Target Compounds			
4) N-TETRADECANE	8.372	256529	1.408 ug/ml
7) N-EICOSANE	12.779	238659	1.076 ug/ml
8) N-DOCOSANE	13.973	1501600	6.845 ug/ml
10) N-TETRACOSANE	15.082	256796	1.204 ug/ml
13) N-TRIACONTANE	17.878	277276	1.756 ug/ml
14) N-DOTRIACONTANE	18.708	274278	1.691 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE011818\
Data File : FE025694.D
Signal(s) : FID1B.CH
Acq On : 19 Jan 2018 2:11
Operator : UA/AJ
Sample : J1010-06 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 19 03:24:18 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Thu Jan 18 13:52:52 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

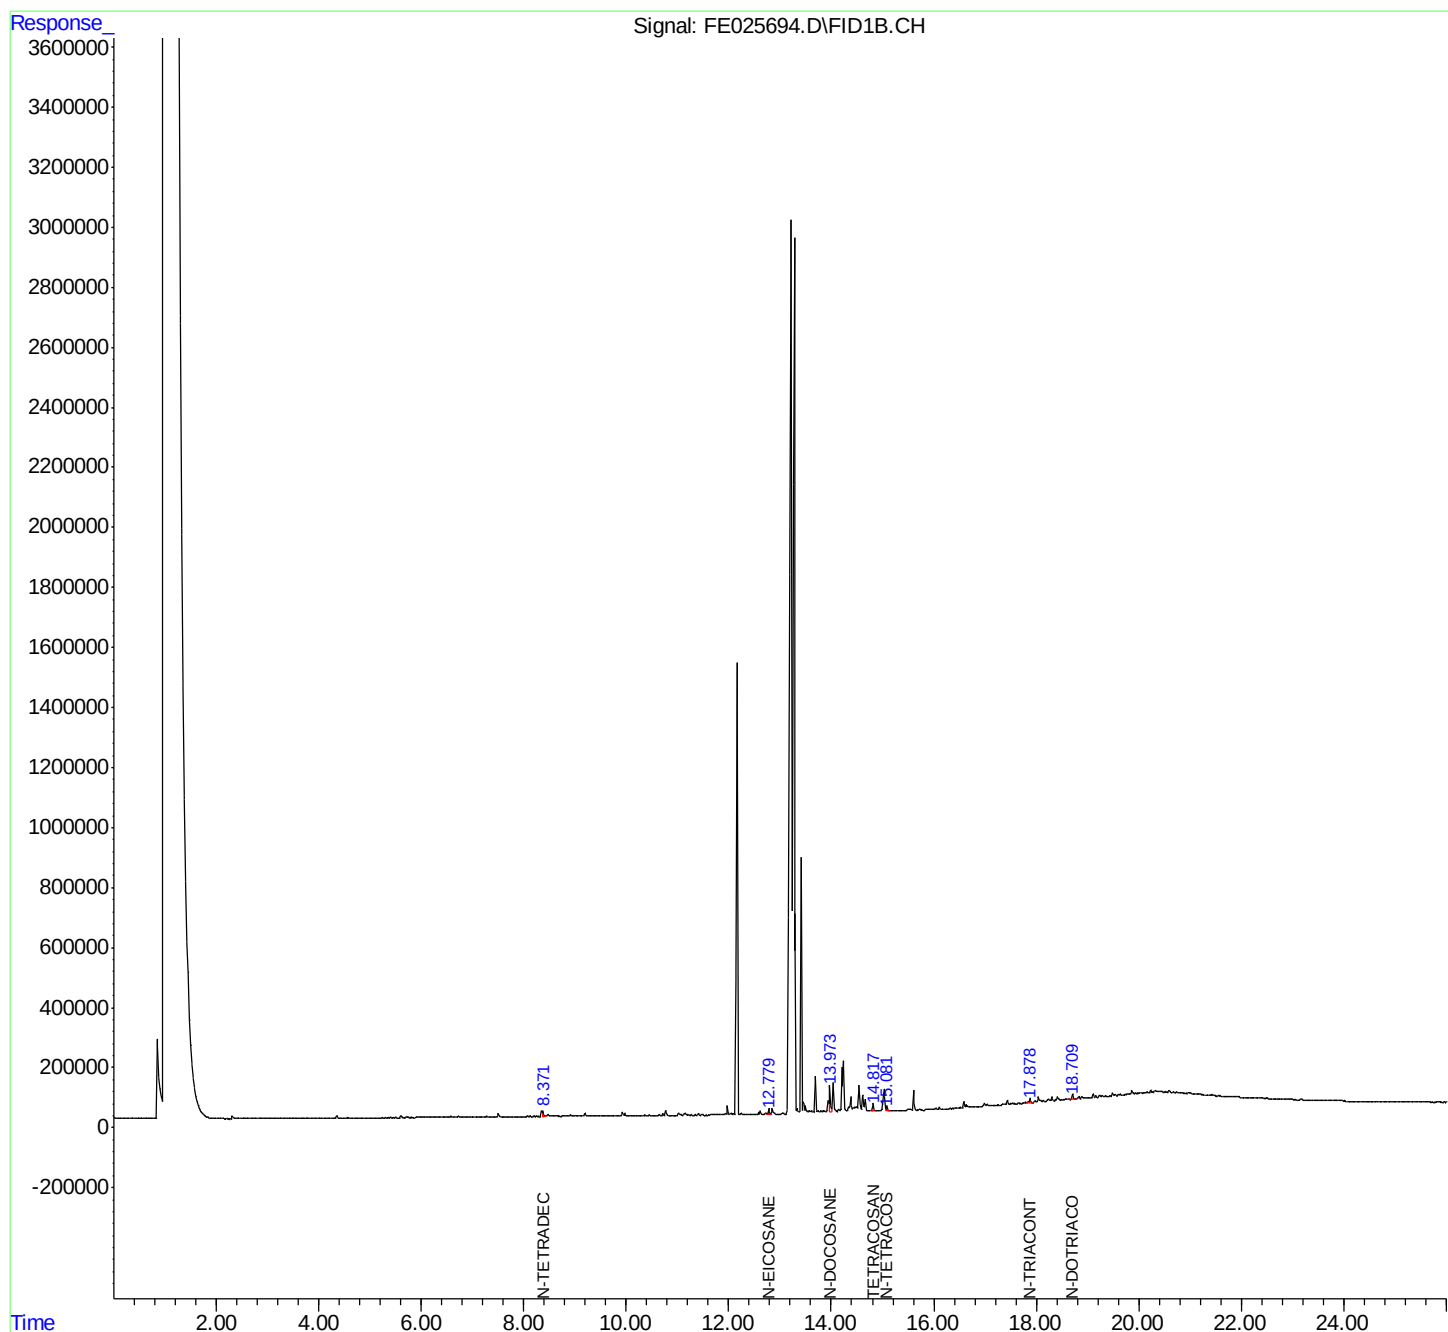


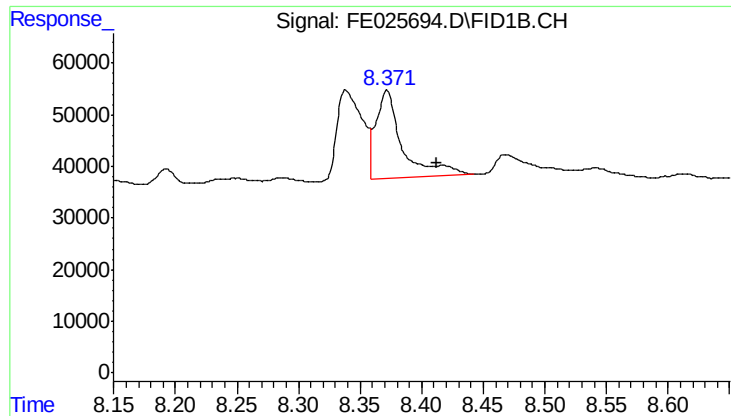

#4 N-TETRADECANE


R.T.: 8.372 min
Delta R.T.: -0.040 min
Response: 256529
Conc: 1.41 ug/ml

Instrument :
FID_E
ClientSampleId :

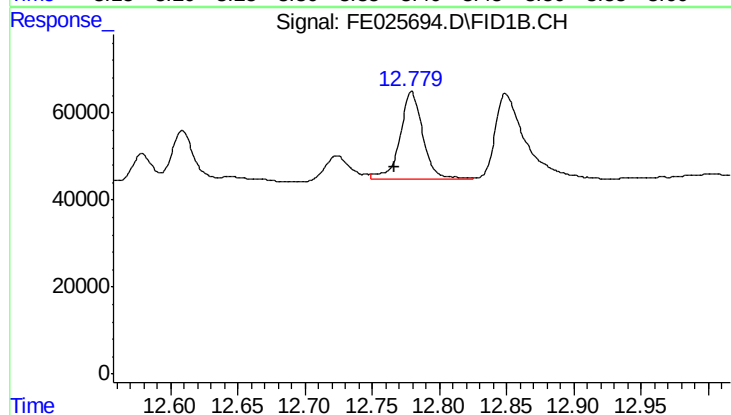


#7 N-EICOSANE

R.T.: 12.779 min
Delta R.T.: 0.013 min
Response: 238659
Conc: 1.08 ug/ml

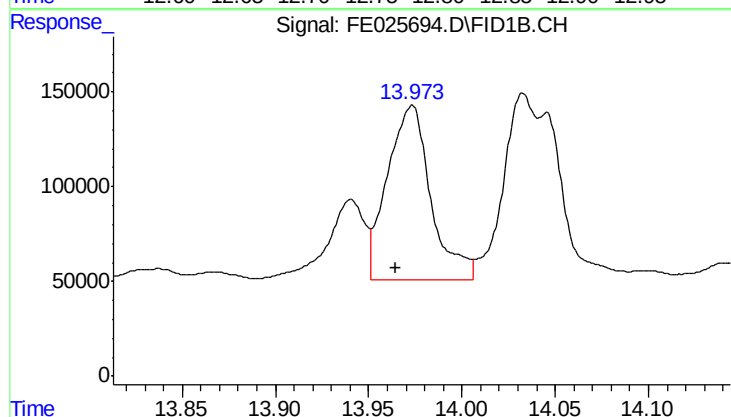


#8 N-DOCOSANE

R.T.: 13.973 min
Delta R.T.: 0.008 min
Response: 1501600
Conc: 6.84 ug/ml

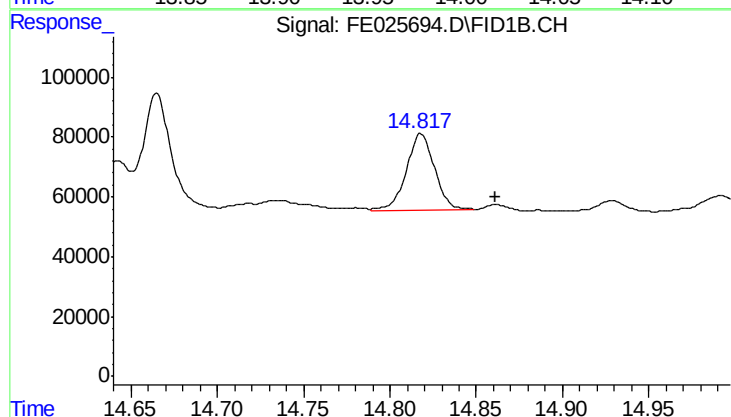

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.818 min
Delta R.T.: -0.043 min
Response: 285567
Conc: 1.57 ug/ml

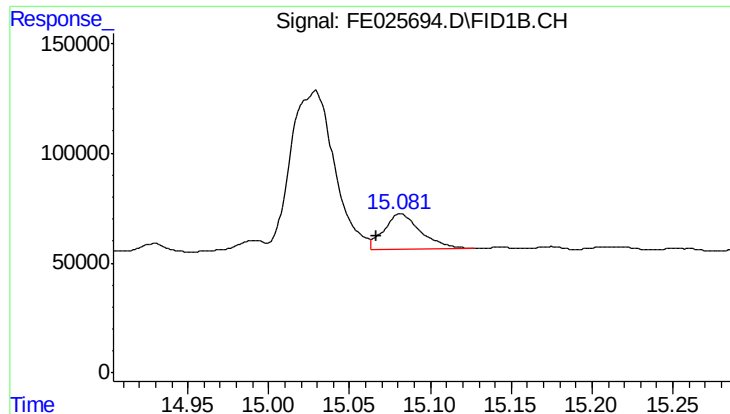

#10 N-TETRACOSANE


R.T.: 15.082 min
Delta R.T.: 0.015 min
Response: 256796
Conc: 1.20 ug/ml

Instrument :
FID_E
ClientSampleId :

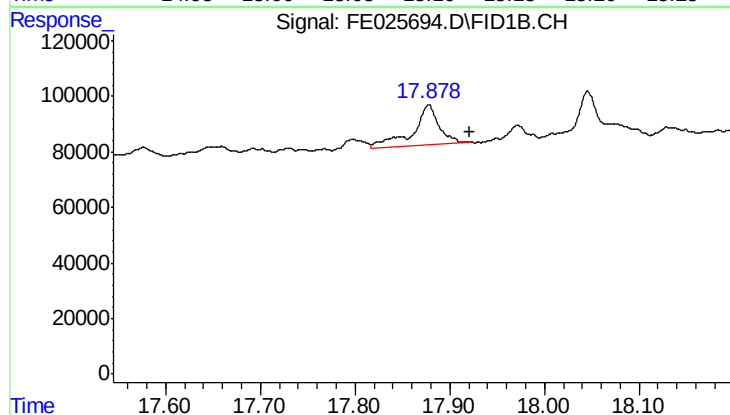

#13 N-TRIACONTANE

R.T.: 17.878 min
Delta R.T.: -0.043 min
Response: 277276
Conc: 1.76 ug/ml

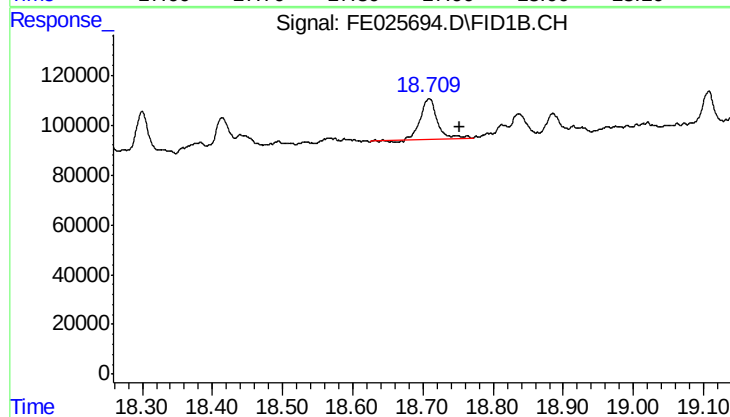

#14 N-DOTRIACONTANE

R.T.: 18.708 min
Delta R.T.: -0.044 min
Response: 274278
Conc: 1.69 ug/ml