

Data Path : P:\HPCHEM1\FID E\Data\FE011818\
 Data File : FE025701.D
 Signal(s) : FID1B.CH
 Acq On : 19 Jan 2018 7:57
 Operator : UA/AJ
 Sample : J1187-09 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 19 08:42:32 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Thu Jan 18 13:52:52 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.901	322572	1.773 ug/ml
Target Compounds			
7) N-EICOSANE	12.706f	548539	2.474 ug/ml
8) N-DOCOSANE	14.006	358933	1.636 ug/ml
10) N-TETRACOSANE	15.073	3695051	17.326 ug/ml
11) N-HEXACOSANE	16.142f	268781	1.395 ug/ml
12) N-OCTACOSANE	16.997	2890073	17.190 ug/ml
13) N-TRIACONTANE	17.880	214292	1.357 ug/ml
14) N-DOTRIACONTANE	18.715	359717	2.218 ug/ml
15) N-TETRATRIACONTANE	19.536	99286	0.639 ug/ml
16) N-HEXATRIACONTANE	20.299	428495	3.224 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE011818\
Data File : FE025701.D
Signal(s) : FID1B.CH
Acq On : 19 Jan 2018 7:57
Operator : UA/AJ
Sample : J1187-09 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 19 08:42:32 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Thu Jan 18 13:52:52 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

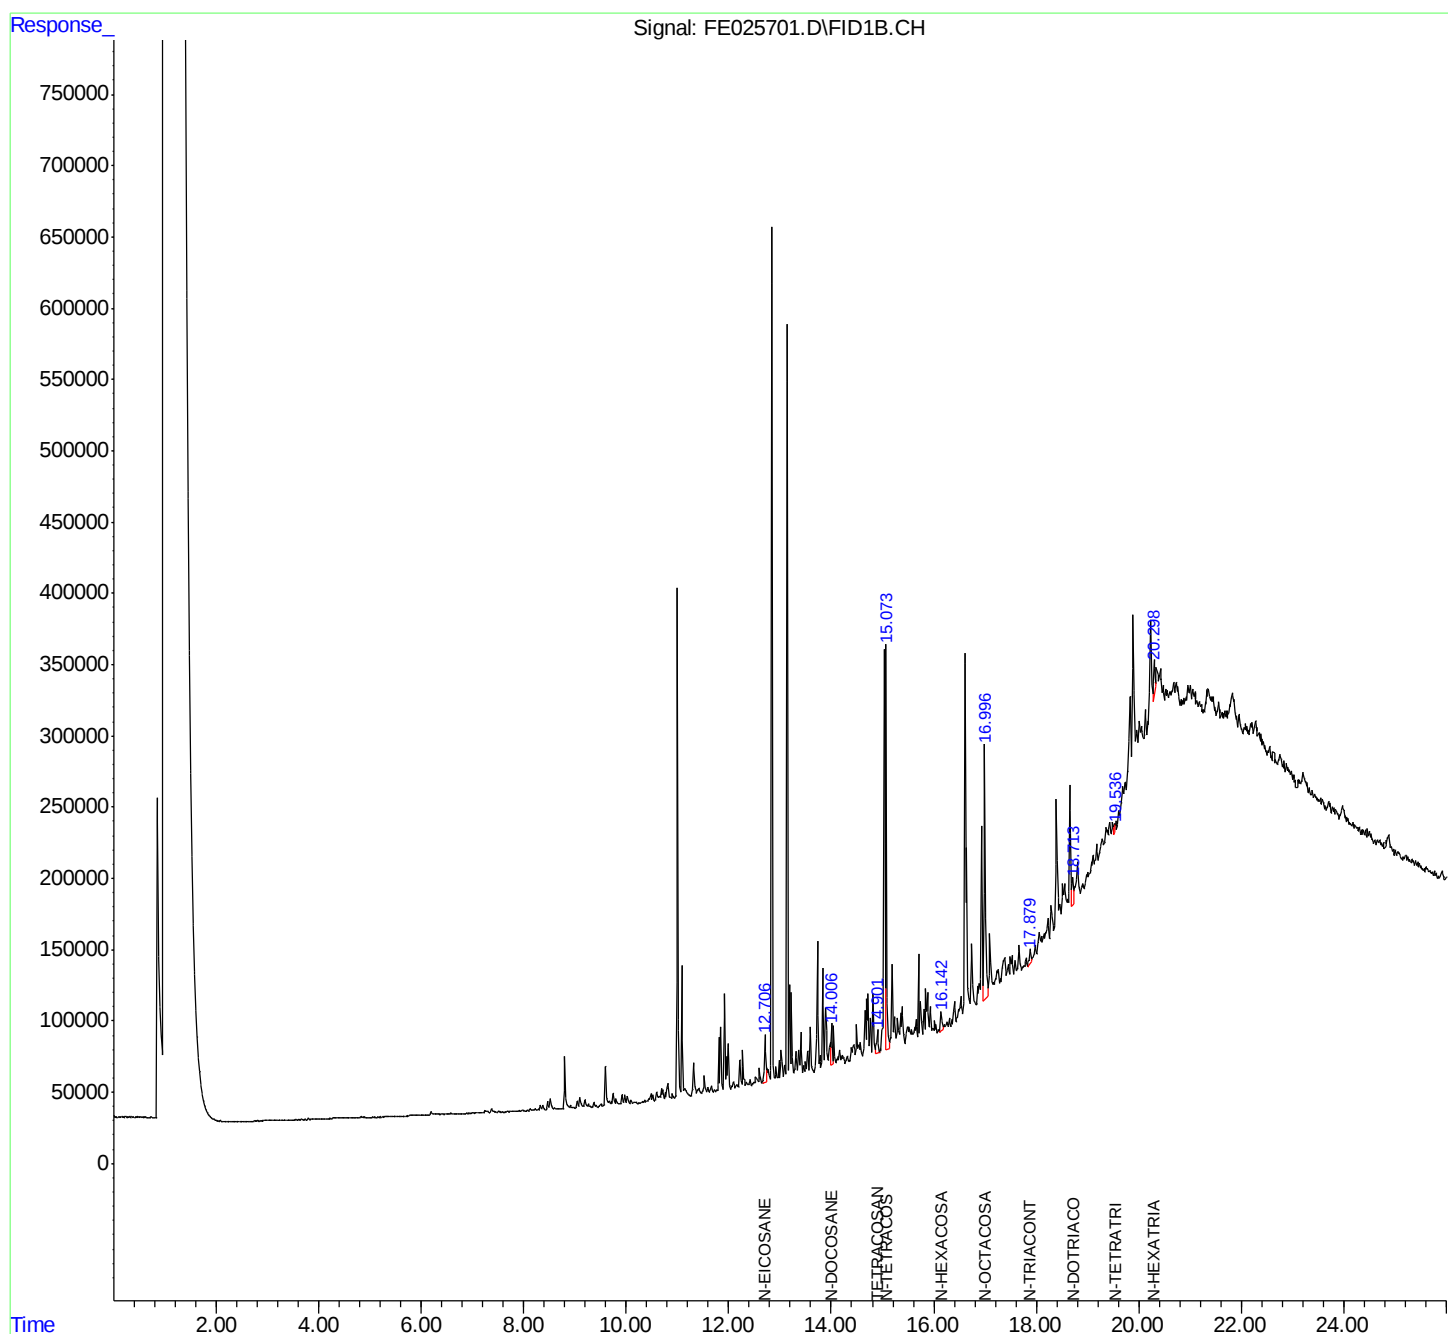


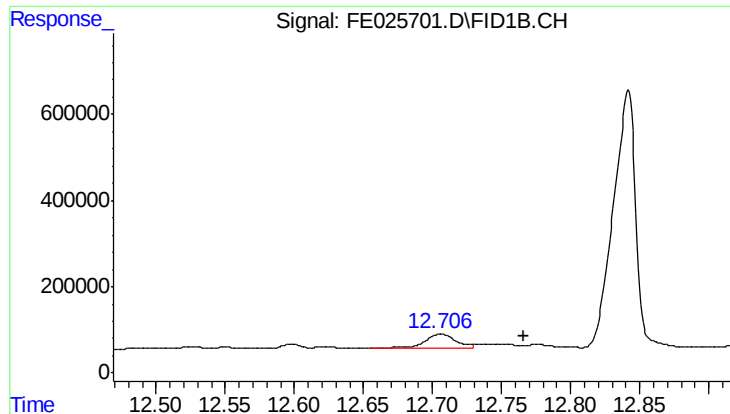

#7 N-EICOSANE


R.T.: 12.706 min
Delta R.T.: -0.060 min
Response: 548539
Conc: 2.47 ug/ml

Instrument :
FID_E
ClientSampleId :

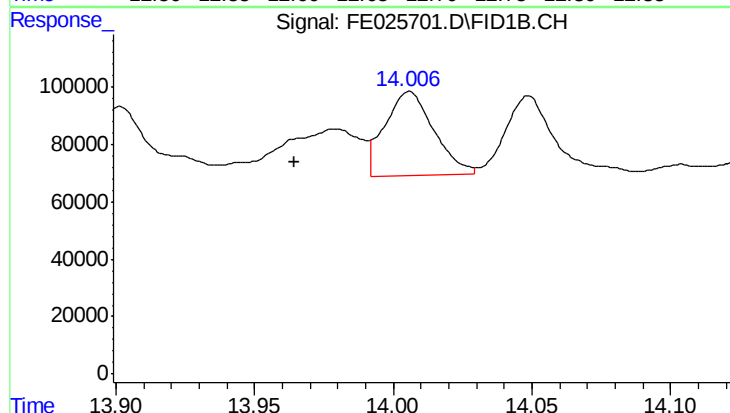


#8 N-DOCOSANE

R.T.: 14.006 min
Delta R.T.: 0.041 min
Response: 358933
Conc: 1.64 ug/ml

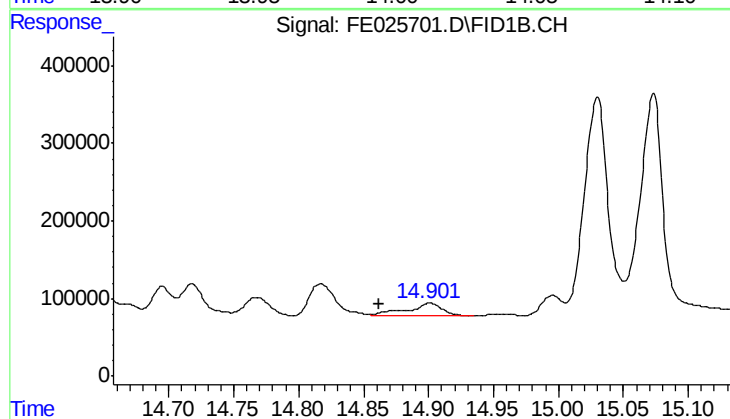


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.901 min
Delta R.T.: 0.040 min
Response: 322572
Conc: 1.77 ug/ml

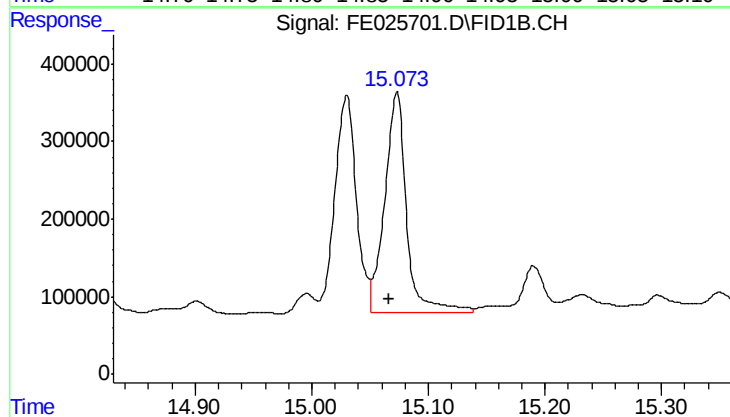

#10 N-TETRACOSANE


R.T.: 15.073 min
Delta R.T.: 0.006 min
Response: 3695051
Conc: 17.33 ug/ml

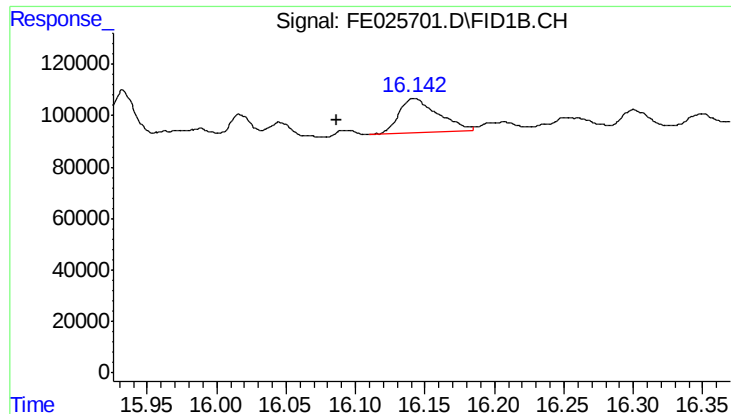

#11 N-HEXACOSANE


R.T.: 16.142 min
Delta R.T.: 0.056 min
Response: 268781
Conc: 1.39 ug/ml

Instrument :
FID_E
ClientSampleId :

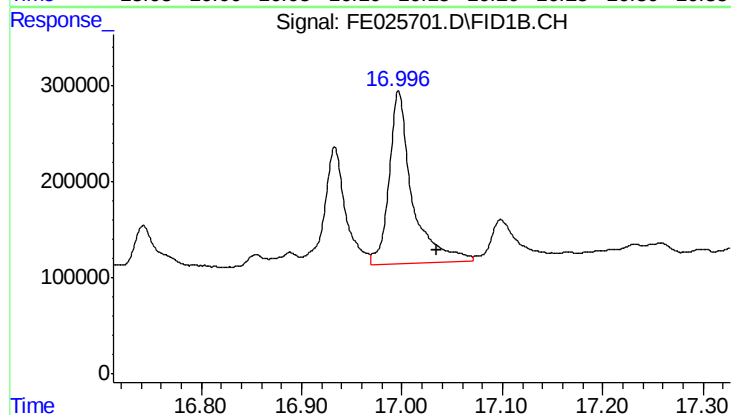


#12 N-OCTACOSANE

R.T.: 16.997 min
Delta R.T.: -0.037 min
Response: 2890073
Conc: 17.19 ug/ml

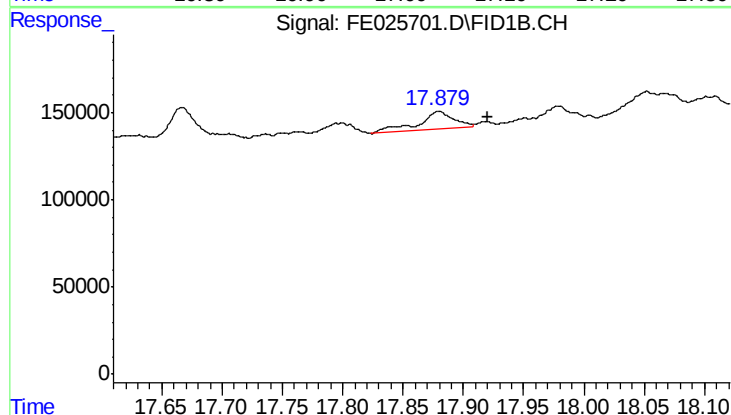


#13 N-TRIACONTANE

R.T.: 17.880 min
Delta R.T.: -0.041 min
Response: 214292
Conc: 1.36 ug/ml

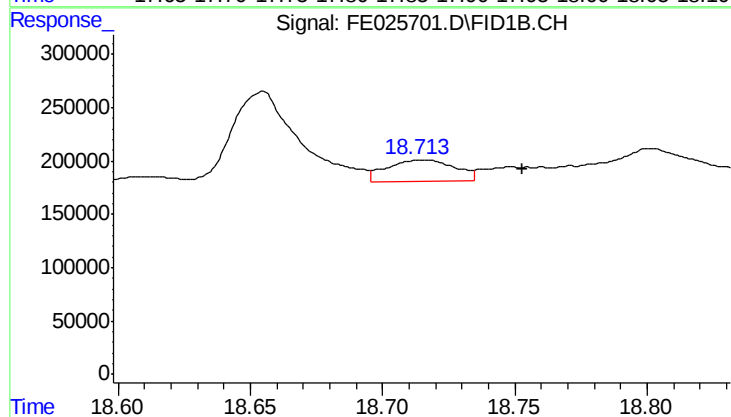

#14 N-DOTRIACONTANE


R.T.: 18.715 min
Delta R.T.: -0.037 min
Response: 359717
Conc: 2.22 ug/ml

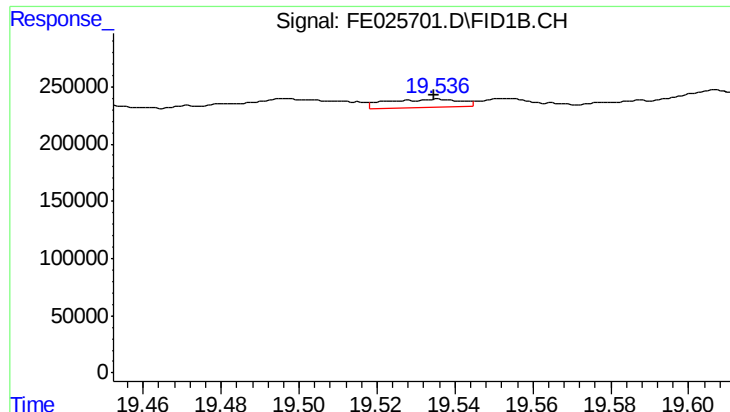

#15 N-TETRATRIACONTANE

R.T.: 19.536 min
Delta R.T.: 0.001 min
Response: 99286
Conc: 0.64 ug/ml

Instrument :
FID_E
ClientSampleId :

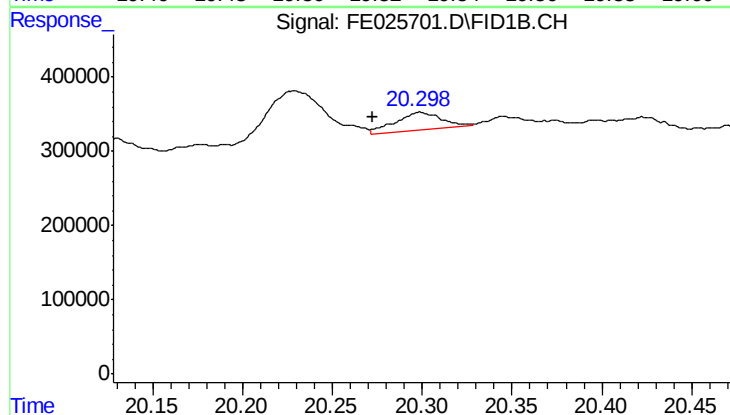

#16 N-HEXATRIACONTANE

R.T.: 20.299 min
Delta R.T.: 0.027 min
Response: 428495
Conc: 3.22 ug/ml