

Data Path : P:\HPCHEM1\FID_E\Data\FE012518\
 Data File : FE025800.D
 Signal(s) : FID1B.CH
 Acq On : 25 Jan 2018 10:00
 Operator : UA/AJ
 Sample : J1258-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 25 11:47:15 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\C44-FE010418.M
 Quant Title :
 QLast Update : Thu Jan 25 11:46:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
6)	N-TETRADECANE	8.442	954513	6.516 ug/ml
7)	N-HEXADECANE	10.064	317397	2.063 ug/ml
8)	N-OCTADECANE	11.492	2462137	15.618 ug/ml
10)	N-TETRACOSANE	15.055	279402	2.025 ug/ml
12)	N-DOTRIACONTANE	18.791	187871	1.564 ug/ml
16)	N-TETRTETRACOOCTANE	24.745	324301	5.887 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_E\Data\FE012518\
Data File : FE025800.D
Signal(s) : FID1B.CH
Acq On : 25 Jan 2018 10:00
Operator : UA/AJ
Sample : J1258-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 25 11:47:15 2018
Quant Method : P:\HPCHEM1\FID_E\methods\C44-FE010418.M
Quant Title :
QLast Update : Thu Jan 25 11:46:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

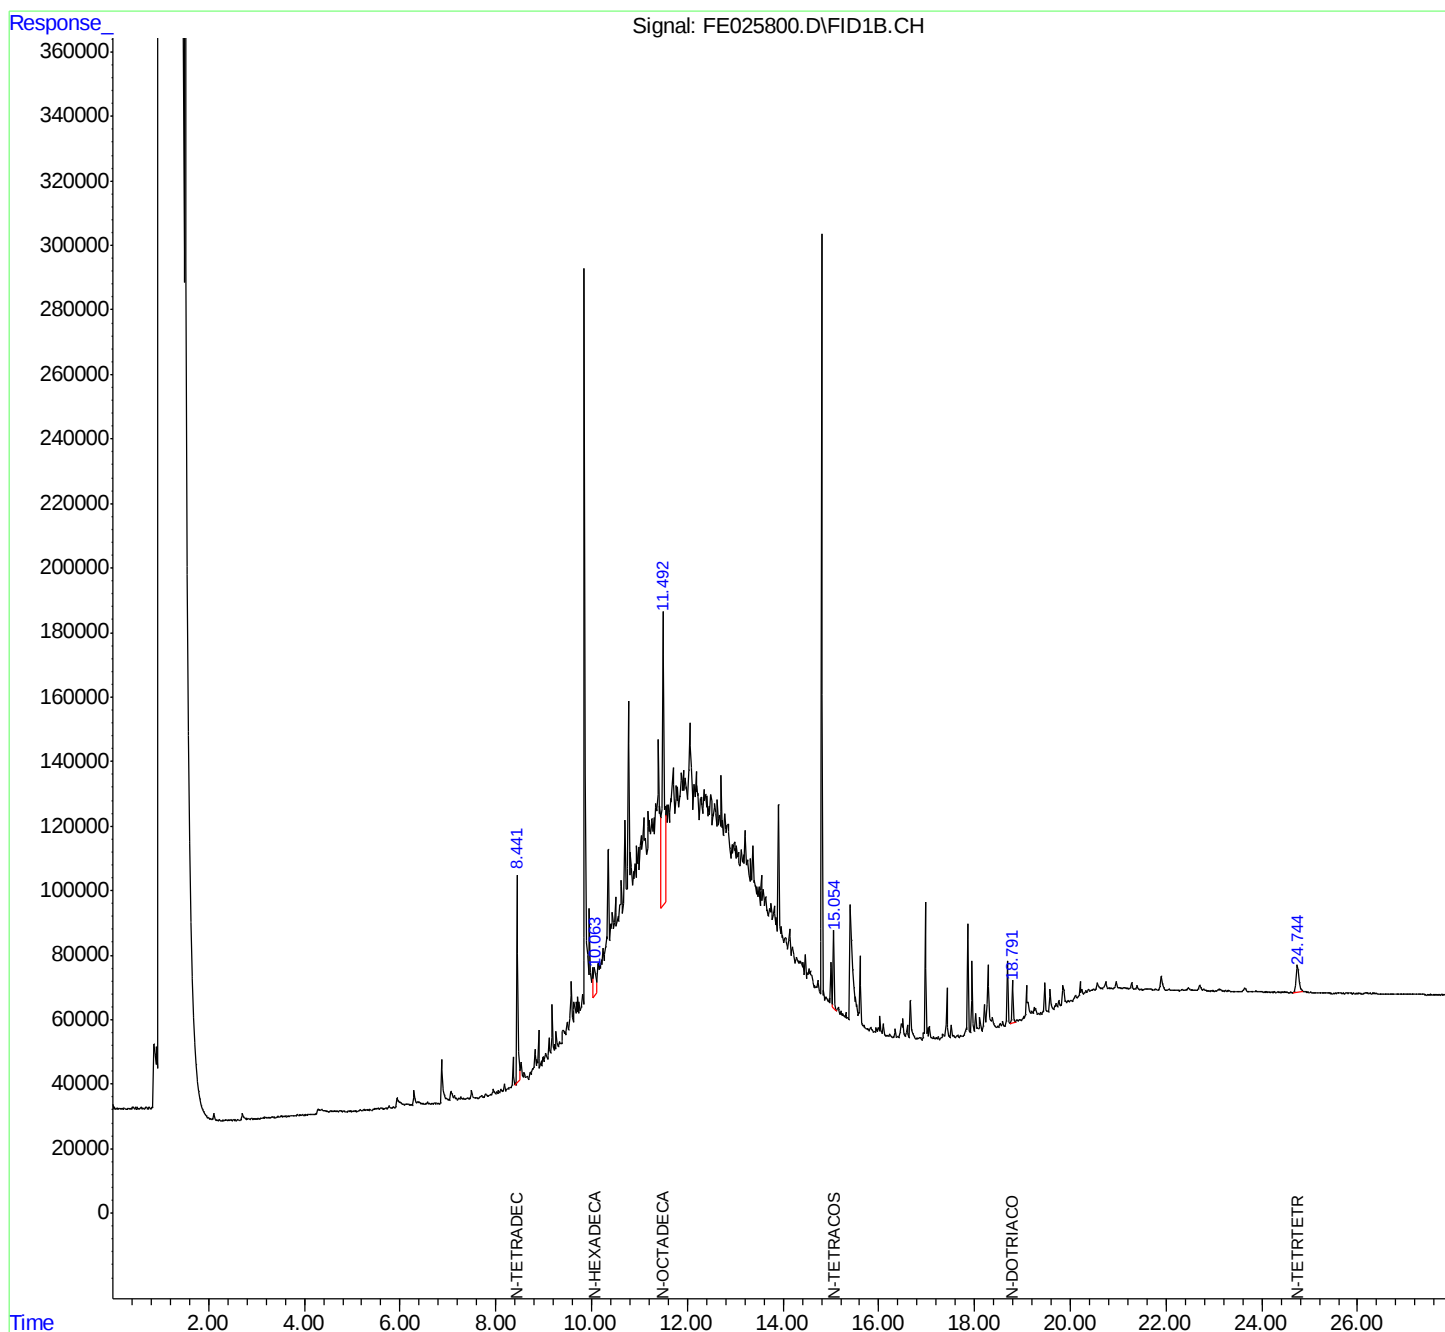

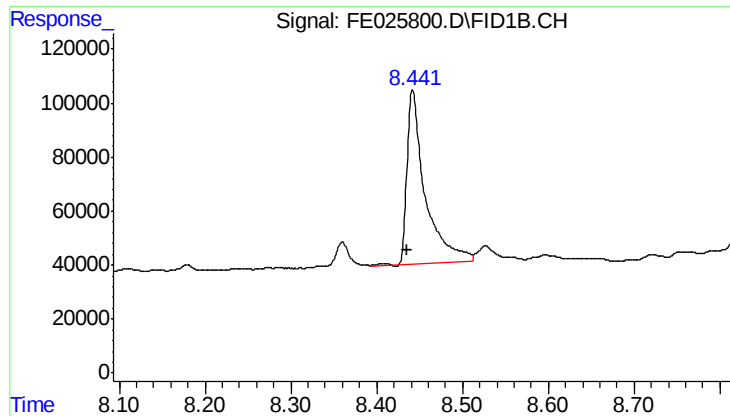


#6 N-TETRADECANE

R.T.: 8.442 min
Delta R.T.: 0.006 min
Response: 954513
Conc: 6.52 ug/ml

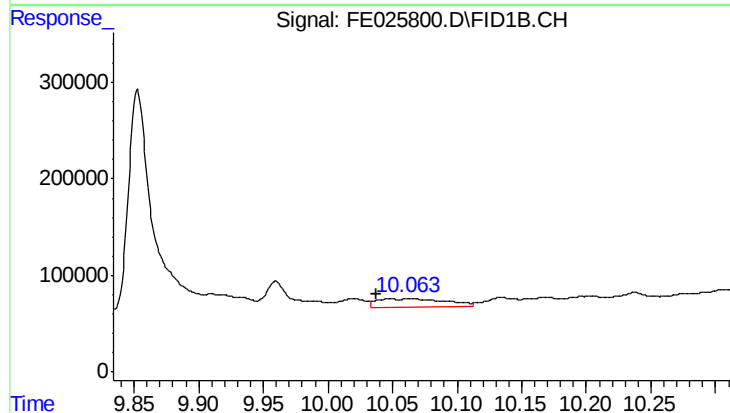


#7 N-HEXADECANE

R.T.: 10.064 min
Delta R.T.: 0.026 min
Response: 317397
Conc: 2.06 ug/ml

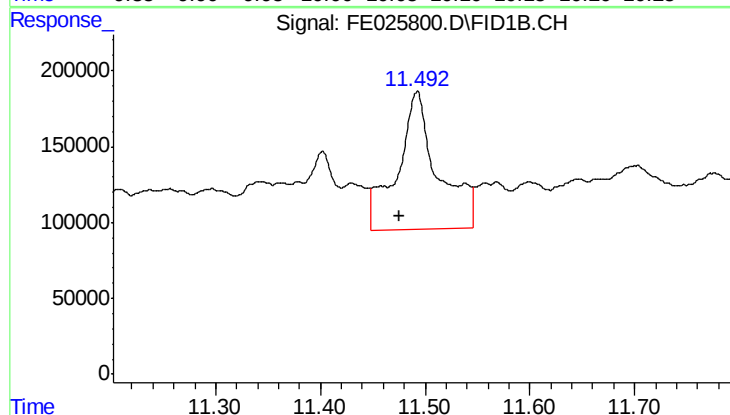


#8 N-OCTADECANE

R.T.: 11.492 min
Delta R.T.: 0.017 min
Response: 2462137
Conc: 15.62 ug/ml

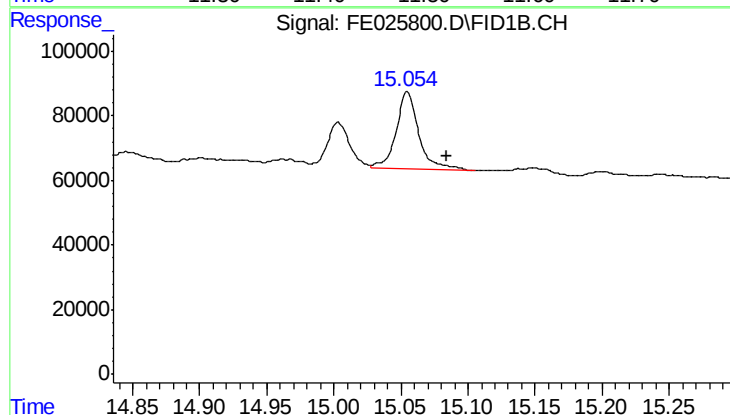


#10 N-TETRACOSANE

R.T.: 15.055 min
Delta R.T.: -0.030 min
Response: 279402
Conc: 2.03 ug/ml

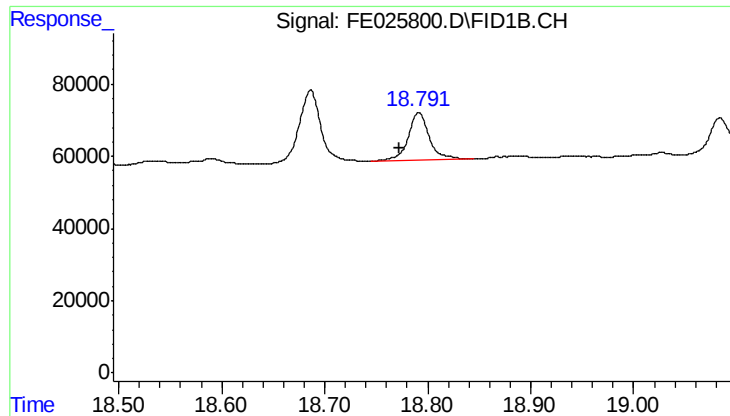


#12 N-DOTRIACONTANE

R.T.: 18.791 min
Delta R.T.: 0.019 min
Response: 187871
Conc: 1.56 ug/ml

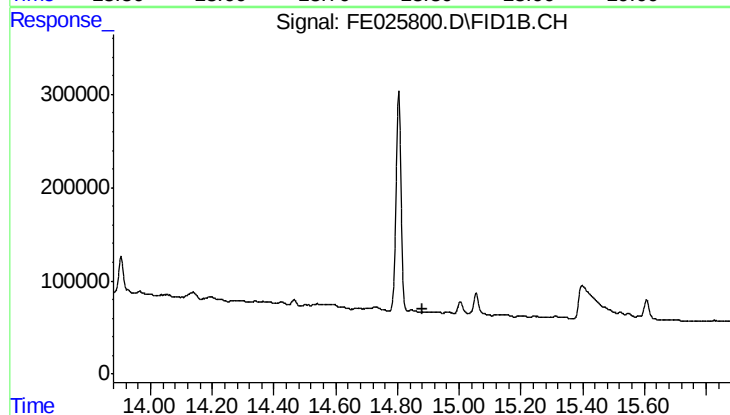

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.880 min
Response: 0
Conc: N.D.

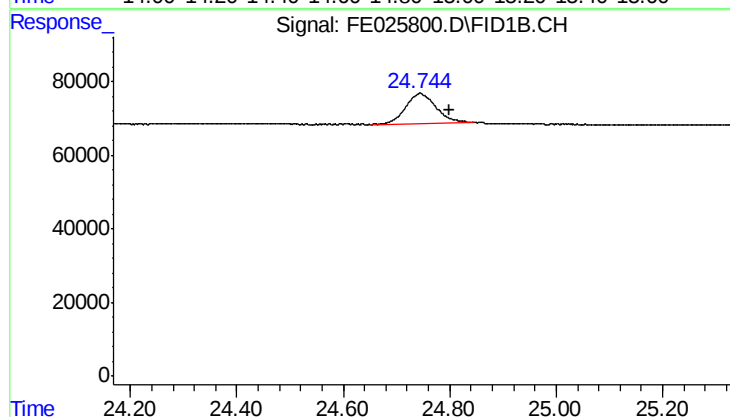

#16 N-TETRTETRACOOCTANE

R.T.: 24.745 min
Delta R.T.: -0.055 min
Response: 324301
Conc: 5.89 ug/ml